


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135597.D
Acq On : 05 Oct 2023 13:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 17:06:20 2023

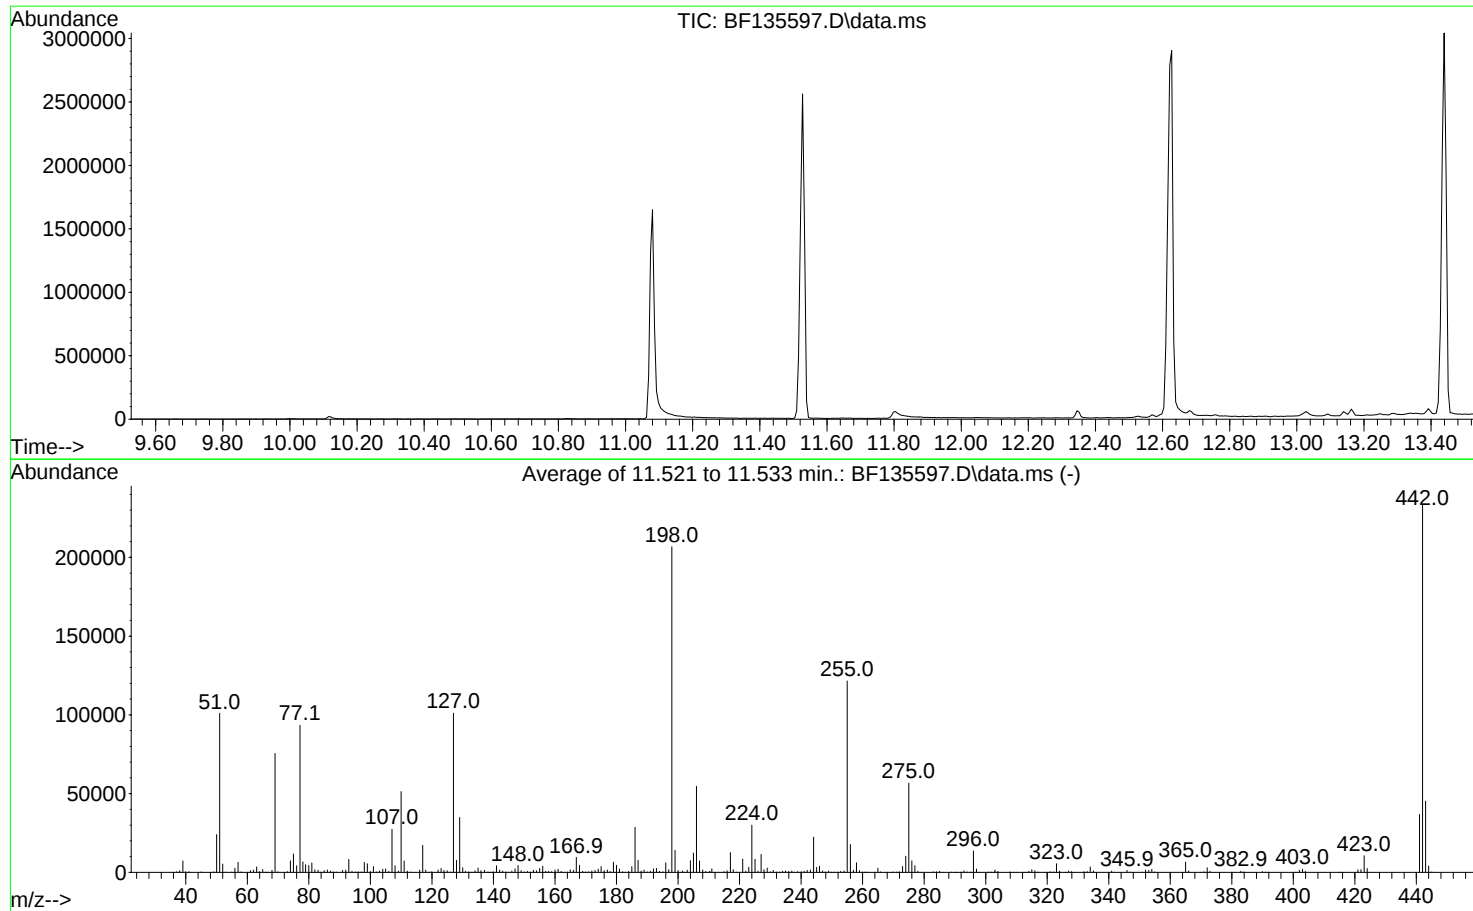




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	100960	PASS
68	69	0.00	2	1.7	1301	PASS
69	198	0.00	100	36.5	75536	PASS
70	69	0.00	2	0.6	451	PASS
127	198	10	80	48.9	101128	PASS
197	198	0.00	2	0.8	1690	PASS
198	198	100	100	100.0	206763	PASS
199	198	5	9	6.8	14062	PASS
275	198	10	60	27.4	56747	PASS
365	198	1	100	3.1	6466	PASS
441	198	0.01	100	17.8	36808	PASS
442	442	50	100	100.0	233584	PASS
443	442	15	24	19.4	45259	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135597.D
Acq On : 05 Oct 2023 13:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 06 08:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

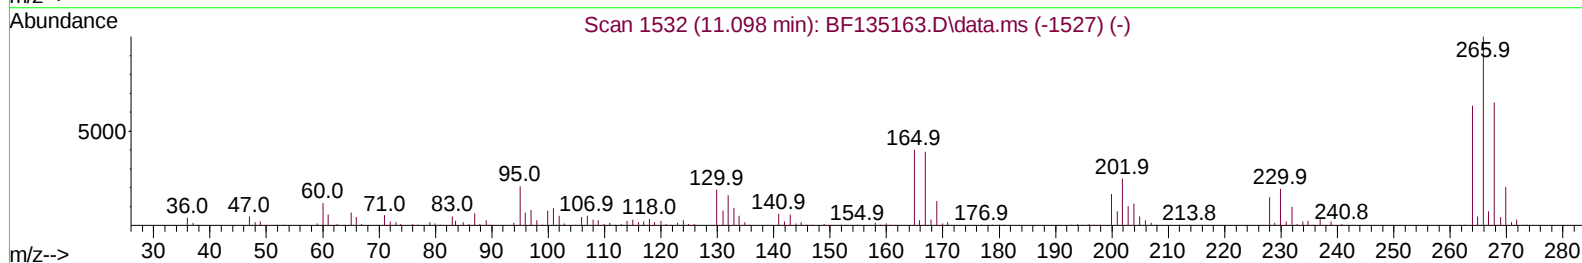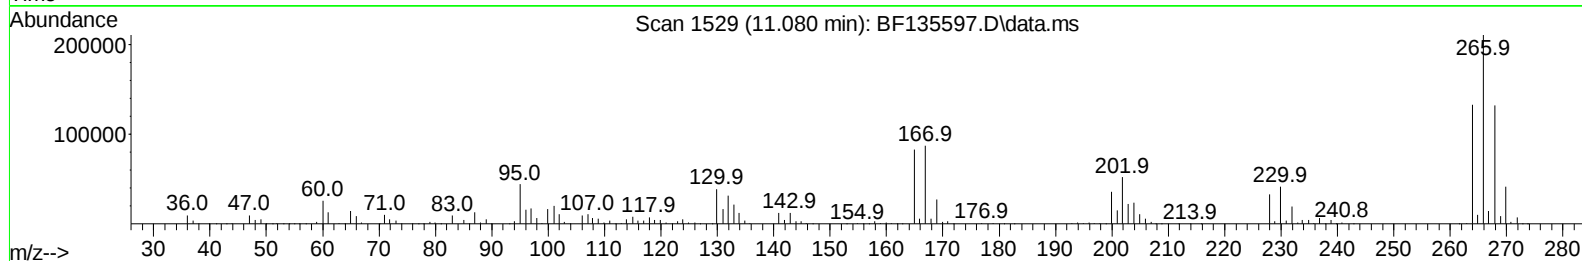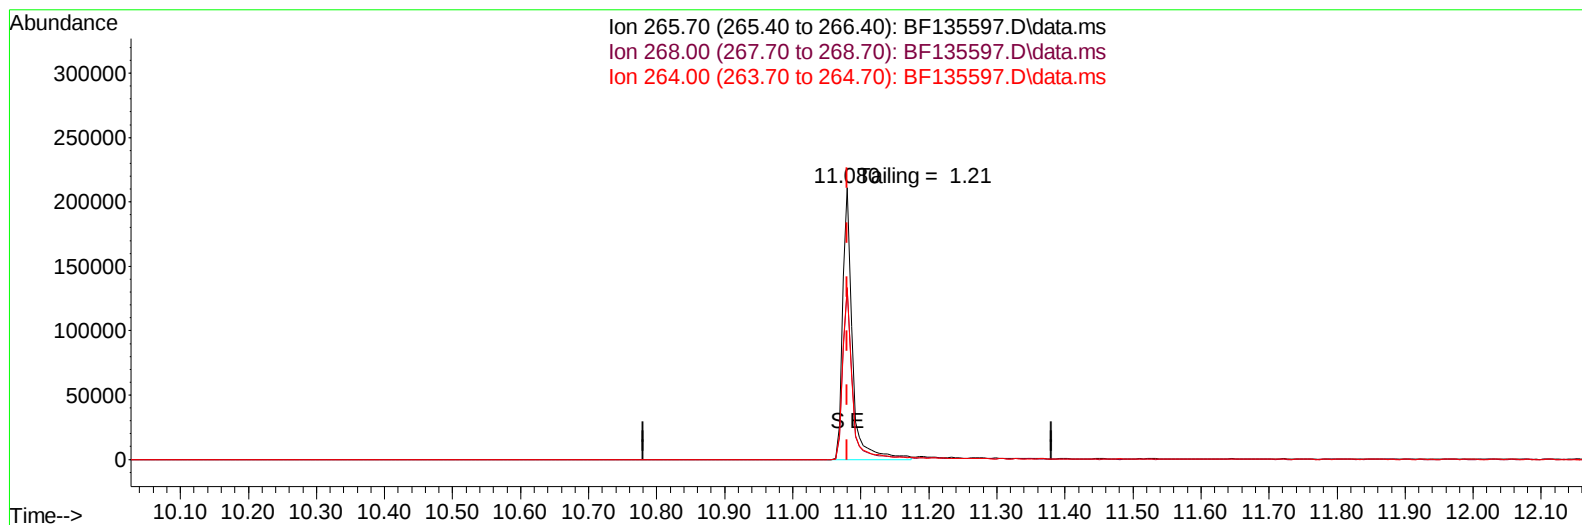

TIC: BF135597.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.000) 525857.35 ng




response 207211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.70
264.00	63.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135597.D
Acq On : 05 Oct 2023 13:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 06 08:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

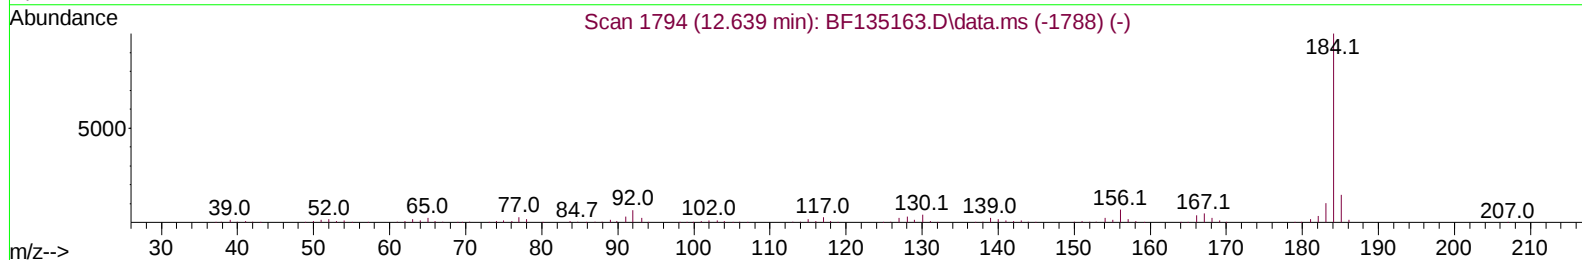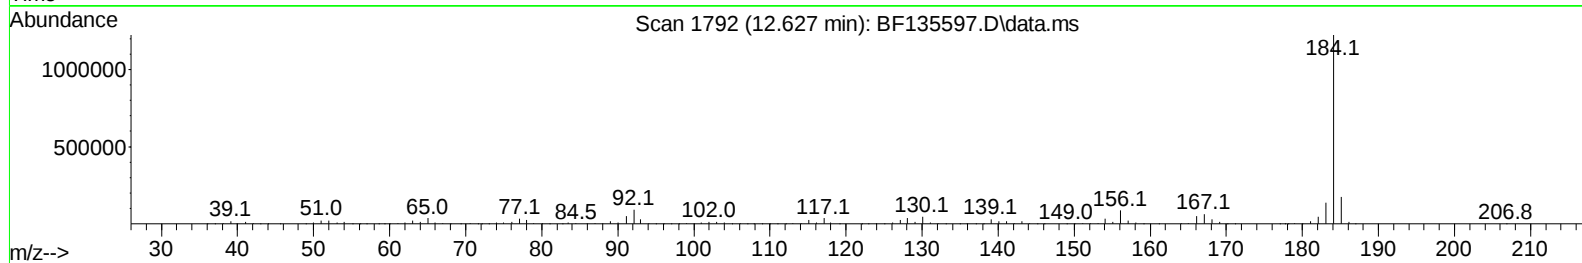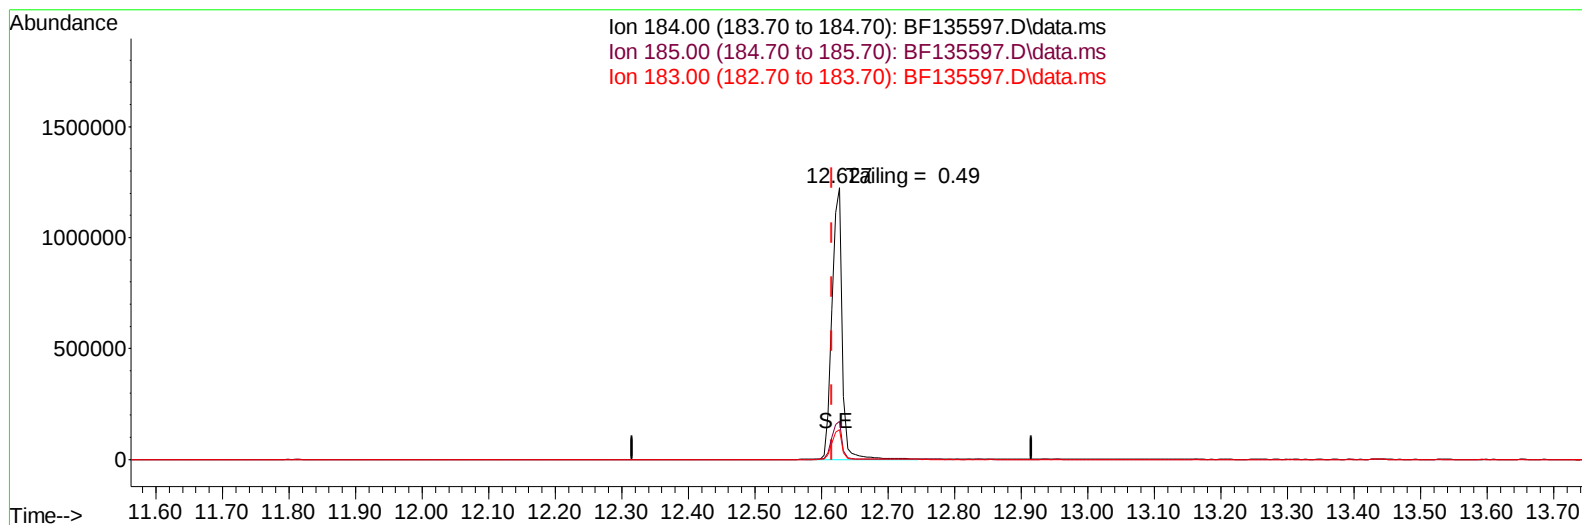

TIC: BF135597.D\data.ms

(77) Benzidine

12.627min (+ 0.012) 7798.62 ng m

response 1316177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.10
183.00	10.30	11.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2023	BNA_F	<u>BF135597.D</u>
Compound Name	Response	Retention Time
DDT	558995	13.439
DDD	14012	13.163
DDE	288	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14300	573295	2.49

Instrument :
BNA_F
ClientSampleId :
DFTPP