

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
 Data File : BF135633.D
 Acq On : 06 Oct 2023 17:21
 Operator : CG\JU
 Sample : 04622-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	485	489	500	rBV	102847	141011	3.35%	0.657%
2	5.375	555	559	578	rBV	1360948	1578336	37.47%	7.353%
3	6.387	728	731	751	rBV	838072	935841	22.22%	4.360%
4	6.740	787	791	799	rBV	731155	693494	16.46%	3.231%
5	7.310	883	888	891	rBV	2409193	2561002	60.80%	11.932%
6	8.016	1004	1008	1026	rBV	1066943	935274	22.20%	4.357%
7	8.245	1043	1047	1049	rBV	48147	54793	1.30%	0.255%
8	8.269	1049	1051	1063	rVB	67571	88741	2.11%	0.413%
9	9.098	1186	1192	1195	rBV	4380364	4212031	100.00%	19.624%
10	9.775	1303	1307	1320	rBV	1242278	1060874	25.19%	4.943%
11	10.575	1438	1443	1446	rBV	2533758	2482195	58.93%	11.565%
12	11.269	1557	1561	1569	rBV	1354049	1142843	27.13%	5.325%
13	12.869	1828	1833	1836	rBV	3999549	4062365	96.45%	18.927%
14	13.927	2010	2013	2024	rVB	901762	829571	19.70%	3.865%
15	15.398	2258	2263	2272	rBV	490033	685388	16.27%	3.193%




Sum of corrected areas: 21463759

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
Data File : BF135633.D
Acq On : 06 Oct 2023 17:21
Operator : CG\JU
Sample : 04622-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

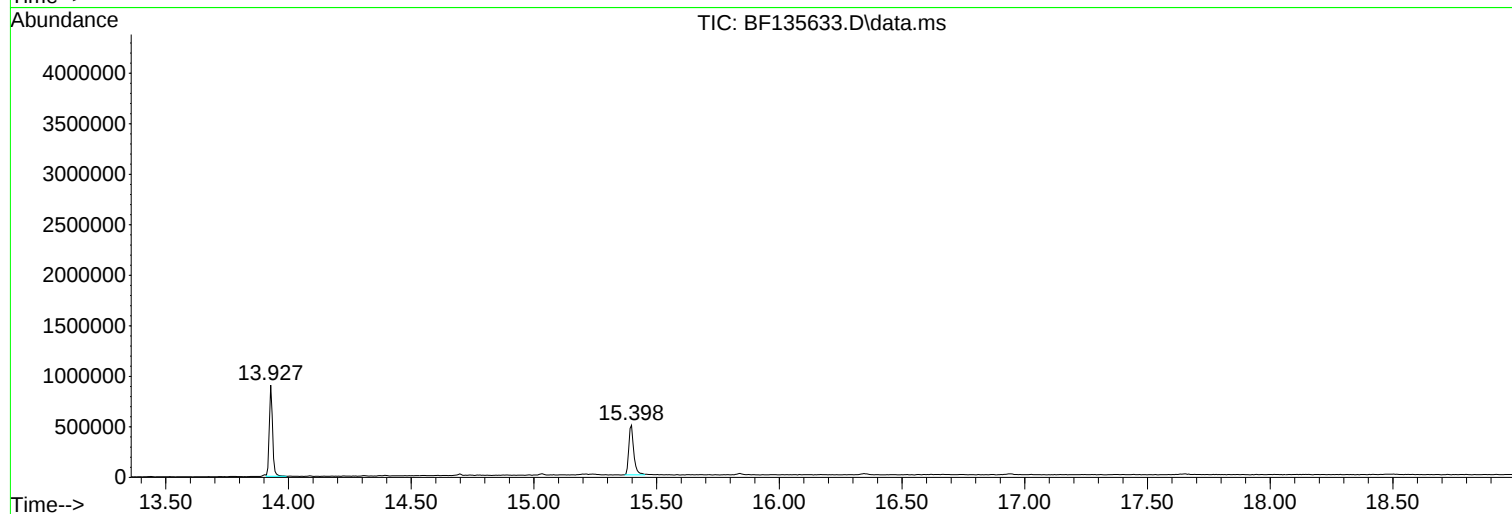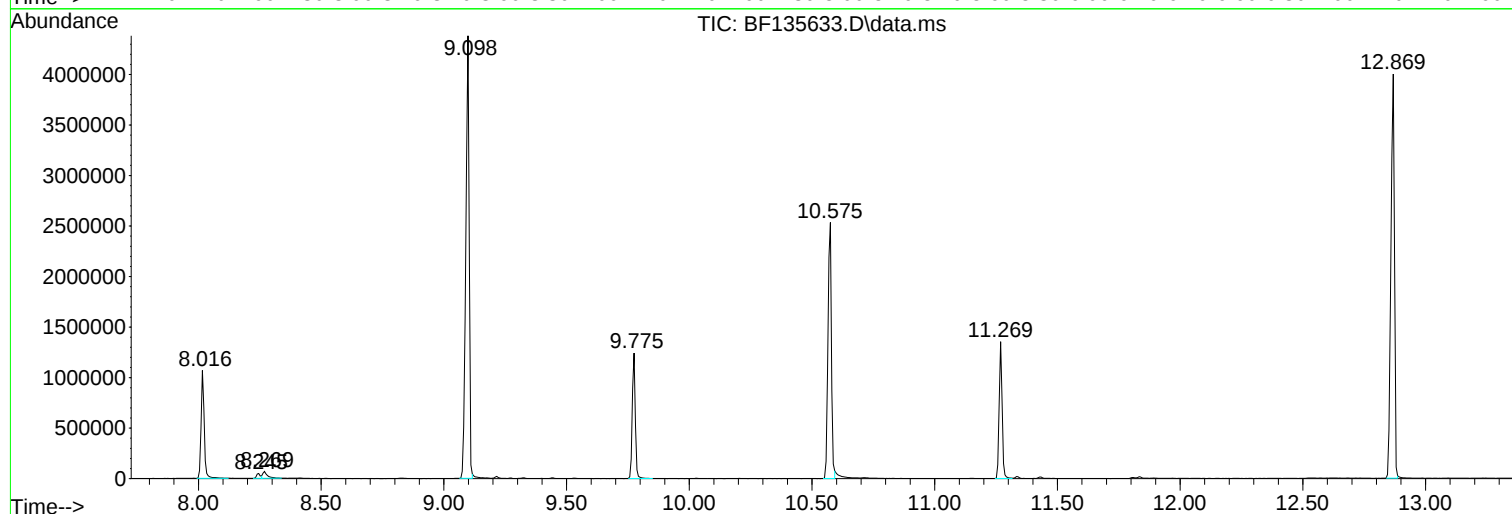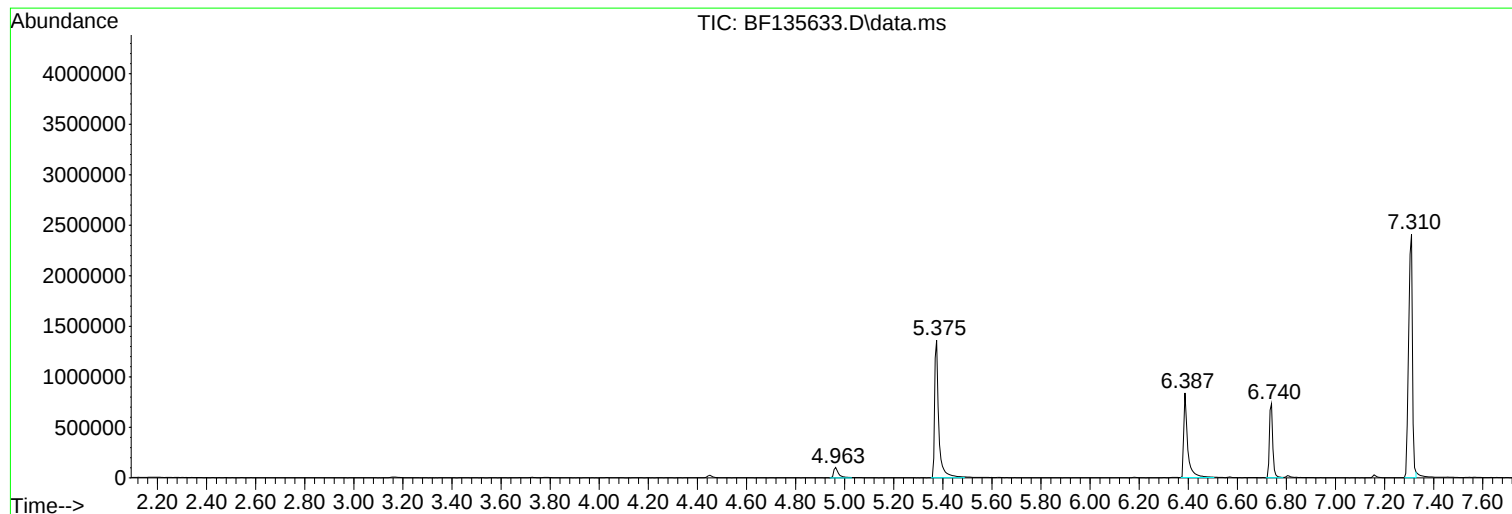

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
Data File : BF135633.D
Acq On : 06 Oct 2023 17:21
Operator : CG\JU
Sample : 04622-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.963	4.07 ng	141011	1,4-Dichlorobenzene-d4	6.740

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36		
3	3-Octanol	130	C8H18O	000589-98-0	33		
4	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		

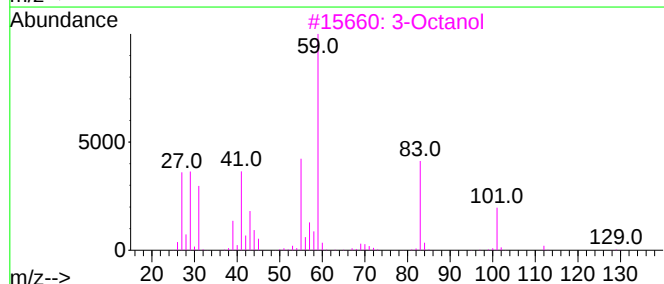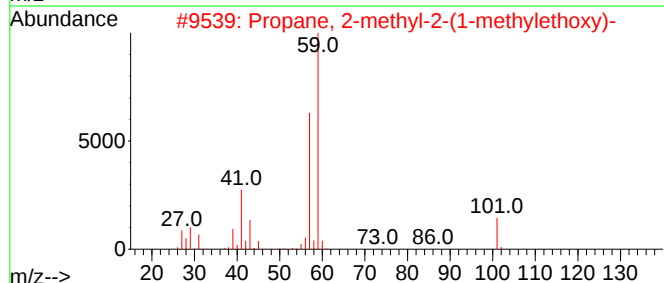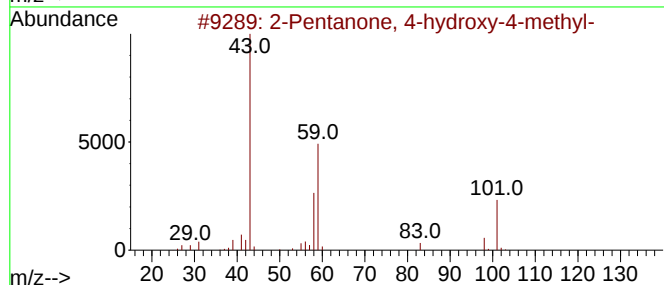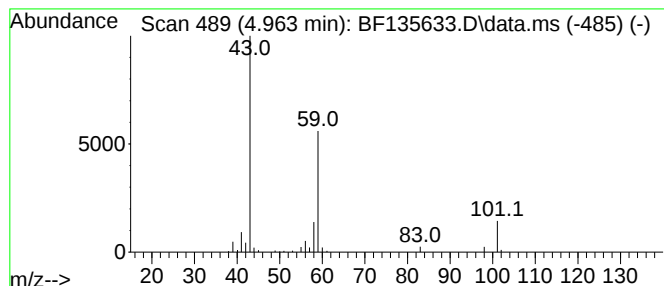

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
Data File : BF135633.D
Acq On : 06 Oct 2023 17:21
Operator : CG\JU
Sample : 04622-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.963	4.1	ng	141011	1	6.740	693494	20.0