


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
Data File : BF135619.D
Acq On : 06 Oct 2023 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 17:06:20 2023

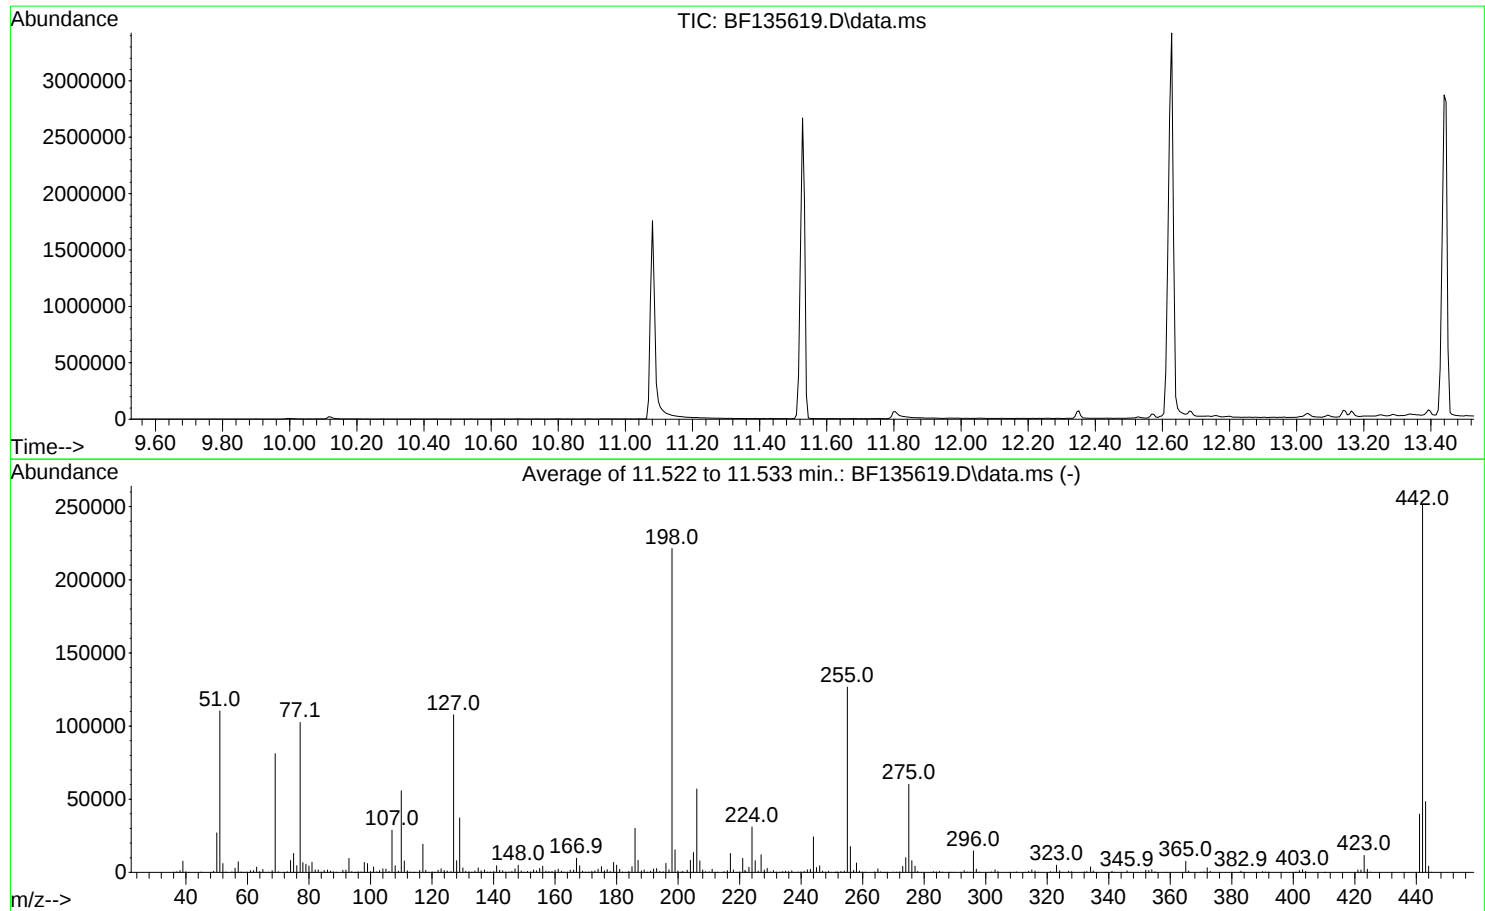




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	110421	PASS
68	69	0.00	2	1.5	1242	PASS
69	198	0.00	100	36.7	81168	PASS
70	69	0.00	2	0.6	463	PASS
127	198	10	80	48.7	107765	PASS
197	198	0.00	2	0.8	1809	PASS
198	198	100	100	100.0	221376	PASS
199	198	5	9	7.0	15471	PASS
275	198	10	60	27.2	60203	PASS
365	198	1	100	3.4	7598	PASS
441	198	0.01	100	18.0	39835	PASS
442	442	50	100	100.0	251483	PASS
443	442	15	24	19.2	48387	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
Data File : BF135619.D
Acq On : 06 Oct 2023 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 07 04:34:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

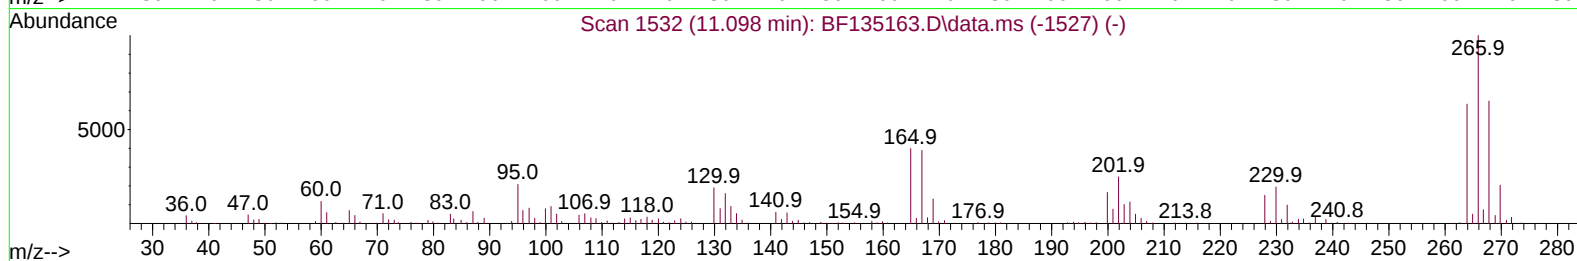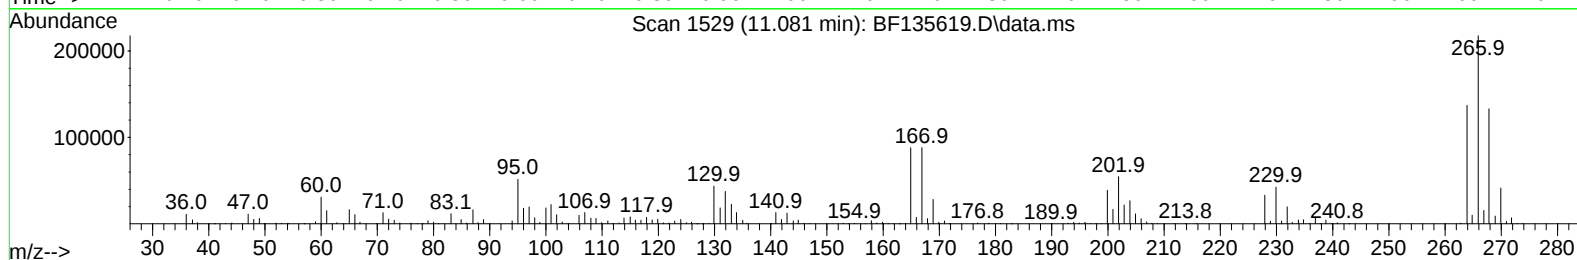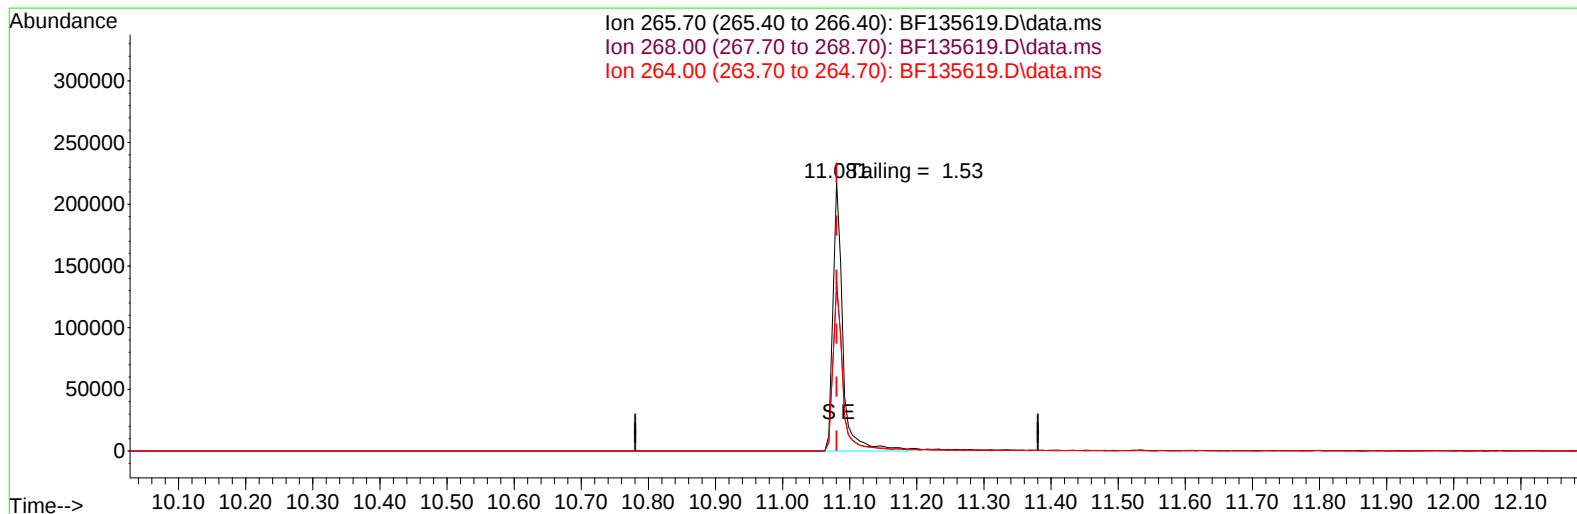

TIC: BF135619.D\data.ms

(70) Pentachlorophenol (C)

11.081min (+ 0.000) 563198.35 ng




response 221925

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.17
264.00	63.50	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100623\
 Data File : BF135619.D
 Acq On : 06 Oct 2023 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 04:34:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 04 17:06:20 2023
 Response via : Initial Calibration

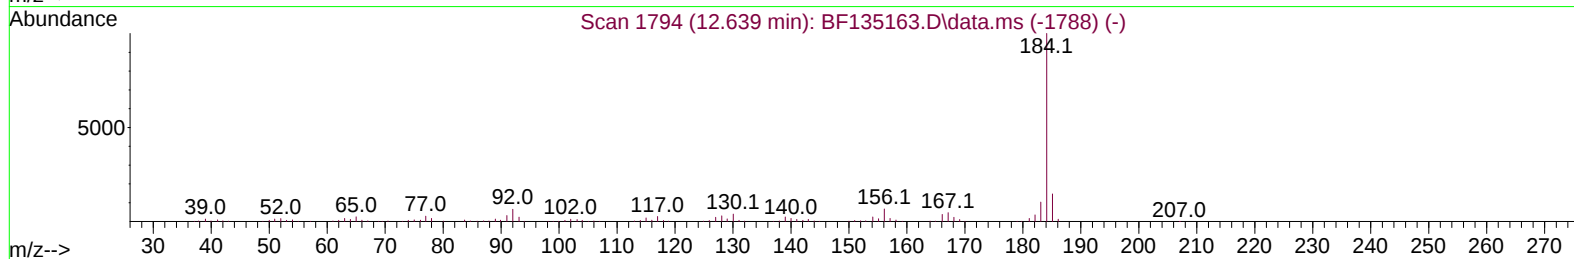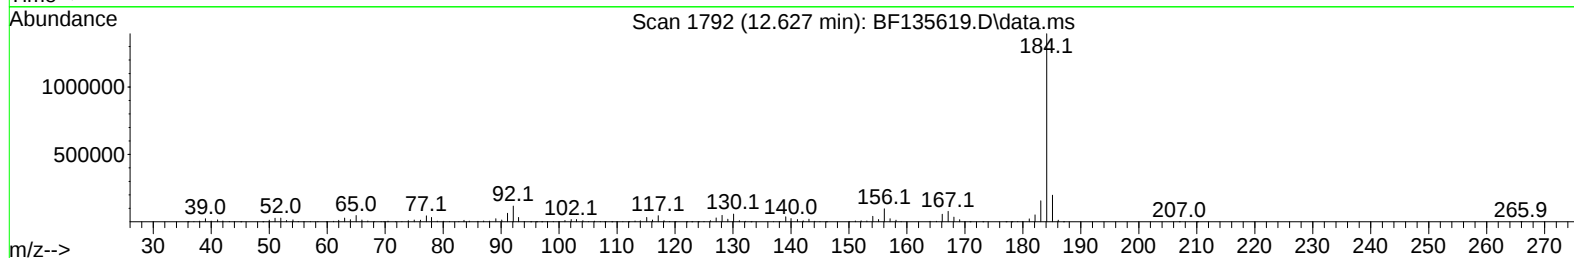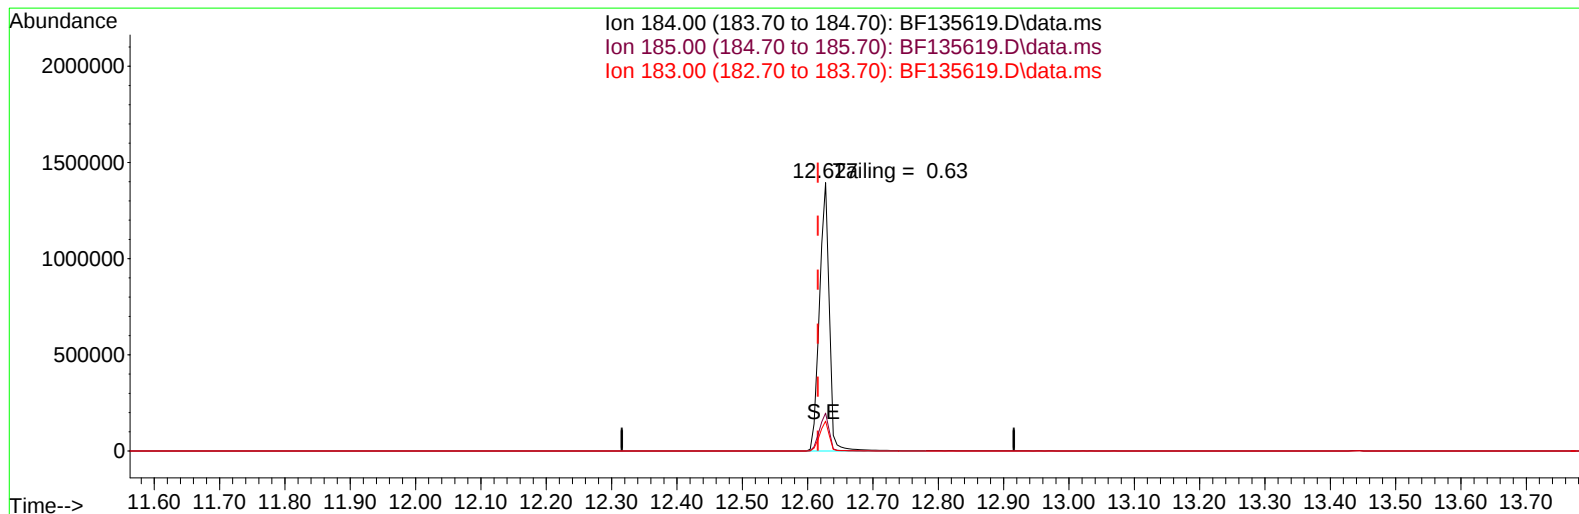

TIC: BF135619.D\data.ms

(77) Benzidine

12.627min (+ 0.012) 192016.75 ng

response 1467313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.12
183.00	10.30	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2023	BNA_F	<u>BF135619.D</u>
Compound Name	Response	Retention Time
DDT	576476	13.445
DDD	20227	13.139
DDE	761	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20988	597464	3.51

Instrument :
BNA_F
ClientSampleId :
DFTPP