
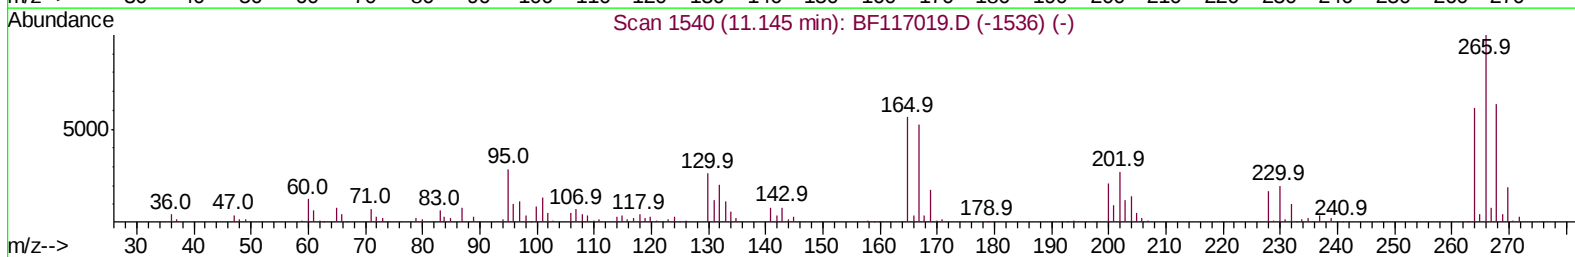
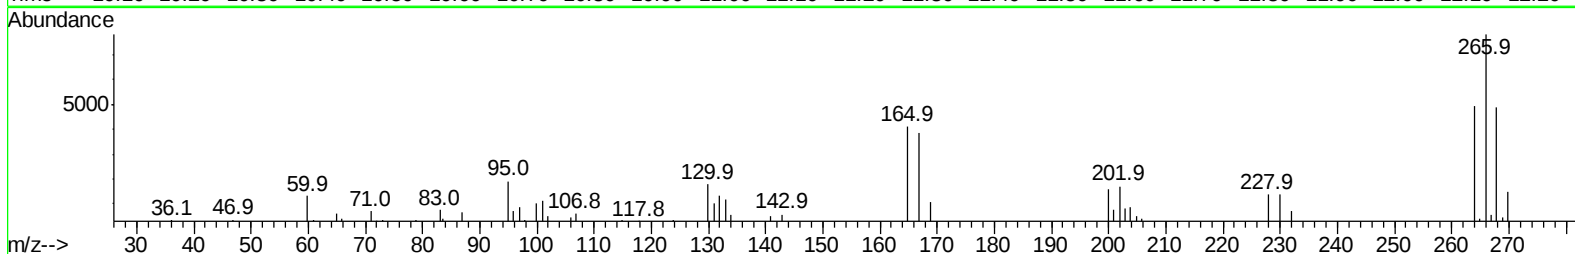


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100919\
Data File : BF117353.D
Acq On : 9 Oct 2019 13:52
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 23:26:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:26:00 2019
Response via : Initial Calibration

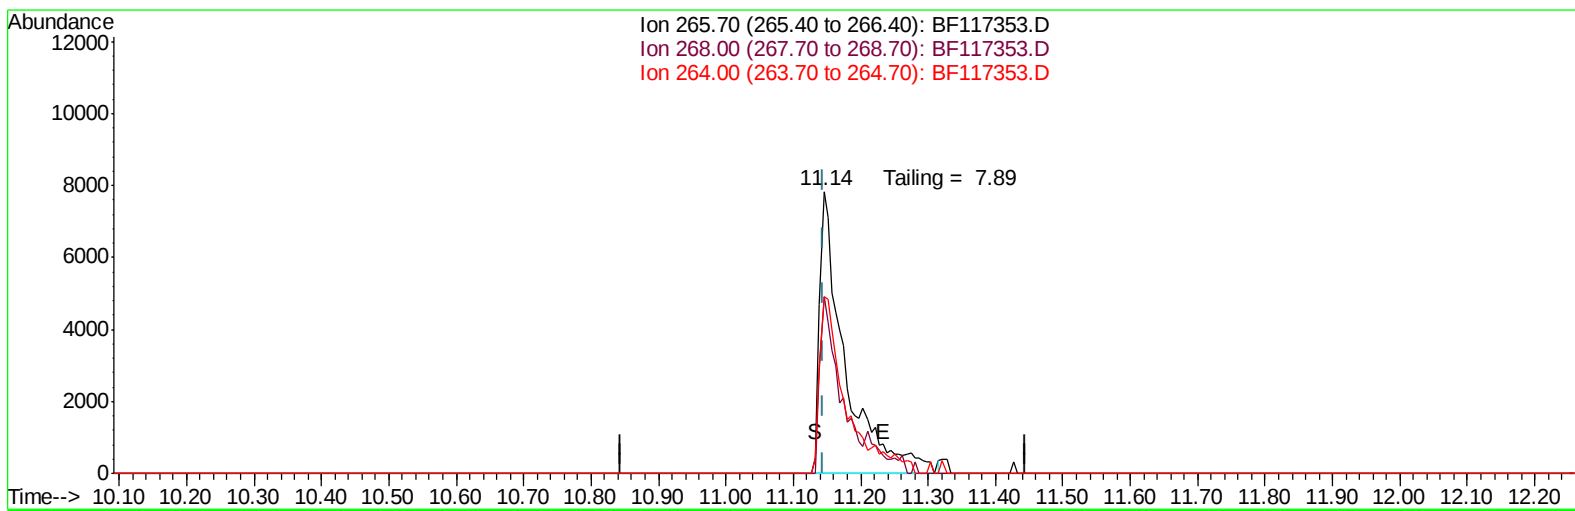

TIC: BF117353.D

(70) Pentachlorophenol (C)




11.145min (-0.000) 28699.31ng

response 19234

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.71
264.00	61.00	62.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100919\
 Data File : BF117353.D
 Acq On : 9 Oct 2019 13:52
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 23:26:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:26:00 2019
 Response via : Initial Calibration

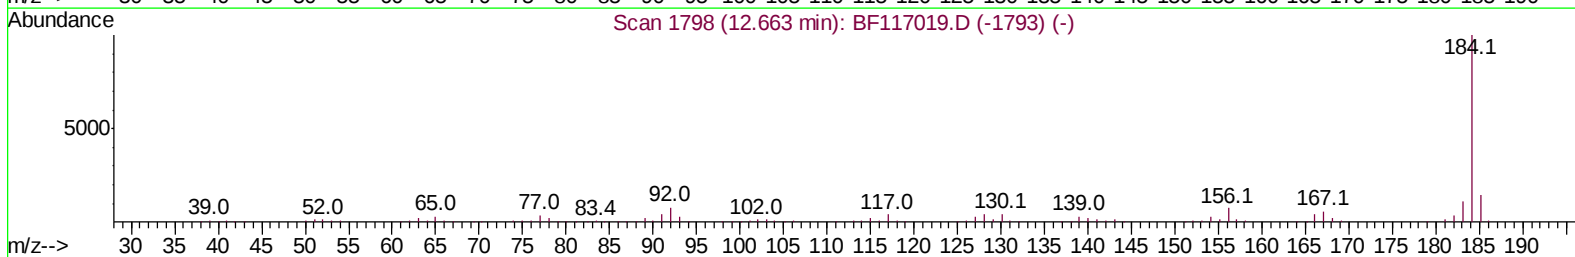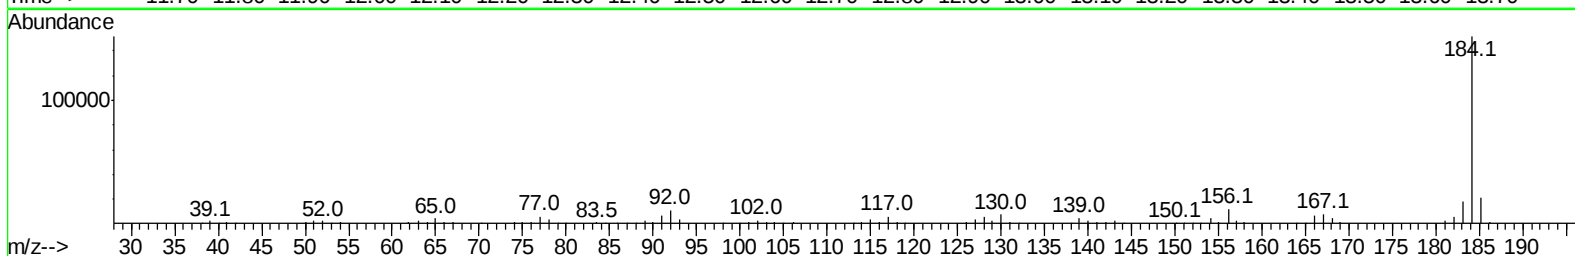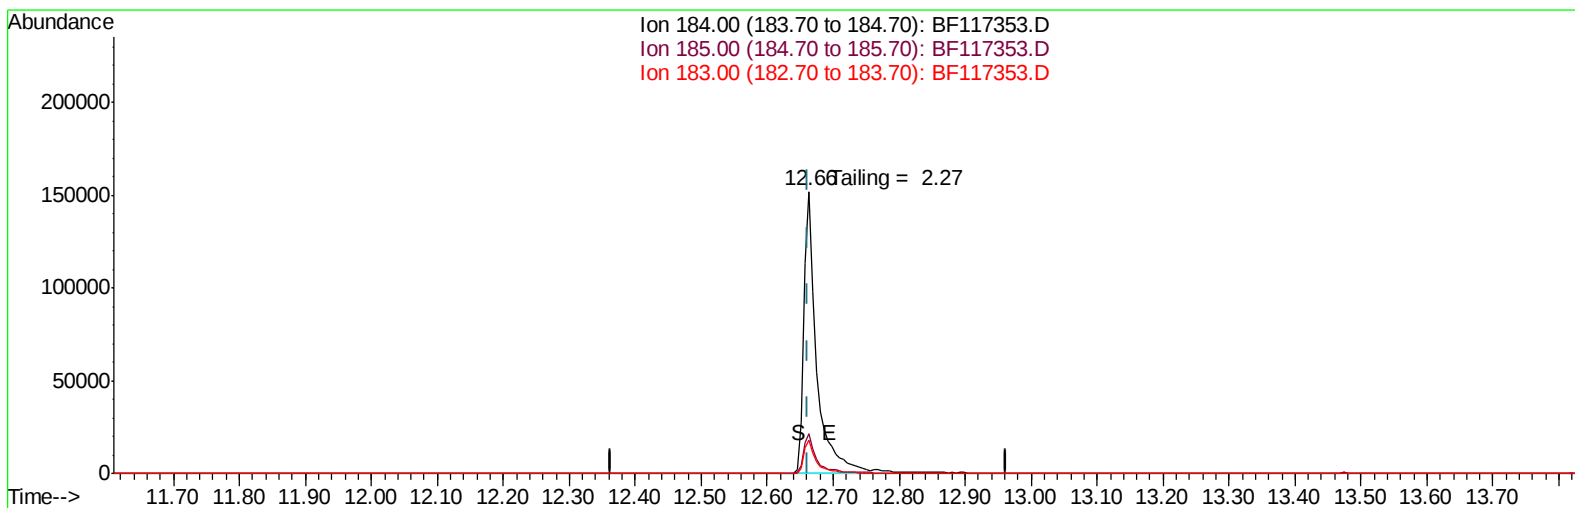

TIC: BF117353.D

(77) Benzidine

12.662min (-0.000) 0.00ng

response 211794

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.14
183.00	11.20	11.69
0.00	0.00	0.00