

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
 Data File : BF135656.D
 Acq On : 09 Oct 2023 17:54
 Operator : CG\JU
 Sample : PB156053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156053BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	579	rBV	3229663	3429227	88.94%	14.084%
2	6.392	727	732	753	rBV	3084760	3447330	89.41%	14.158%
3	6.739	787	791	797	rBV	740542	703325	18.24%	2.889%
4	7.304	883	887	904	rBV	2093241	2260546	58.63%	9.284%
5	8.016	1004	1008	1017	rBV	984810	920020	23.86%	3.778%
6	9.098	1186	1192	1195	rBV	3705183	3712571	96.29%	15.247%
7	9.774	1302	1307	1316	rBV	1144702	1019452	26.44%	4.187%
8	10.574	1439	1443	1461	rBV	2335146	2328443	60.39%	9.563%
9	11.269	1558	1561	1571	rBV	1281116	1119548	29.04%	4.598%
10	12.868	1828	1833	1837	rBV	3521764	3855783	100.00%	15.835%
11	13.933	2010	2014	2026	rVB	928661	894082	23.19%	3.672%
12	15.404	2259	2264	2275	rBV	449830	658662	17.08%	2.705%




Sum of corrected areas: 24348989

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135656.D
Acq On : 09 Oct 2023 17:54
Operator : CG\JU
Sample : PB156053BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

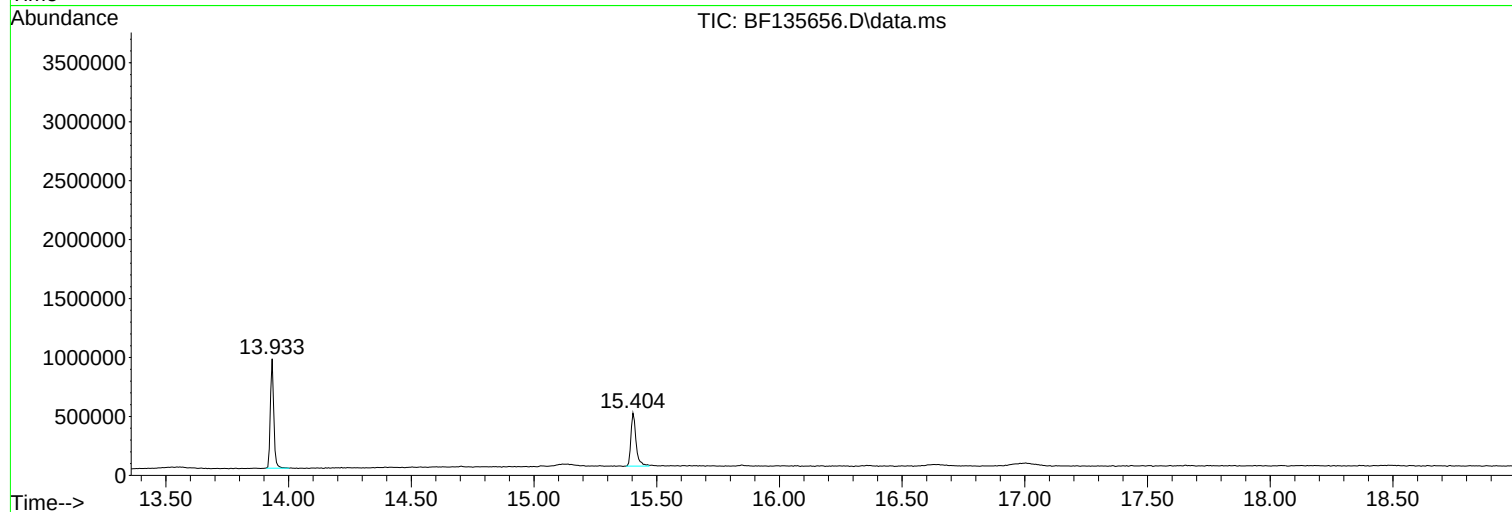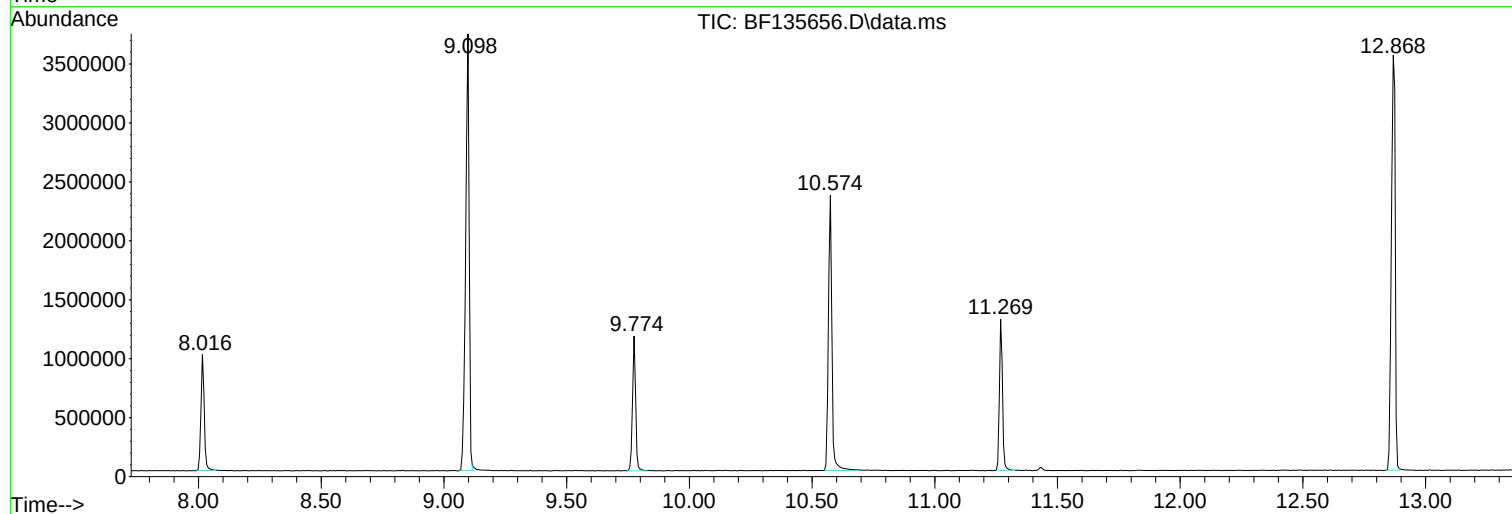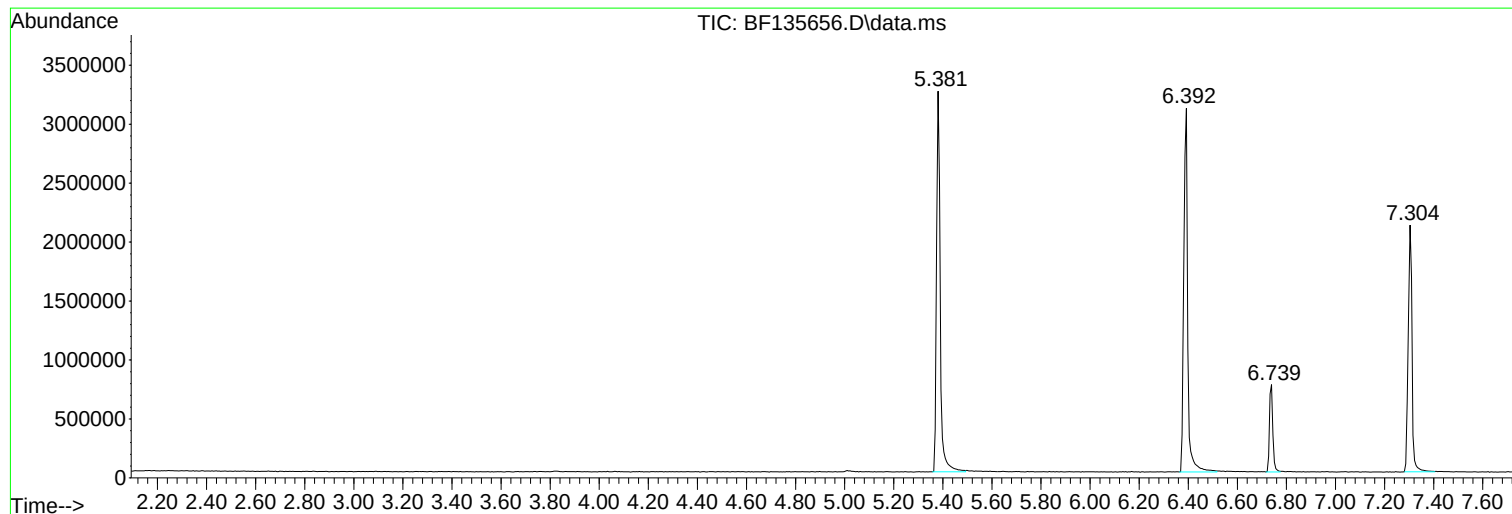

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135656.D
Acq On : 09 Oct 2023 17:54
Operator : CG\JU
Sample : PB156053BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135656.D
Acq On : 09 Oct 2023 17:54
Operator : CG\JU
Sample : PB156053BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------