
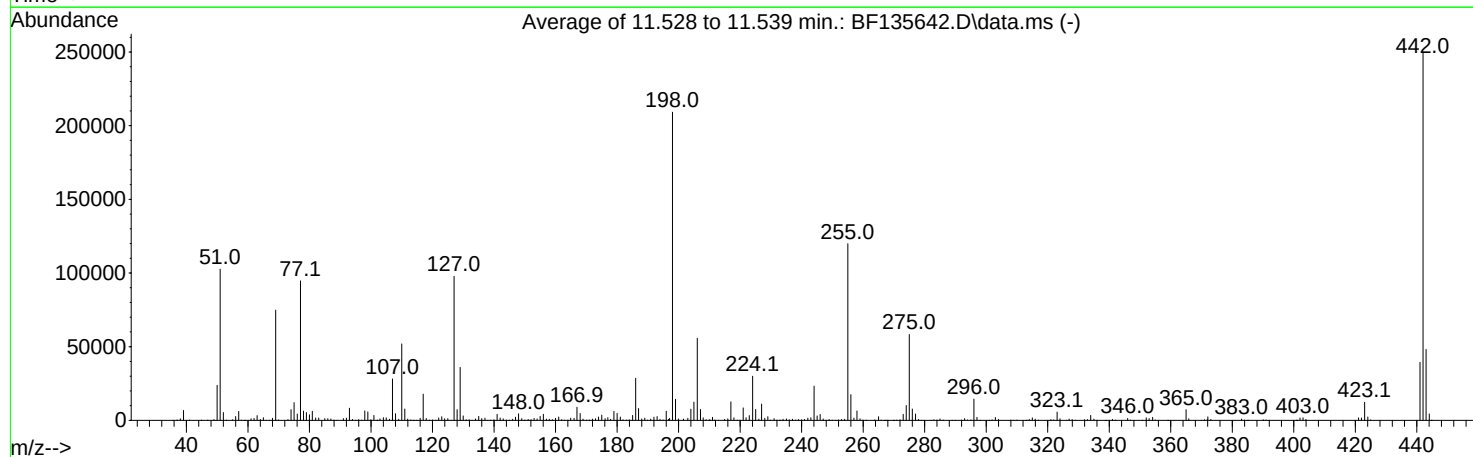


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135642.D
Acq On : 09 Oct 2023 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 17:06:20 2023

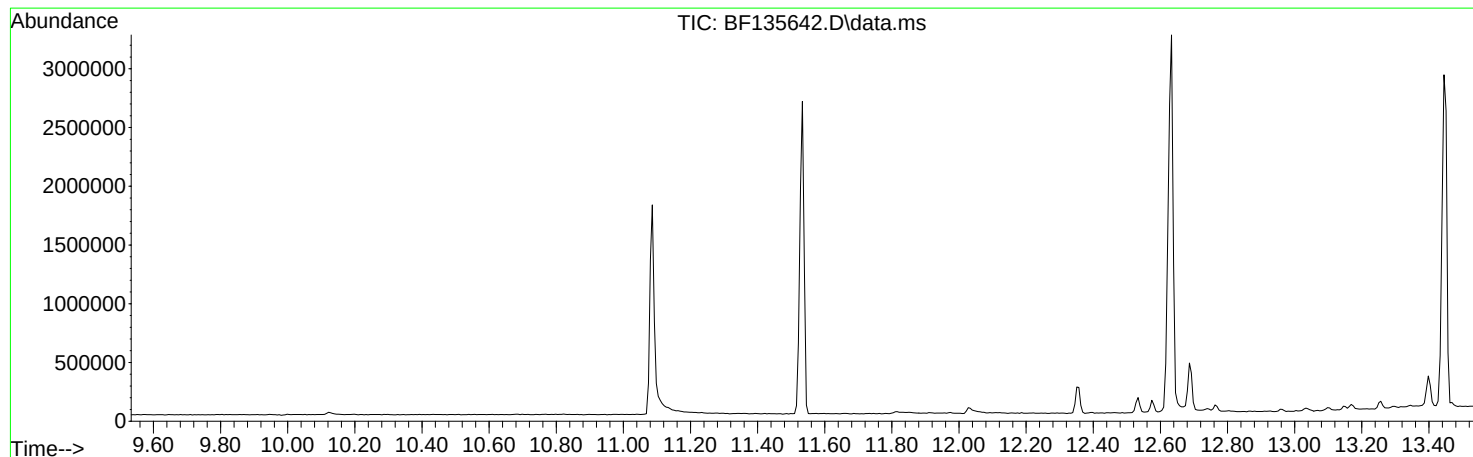




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	102651	PASS
68	69	0.00	2	1.9	1400	PASS
69	198	0.00	100	35.8	74798	PASS
70	69	0.00	2	0.4	324	PASS
127	198	10	80	46.7	97757	PASS
197	198	0.00	2	0.6	1359	PASS
198	198	100	100	100.0	209112	PASS
199	198	5	9	6.9	14356	PASS
275	198	10	60	27.9	58365	PASS
365	198	1	100	3.5	7257	PASS
441	198	0.01	100	18.8	39400	PASS
442	442	50	100	100.0	249643	PASS
443	442	15	24	19.3	48136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135642.D
Acq On : 09 Oct 2023 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 09 12:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

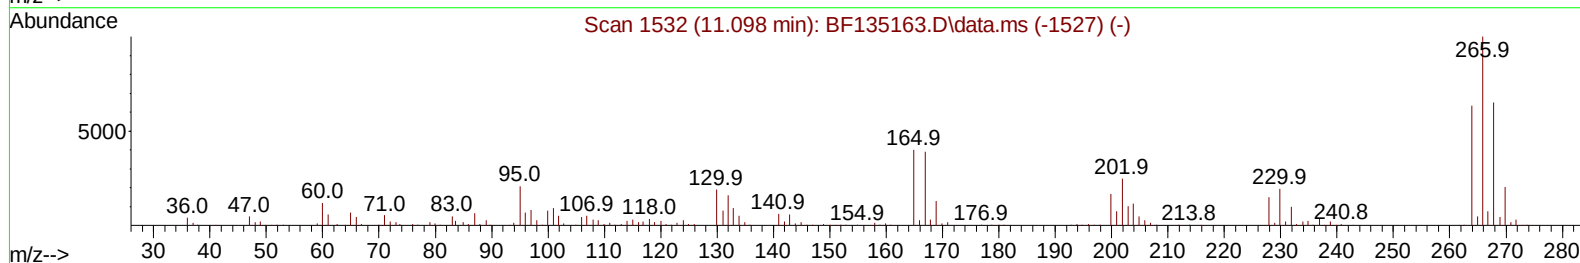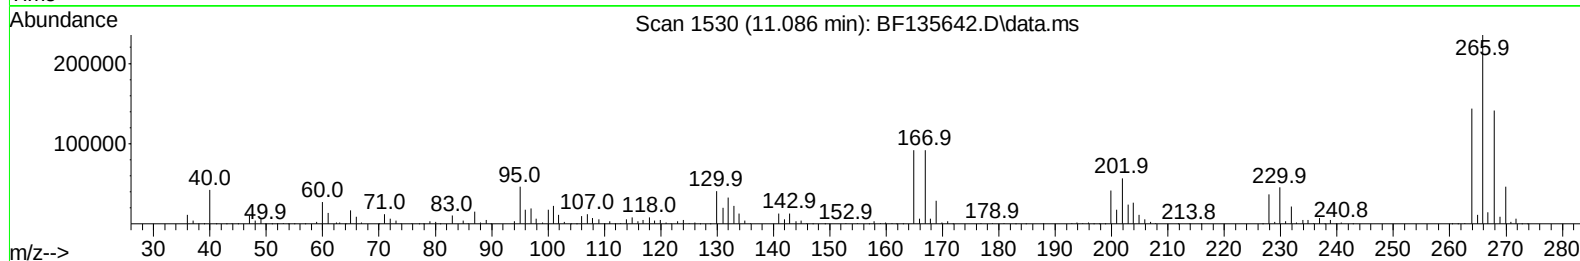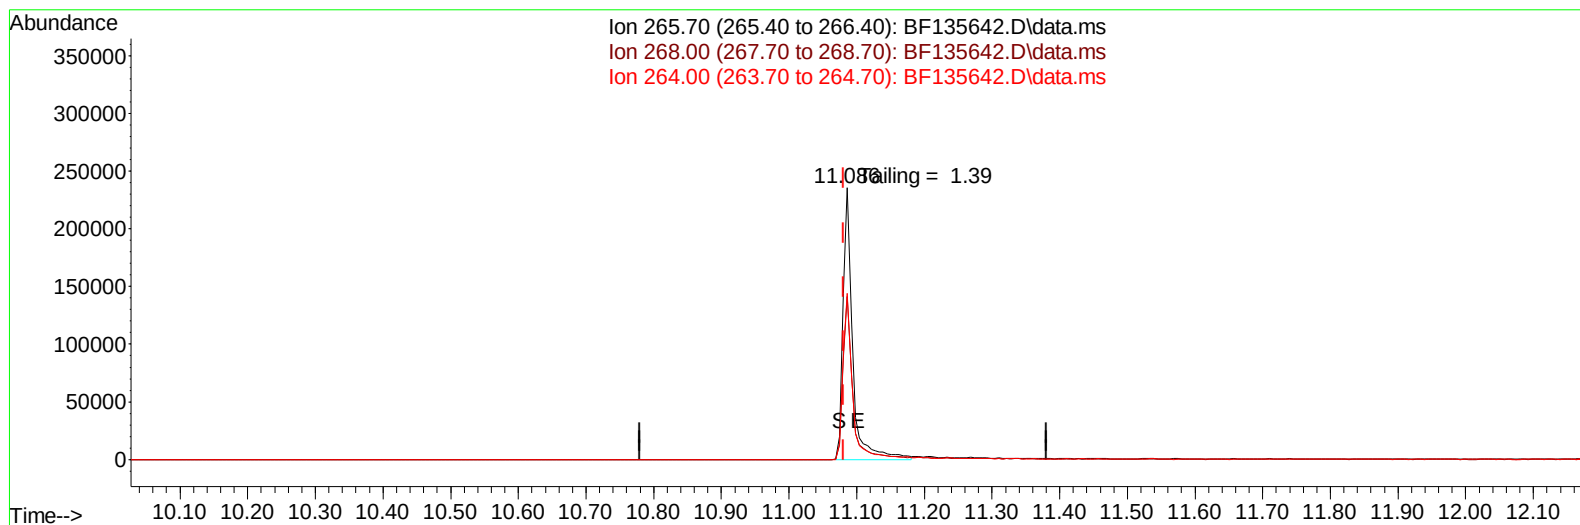

TIC: BF135642.D\data.ms

(70) Pentachlorophenol (C)

11.086min (+ 0.006) 566178.73 ng




response 229964

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	60.00
264.00	63.50	61.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100923\
Data File : BF135642.D
Acq On : 09 Oct 2023 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 09 12:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

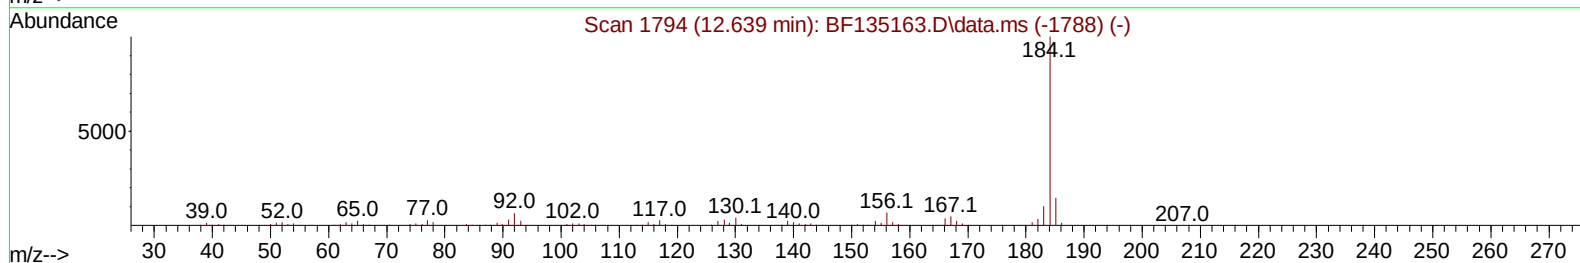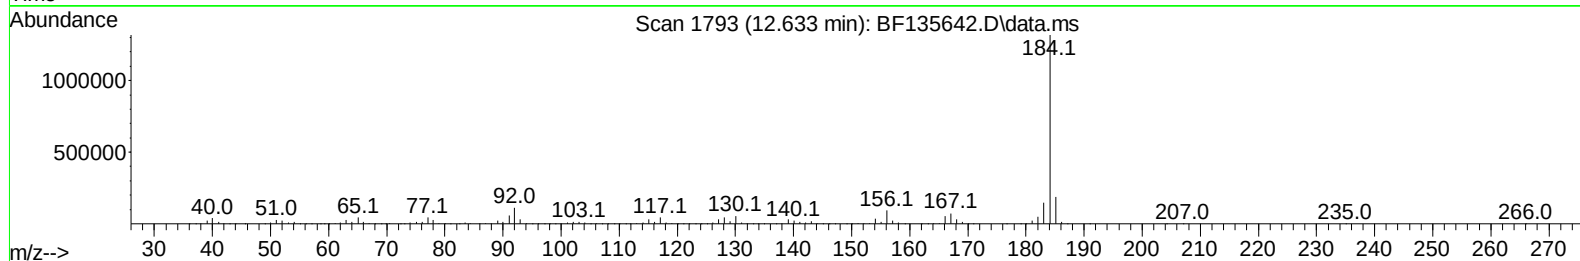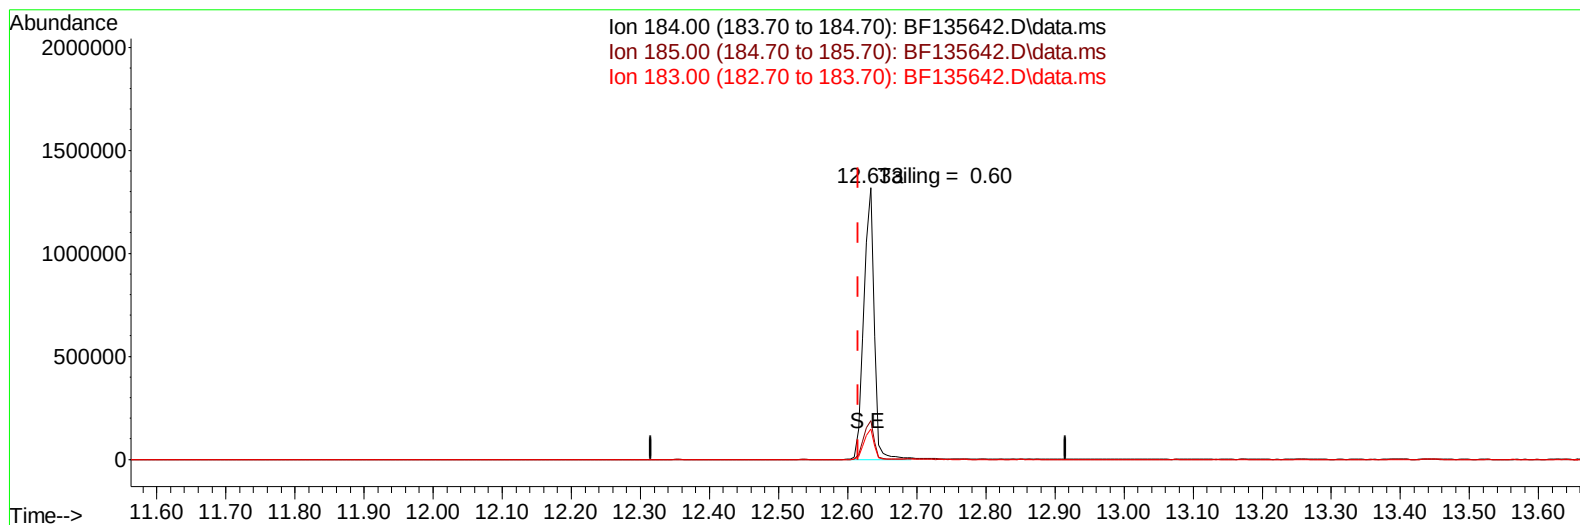

TIC: BF135642.D\data.ms

(77) Benzidine

12.633min (+ 0.018) 190550.09 ng

response 1311666

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.30	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2023	BNA_F	<u>BF135642.D</u>
Compound Name	Response	Retention Time
DDT	563530	13.445
DDD	13882	13.169
DDE	386	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14268	577798	2.47

Instrument :
BNA_F
ClientSampleId :
DFTPP