

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101018\
 Data File : BF109759.D
 Acq On : 10 Oct 2018 23:05
 Operator : JU/SJ
 Sample : J5373-03 4X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RT1499-3783-RT3026

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.875	471	474	481	rVB2	7405	9322	1.26%	0.130%
2	5.310	545	548	565	rBV	118686	212700	28.82%	2.957%
3	6.345	720	724	741	rBV	127662	291549	39.50%	4.053%
4	6.469	741	745	759	rVV	230715	328615	44.52%	4.568%
5	6.692	780	783	806	rBV	388609	485710	65.81%	6.752%
6	6.851	806	810	821	rBV	211444	242459	32.85%	3.370%
7	7.257	876	879	897	rBV	80022	185827	25.18%	2.583%
8	7.975	998	1001	1012	rBV	623780	630115	85.37%	8.759%
9	9.045	1180	1183	1197	rBV	288811	335487	45.45%	4.664%
10	9.445	1248	1251	1256	rBV	44103	45278	6.13%	0.629%
11	9.722	1294	1298	1310	rBV	764542	723052	97.96%	10.051%
12	10.269	1388	1391	1397	rVB2	8211	8735	1.18%	0.121%
13	10.510	1428	1432	1445	rBV	154644	208026	28.18%	2.892%
14	10.633	1447	1453	1458	rVB2	5367	10299	1.40%	0.143%
15	11.204	1546	1550	1552	rBV	532355	574210	77.80%	7.982%
16	11.222	1552	1553	1560	rVV	188585	206126	27.93%	2.865%
17	11.280	1560	1563	1572	rVB	28408	45827	6.21%	0.637%
18	11.704	1632	1635	1637	rBV	17117	16702	2.26%	0.232%
19	11.733	1637	1640	1646	rVV3	27482	32685	4.43%	0.454%
20	11.810	1650	1653	1656	rBV2	26181	30918	4.19%	0.430%
21	11.998	1681	1685	1688	rBV	10121	12896	1.75%	0.179%
22	12.251	1725	1728	1732	rBV3	14554	17500	2.37%	0.243%
23	12.292	1732	1735	1740	rVV4	18490	33846	4.59%	0.470%
24	12.339	1740	1743	1751	rVB3	13858	20775	2.81%	0.289%
25	12.410	1751	1755	1764	rBV	193680	239495	32.45%	3.329%
26	12.557	1778	1780	1784	rVB3	6529	7496	1.02%	0.104%
27	12.633	1788	1793	1800	rVV	202868	243411	32.98%	3.384%
28	12.692	1800	1803	1810	rVB5	11355	17791	2.41%	0.247%
29	12.774	1814	1817	1824	rVV	270327	276586	37.47%	3.845%
30	12.851	1828	1830	1836	rVB2	14315	17425	2.36%	0.242%
31	12.939	1842	1845	1846	rBV2	11622	9565	1.30%	0.133%
32	12.968	1846	1850	1853	rVV2	23248	28702	3.89%	0.399%
33	13.027	1857	1860	1864	rVV3	12904	15986	2.17%	0.222%
34	13.068	1864	1867	1870	rBV2	20254	26420	3.58%	0.367%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101018\
Data File : BF109759.D
Acq On : 10 Oct 2018 23:05
Operator : JU/SJ
Sample : J5373-03 4X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT1499-3783-RT3026

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.157	1879	1882	1884	rBV	21370	18158	2.46%	0.252%
36	13.186	1885	1887	1892	rVB2	12645	14425	1.95%	0.201%
37	13.474	1934	1936	1942	rVB2	18930	23883	3.24%	0.332%
38	13.527	1943	1945	1949	rVB2	10590	8935	1.21%	0.124%
39	13.586	1949	1955	1957	rBV3	24280	44431	6.02%	0.618%
40	13.680	1968	1971	1980	rVB	48595	68918	9.34%	0.958%
41	13.827	1989	1996	1999	rBV2	605858	738084	100.00%	10.260%
42	14.839	2165	2168	2176	rVB	67514	114896	15.57%	1.597%
43	15.168	2222	2224	2230	rVB	60568	84410	11.44%	1.173%
44	15.227	2230	2234	2243	rBV	337550	486035	65.85%	6.756%


Sum of corrected areas: 7193711

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101018\
Data File : BF109759.D
Acq On : 10 Oct 2018 23:05
Operator : JU/SJ
Sample : J5373-03 4X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT1499-3783-RT3026

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

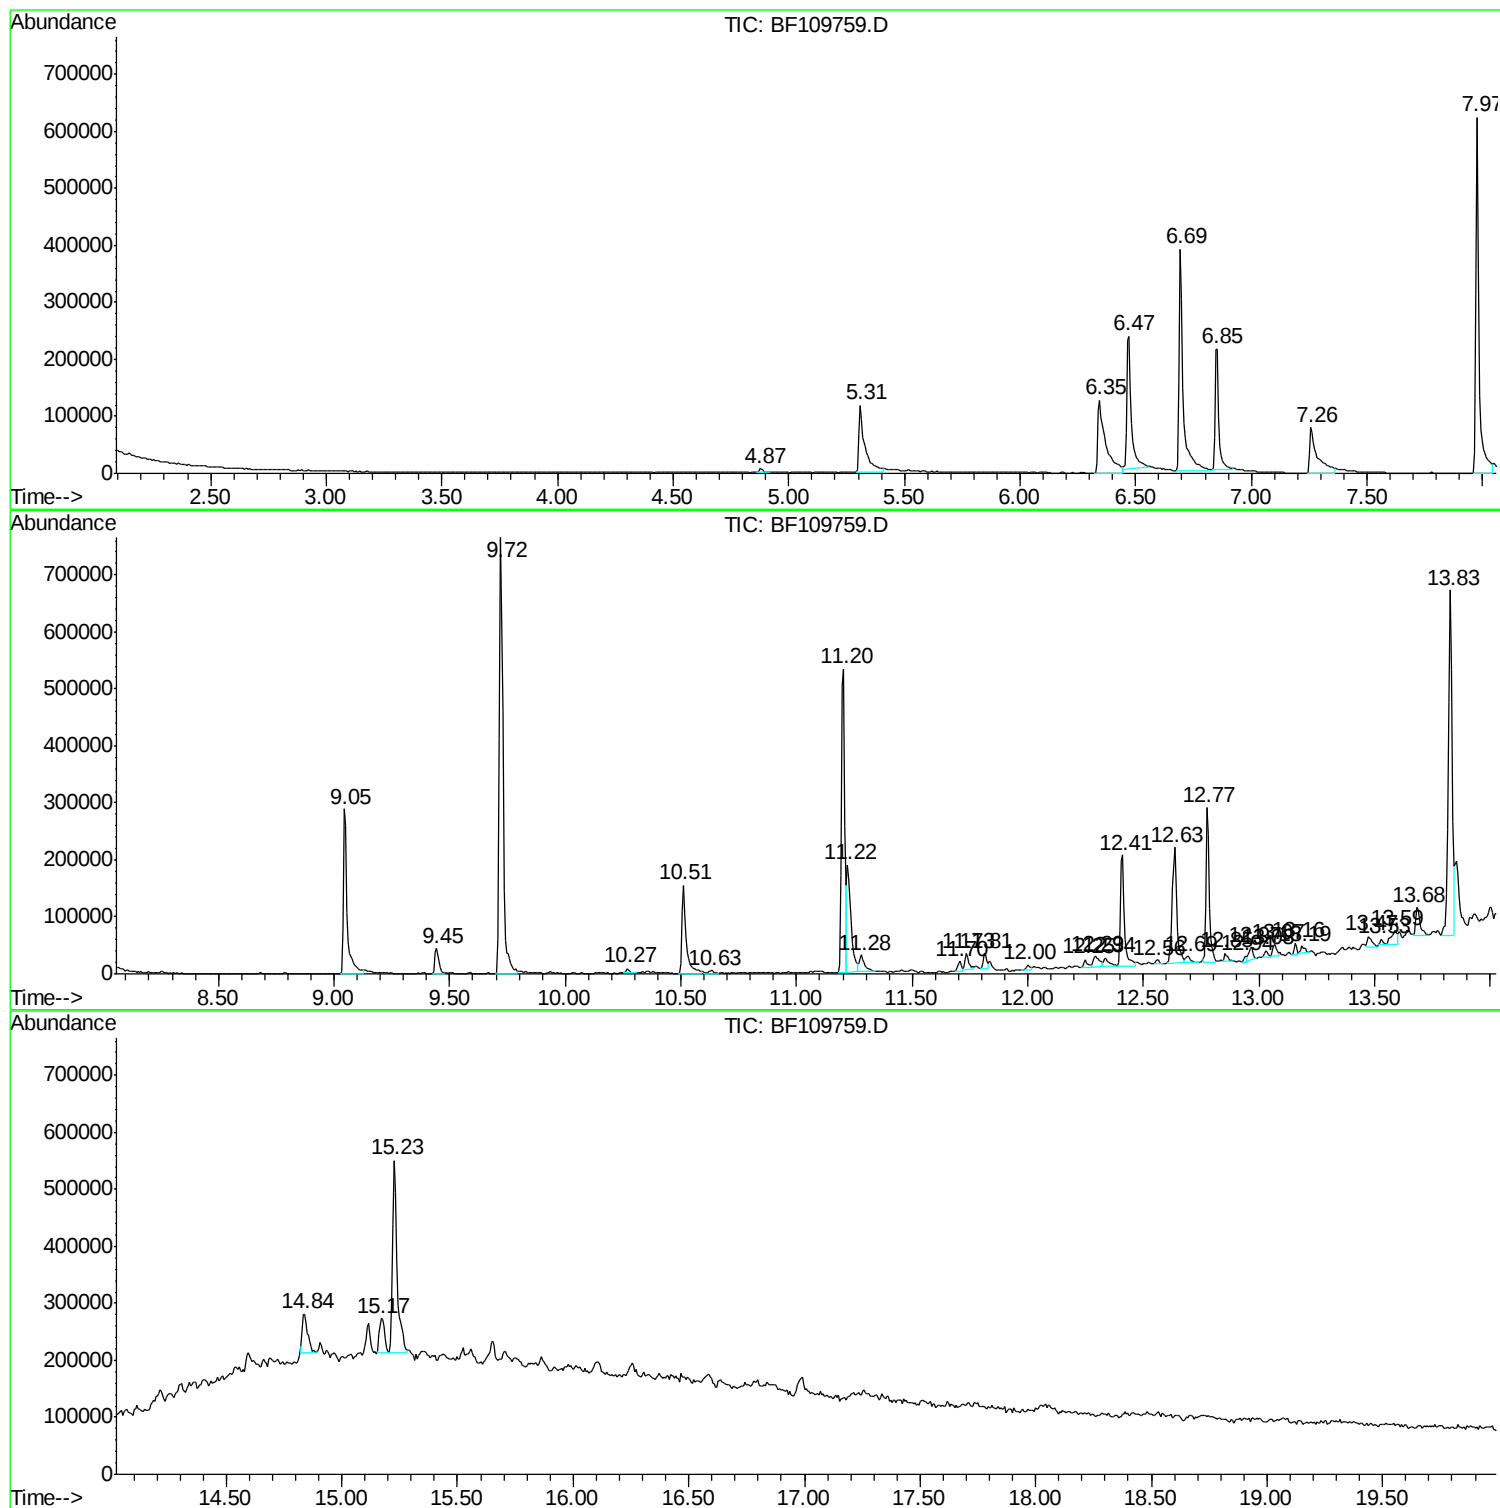

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101018\
Data_File : BF109759.D
Acq_On : 10_Oct_2018_ 23:055
Operator : JU/SJJ
Sample : J5373-03_4XX
Misc :
ALS_Vial : 23_ Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
RT1499-3783-RT3026

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
