
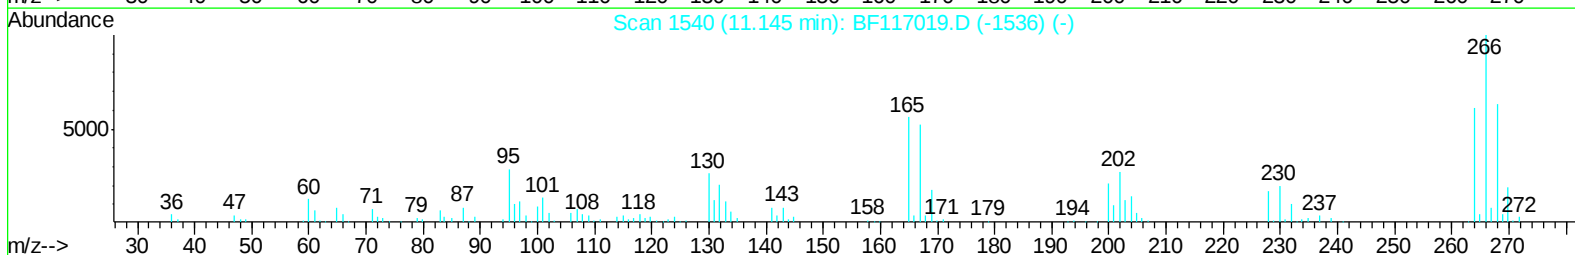
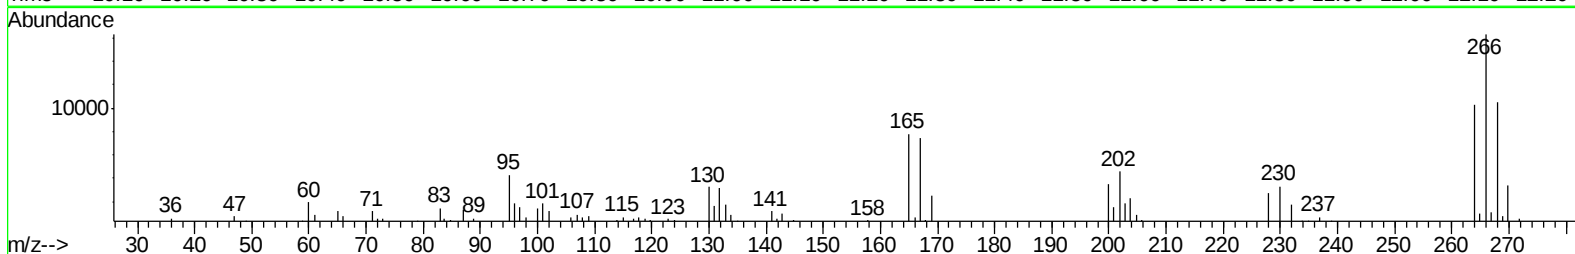


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101019\
 Data File : BF117359.D
 Acq On : 10 Oct 2019 14:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 11 05:20:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:26:00 2019
 Response via : Initial Calibration

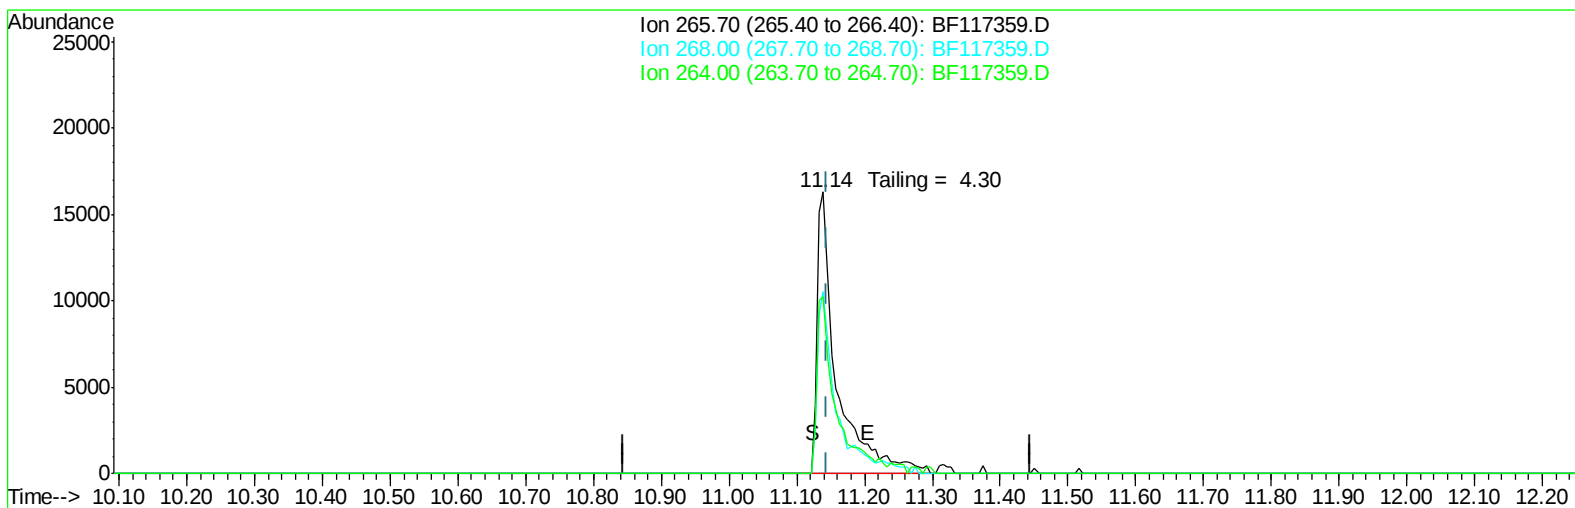

TIC: BF117359.D

(70) Pentachlorophenol (C)

11.139min (-0.006) 0.00ng




response 30703

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	64.37
264.00	61.00	62.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101019\
Data File : BF117359.D
Acq On : 10 Oct 2019 14:51
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 11 05:20:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:26:00 2019
Response via : Initial Calibration

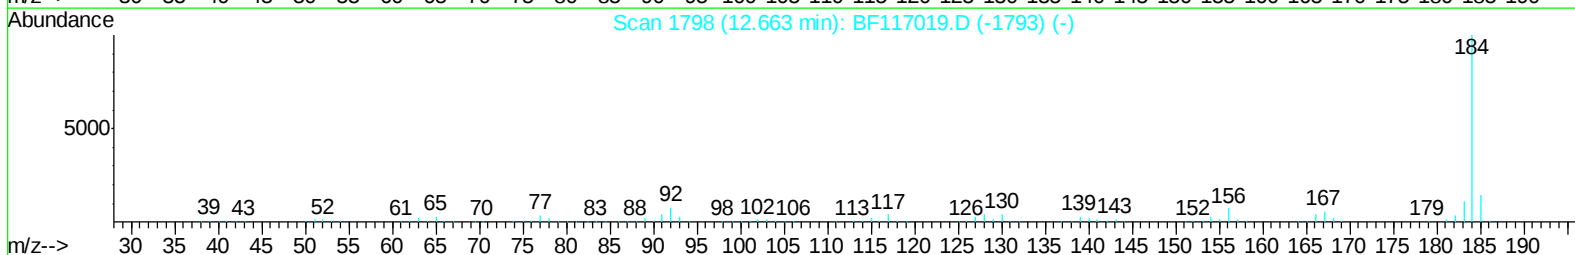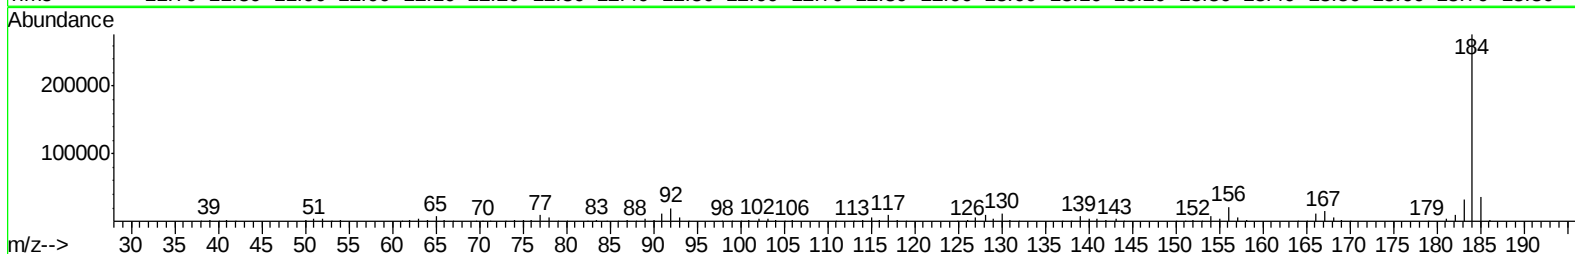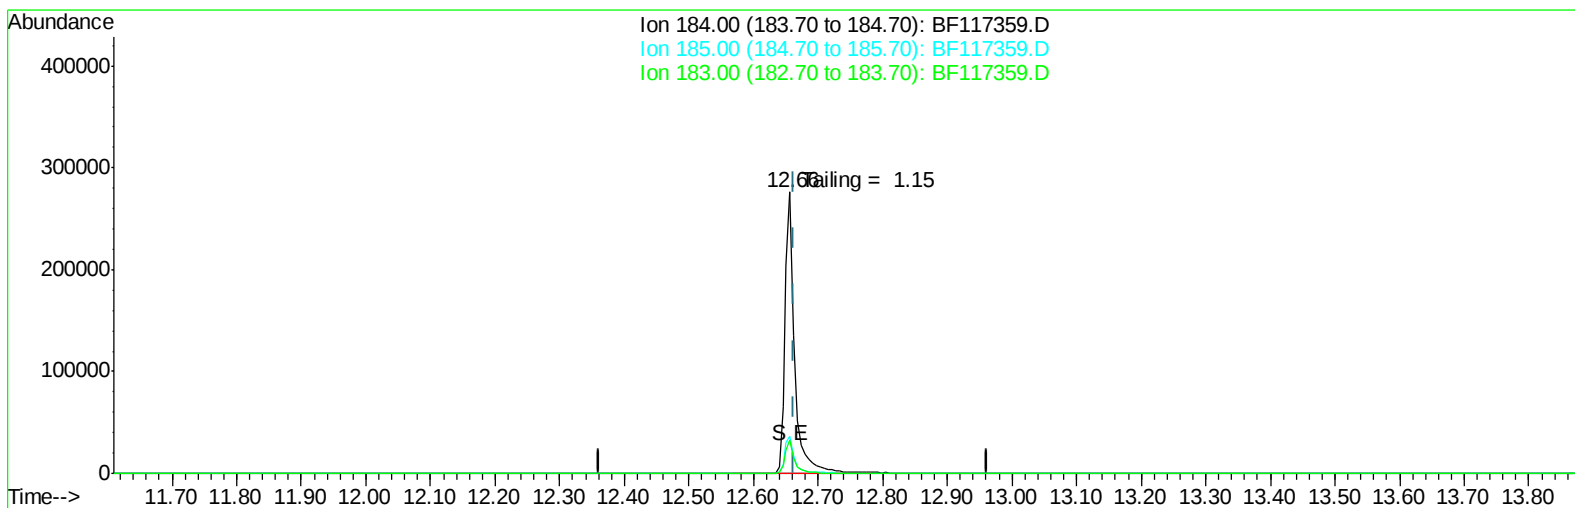

TIC: BF117359.D

(77) Benzidine

12.657min (-0.006) 0.00ng

response 303544

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	13.01
183.00	11.20	11.62
0.00	0.00	0.00