


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101019\
 Data File : BF117359.D
 Acq On : 10 Oct 2019 14:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:26:00 2019

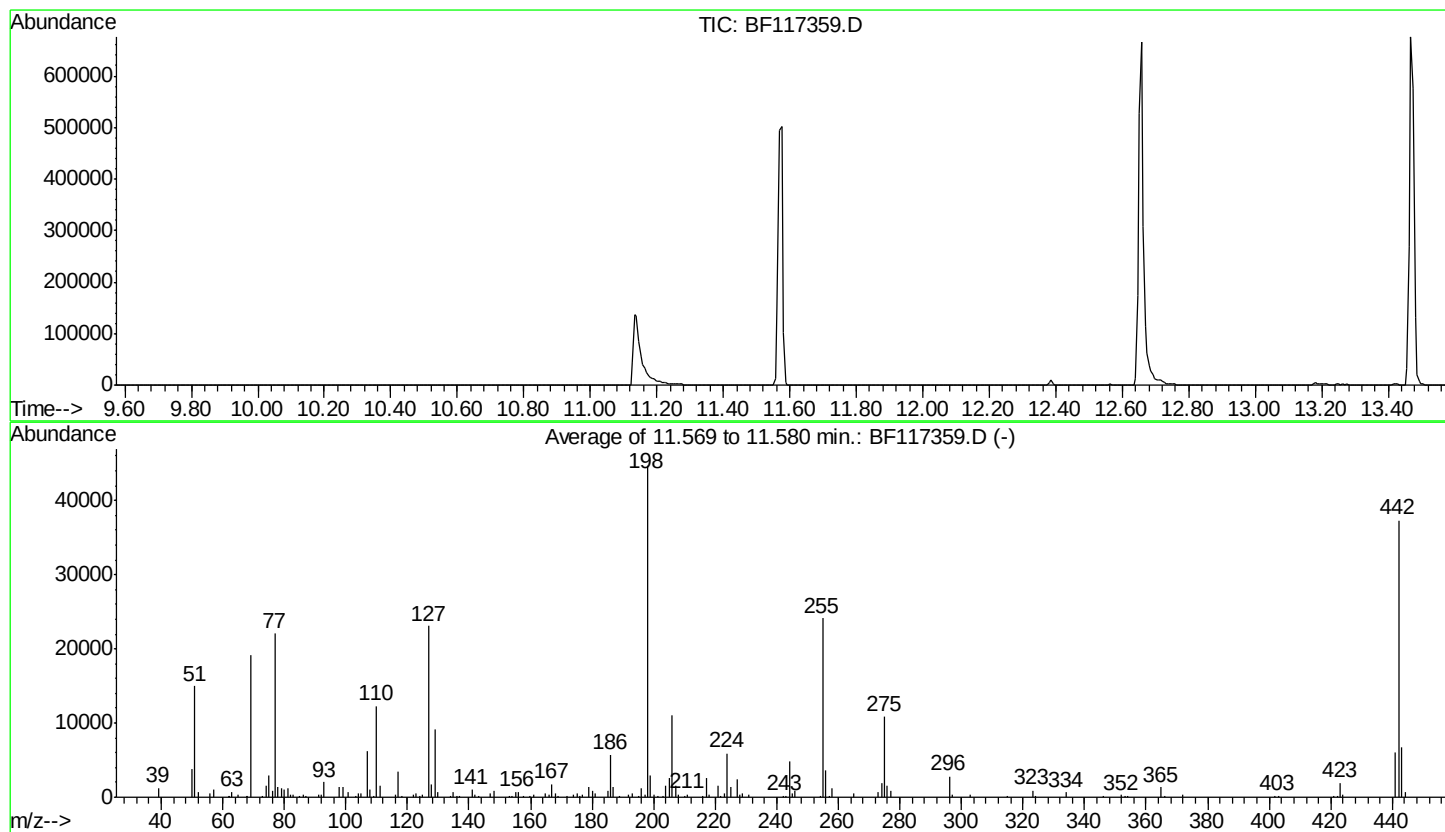

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	15011	PASS
68	69	0.00	2	0.6	119	PASS
69	198	0.00	100	43.0	19221	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	23107	PASS
197	198	0.00	2	0.9	405	PASS
198	198	100	100	100.0	44698	PASS
199	198	5	9	6.5	2919	PASS
275	198	10	60	24.2	10830	PASS
365	198	1	100	3.0	1332	PASS
441	198	0.01	100	13.6	6082	PASS
442	198	50	100	83.4	37277	PASS
443	442	15	24	18.0	6714	PASS