
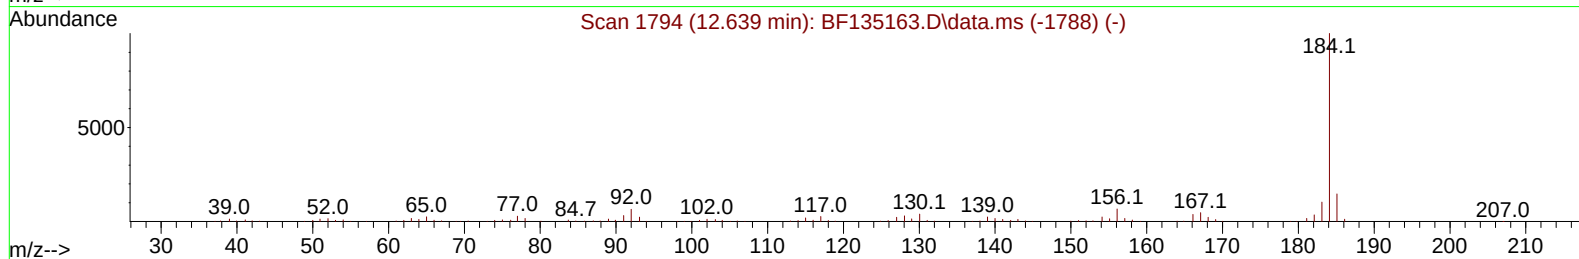
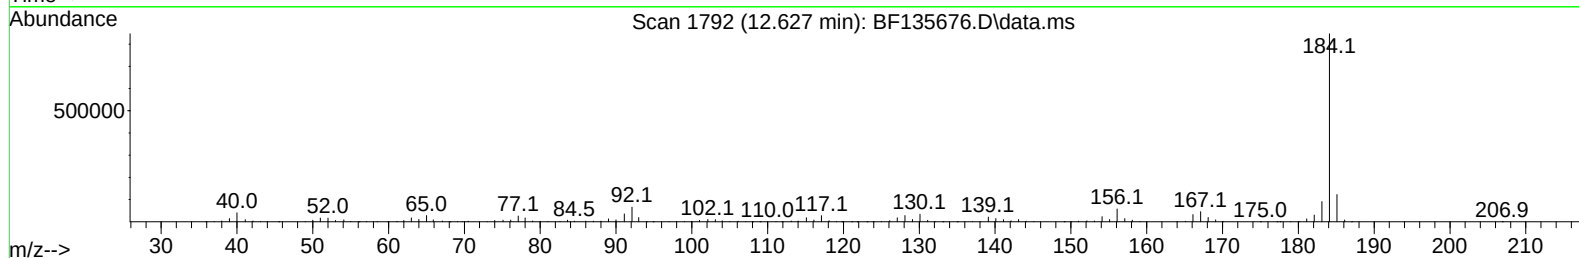


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135676.D
Acq On : 10 Oct 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 11:42:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

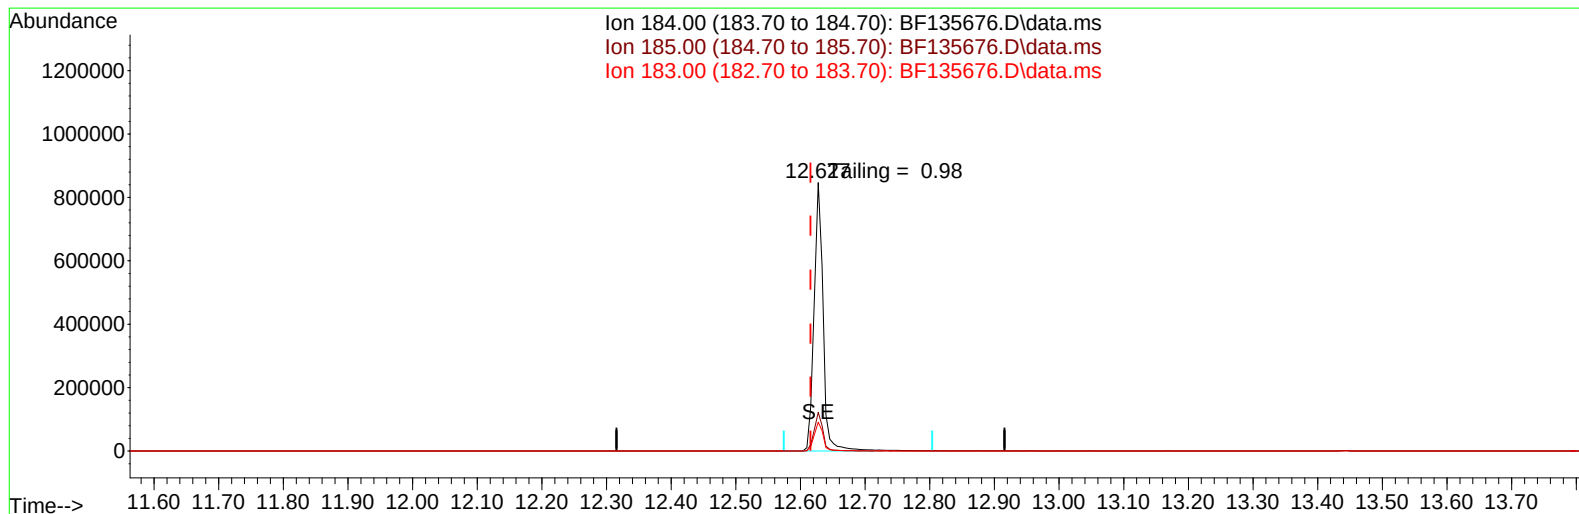




TIC: BF135676.D\data.ms

(77) Benzidine**12.627min (+ 0.012) 305572.76 ng****response 832609**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.45
183.00	10.30	10.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135676.D
Acq On : 10 Oct 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 11:42:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

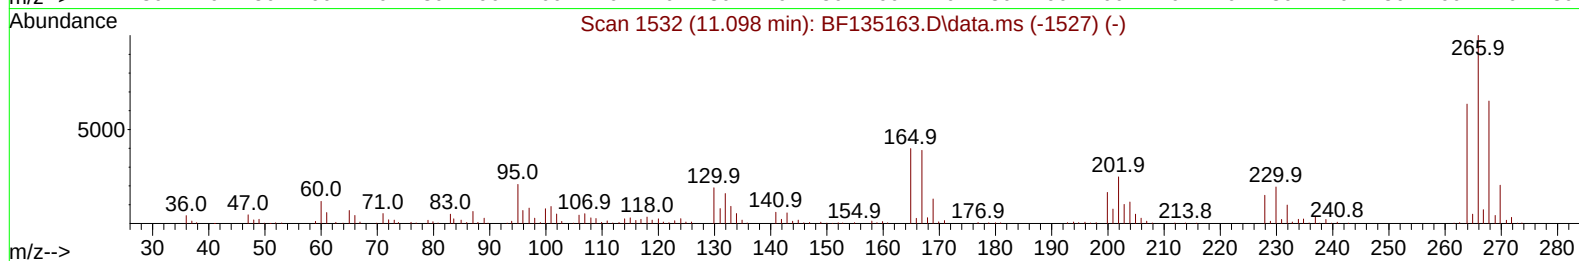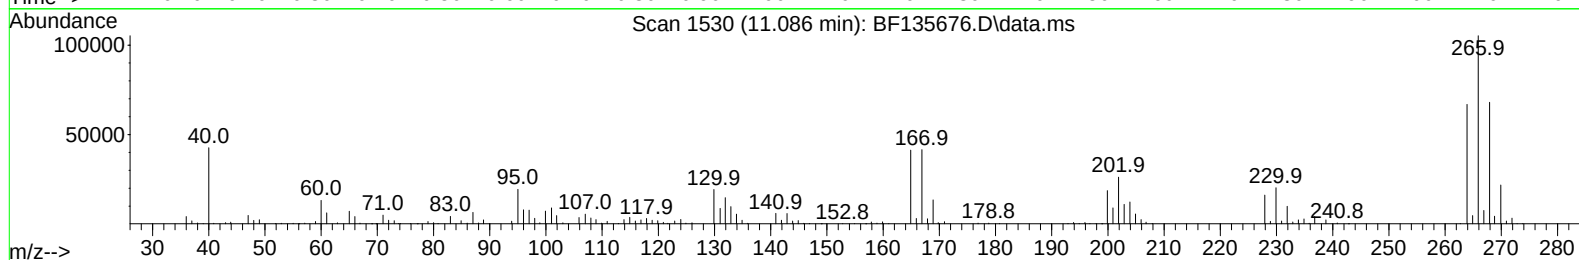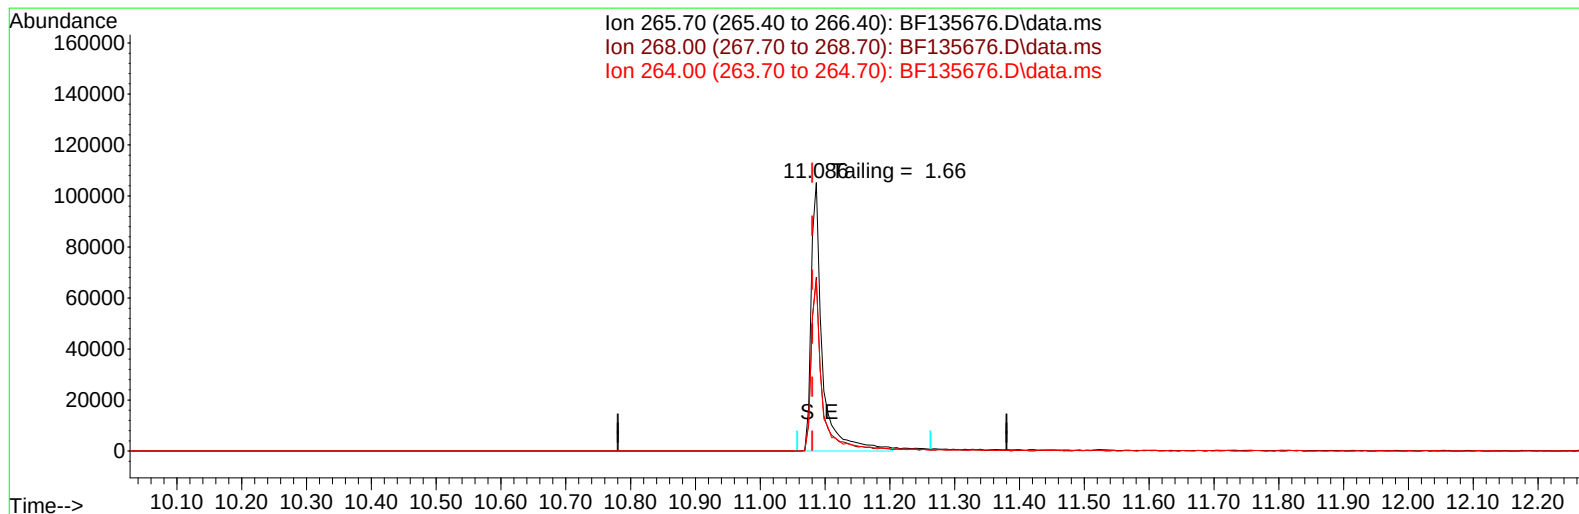

TIC: BF135676.D\data.ms

(70) Pentachlorophenol (C)

11.086min (+ 0.006) 28896.51 ng

response 130682

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.68
264.00	63.50	63.57
0.00	0.00	0.00