

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
 Data File : BF135683.D
 Acq On : 10 Oct 2023 14:21
 Operator : CG\JU
 Sample : PB156207BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156207BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	488	492	505	rBV	468743	782293	20.91%	3.205%
2	5.381	556	560	582	rBV	2977392	3439212	91.91%	14.092%
3	6.393	727	732	751	rBV	3074589	3411325	91.16%	13.978%
4	6.740	787	791	799	rBV	655165	630293	16.84%	2.583%
5	7.304	883	887	898	rBV	2032041	2250448	60.14%	9.221%
6	8.016	1004	1008	1015	rBV	884436	812790	21.72%	3.330%
7	9.098	1186	1192	1195	rBV	3704405	3742086	100.00%	15.333%
8	9.775	1302	1307	1318	rBV	1010730	908721	24.28%	3.724%
9	10.575	1438	1443	1471	rBV	2333972	2435370	65.08%	9.979%
10	11.269	1558	1561	1571	rBV	1132605	991107	26.49%	4.061%
11	12.869	1828	1833	1836	rBV	3519301	3728998	99.65%	15.280%
12	13.933	2010	2014	2022	rBV	754229	704568	18.83%	2.887%
13	15.404	2259	2264	2273	rBV	385291	567794	15.17%	2.327%




Sum of corrected areas: 24405005

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135683.D
Acq On : 10 Oct 2023 14:21
Operator : CG\JU
Sample : PB156207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

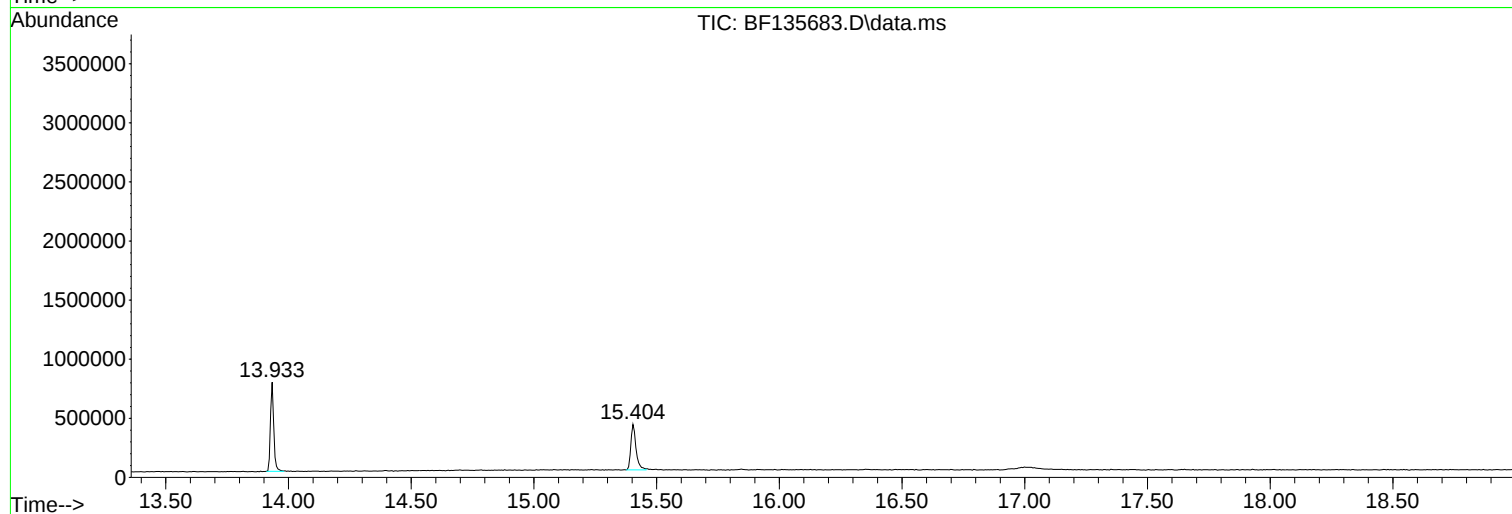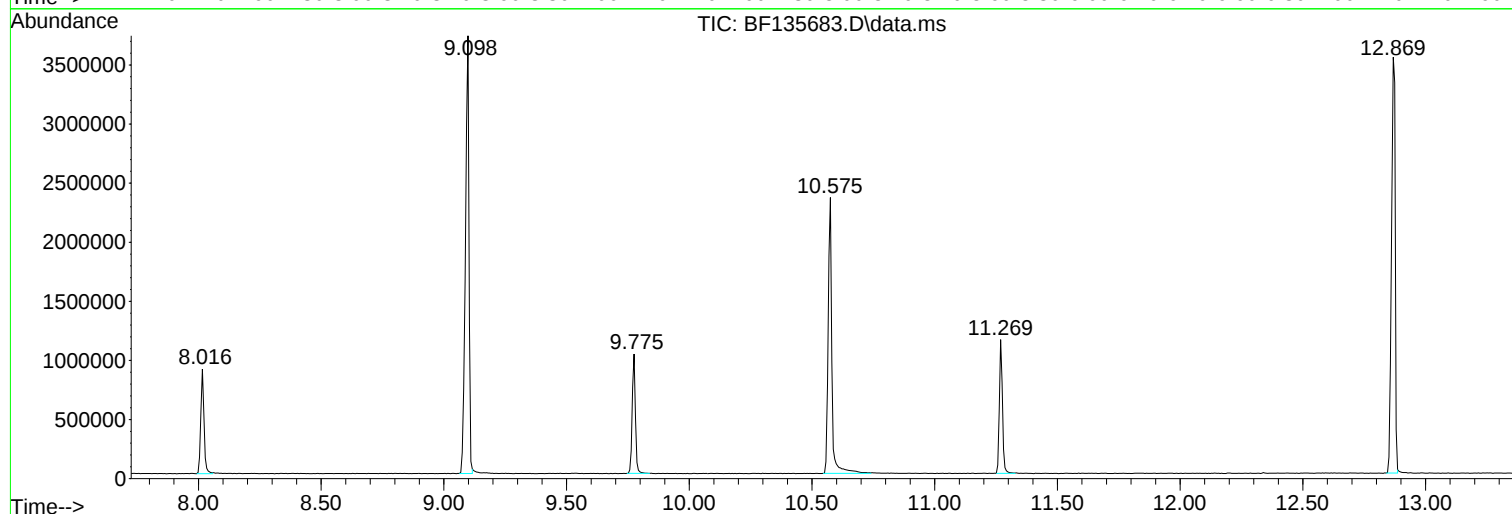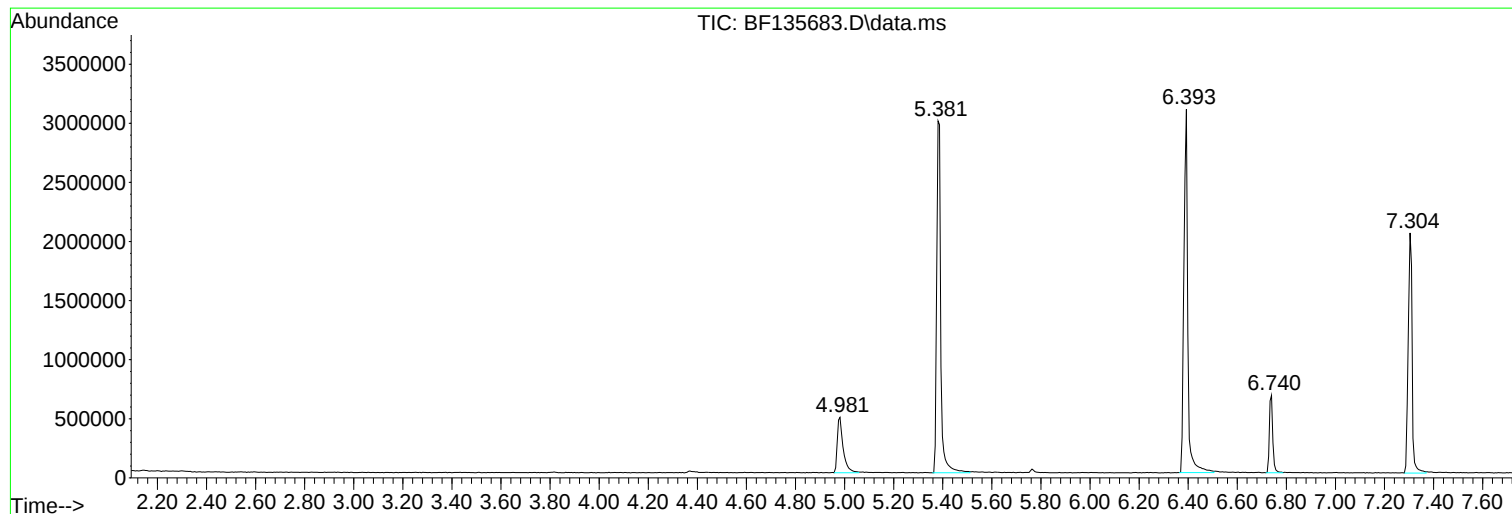

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135683.D
Acq On : 10 Oct 2023 14:21
Operator : CG\JU
Sample : PB156207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.981	24.82 ng	782293	1,4-Dichlorobenzene-d4	6.740

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	42
3			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
4			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135683.D
Acq On : 10 Oct 2023 14:21
Operator : CG\JU
Sample : PB156207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.981	24.8	ng	782293	1	6.740	630293	20.0