

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135687.D
Acq On : 10 Oct 2023 16:25
Operator : CG\JU
Sample : PB155881BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155881BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	578	rBV	3099641	3177926	91.16%	14.707%
2	6.393	728	732	756	rBV	2861046	3202982	91.88%	14.823%
3	6.740	787	791	804	rBV	617182	576186	16.53%	2.666%
4	7.304	883	887	898	rBV	1971764	2096330	60.14%	9.701%
5	8.016	1004	1008	1023	rBV	814104	753141	21.60%	3.485%
6	9.098	1186	1192	1195	rBV	3521091	3485977	100.00%	16.132%
7	9.775	1302	1307	1316	rVB	909246	823474	23.62%	3.811%
8	10.575	1438	1443	1455	rBV	2000965	2107814	60.47%	9.755%
9	11.269	1557	1561	1571	rBV	998736	901542	25.86%	4.172%
10	12.869	1828	1833	1836	rBV	3292656	3374996	96.82%	15.619%
11	13.933	2010	2014	2023	rBV	596649	584858	16.78%	2.707%
12	15.404	2259	2264	2278	rBV	350290	523202	15.01%	2.421%




Sum of corrected areas: 21608428

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135687.D
Acq On : 10 Oct 2023 16:25
Operator : CG\JU
Sample : PB155881BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155881BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

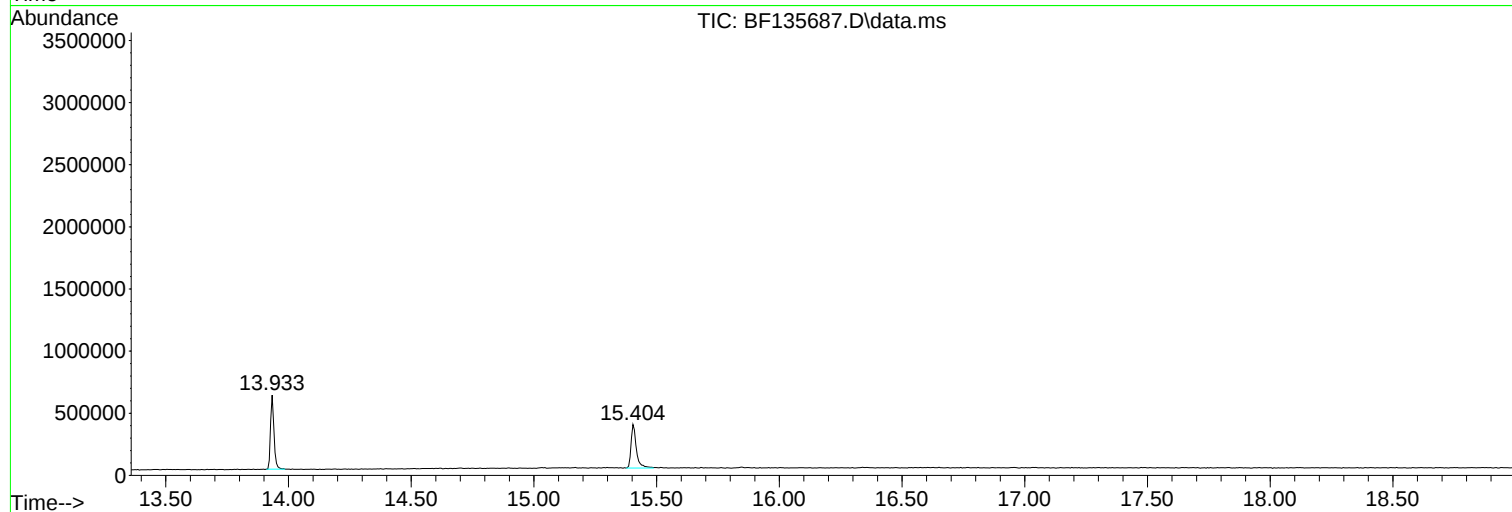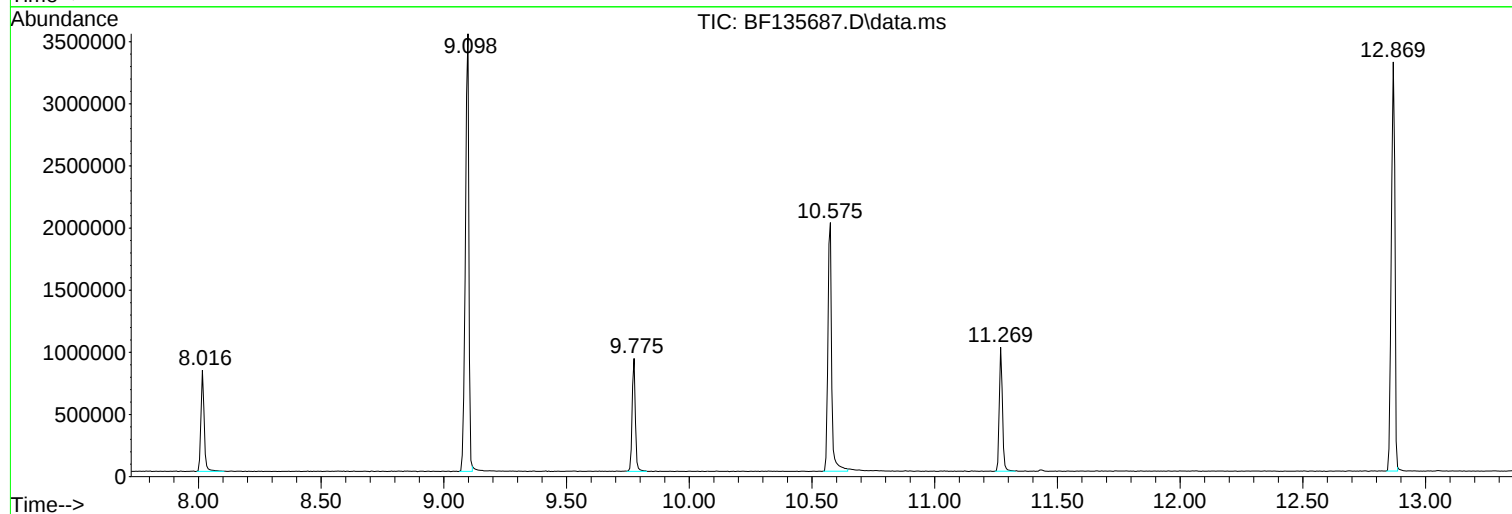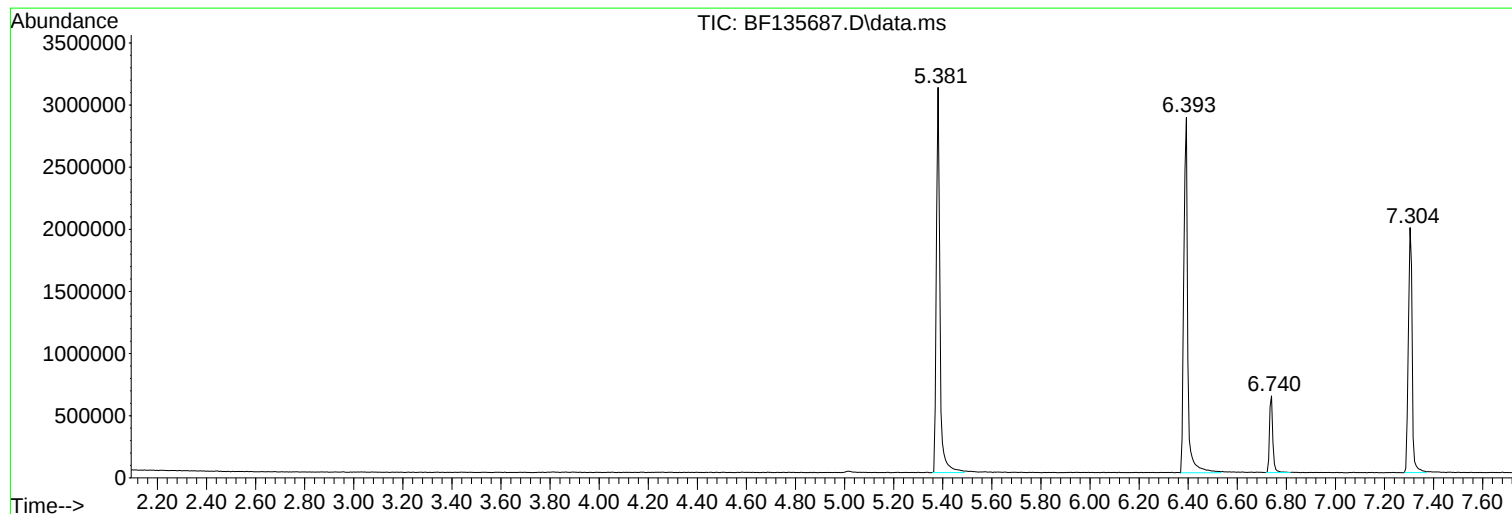

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135687.D
Acq On : 10 Oct 2023 16:25
Operator : CG\JU
Sample : PB155881BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155881BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135687.D
Acq On : 10 Oct 2023 16:25
Operator : CG\JU
Sample : PB155881BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155881BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------