
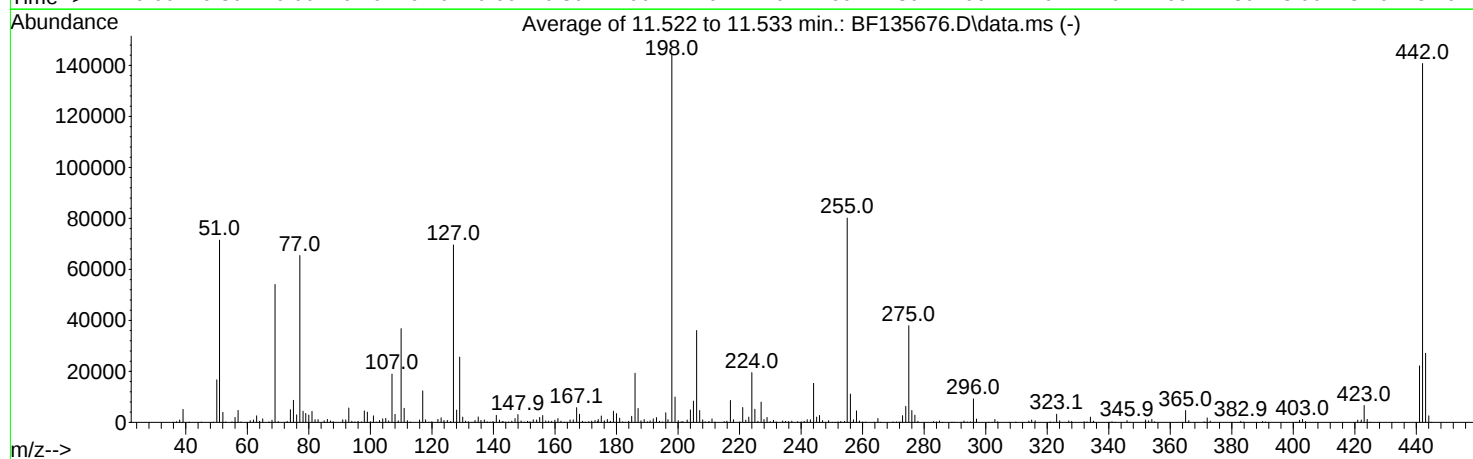


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135676.D
Acq On : 10 Oct 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 11 02:43:17 2023

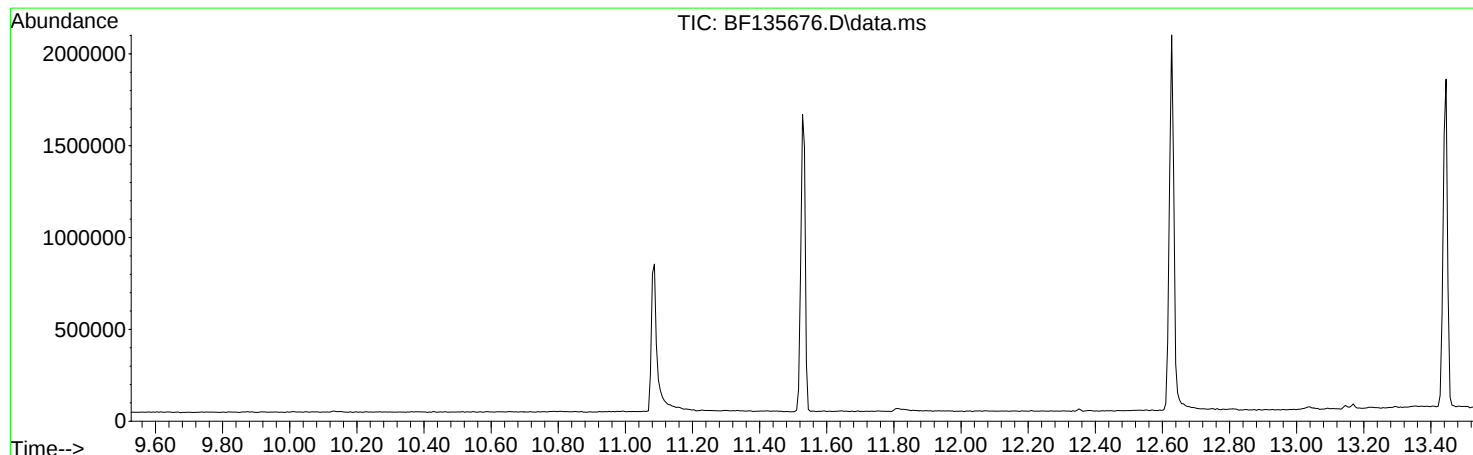




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	71502	PASS
68	69	0.00	2	1.7	907	PASS
69	198	0.00	100	37.5	54107	PASS
70	69	0.00	2	0.6	311	PASS
127	198	10	80	48.3	69624	PASS
197	198	0.00	2	0.8	1087	PASS
198	198	100	100	100.0	144283	PASS
199	198	5	9	6.9	9925	PASS
275	198	10	60	26.3	37896	PASS
365	198	1	100	3.2	4645	PASS
441	198	0.01	100	15.4	22151	PASS
442	442	50	100	100.0	140757	PASS
443	442	15	24	19.3	27144	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135676.D
Acq On : 10 Oct 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 11:42:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

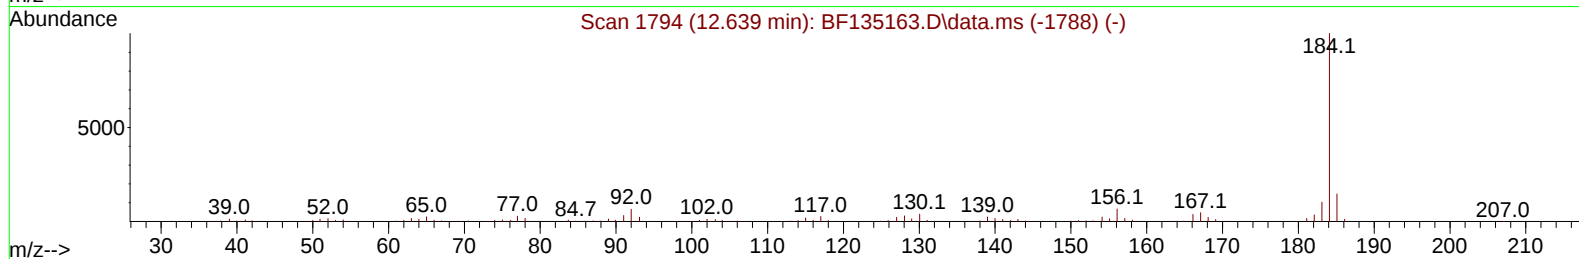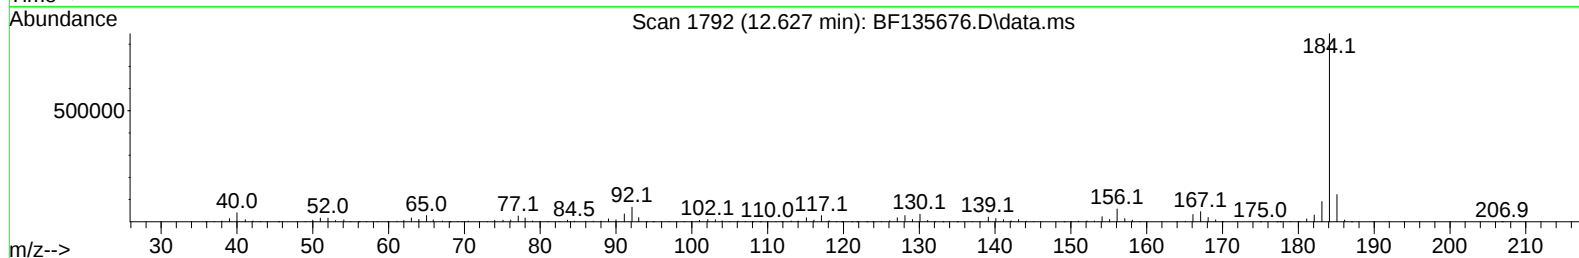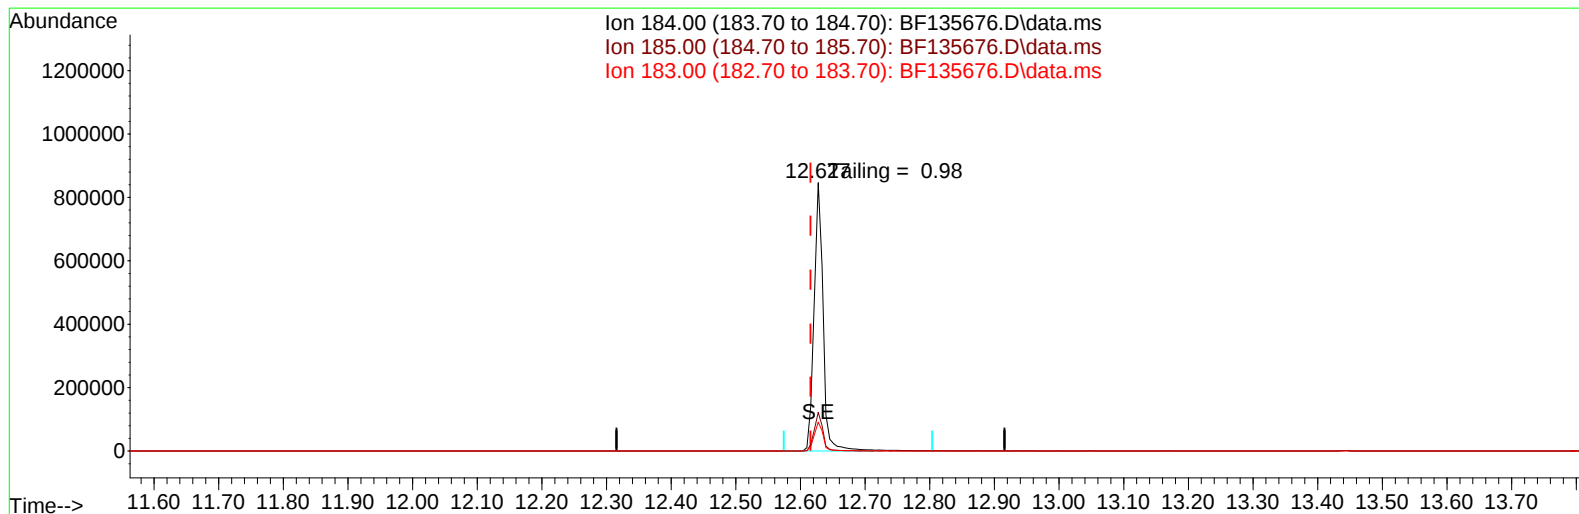

TIC: BF135676.D\data.ms

(77) Benzidine

12.627min (+ 0.012) 305572.76 ng




response 832609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.45
183.00	10.30	10.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135676.D
Acq On : 10 Oct 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 11:42:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

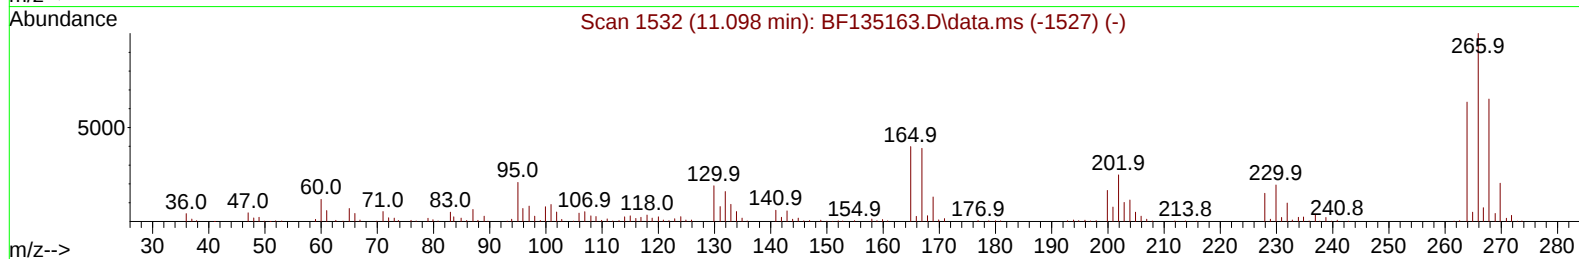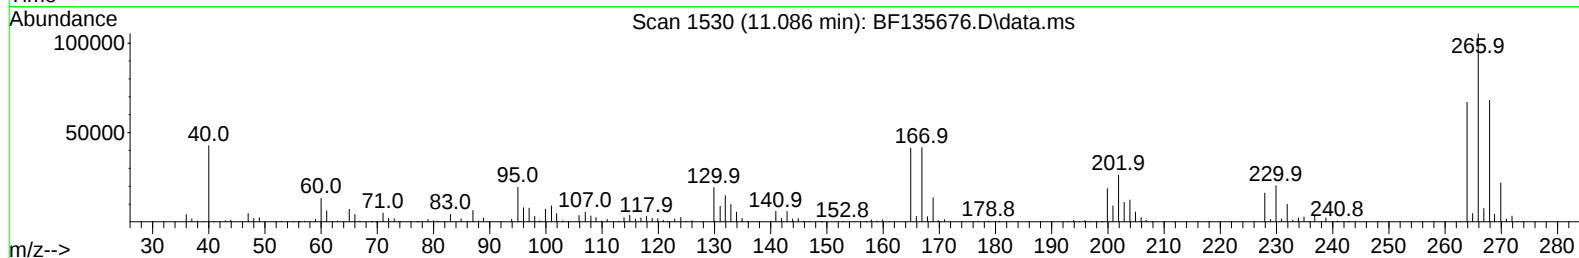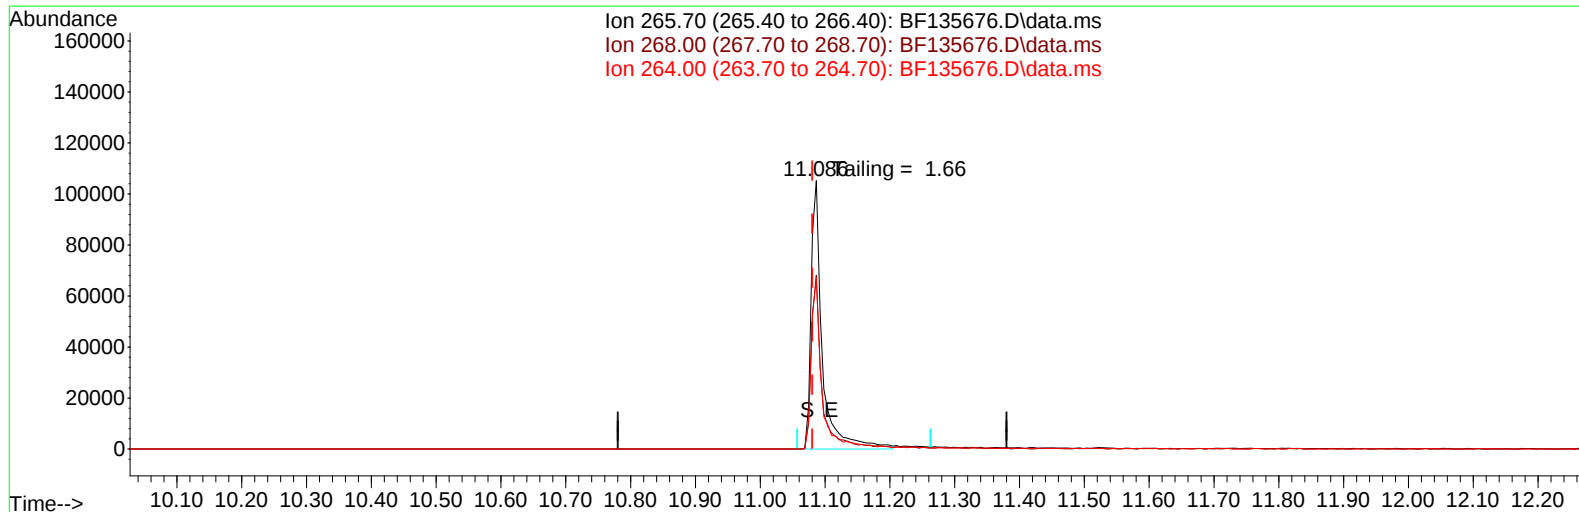

TIC: BF135676.D\data.ms

(70) Pentachlorophenol (C)

11.086min (+ 0.006) 28896.51 ng

response 130682

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.68
264.00	63.50	63.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2023	BNA_F	<u>BF135676.D</u>
Compound Name	Response	Retention Time
DDT	328095	13.445
DDD	7424	13.169
DDE	226	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7650	335745	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP