
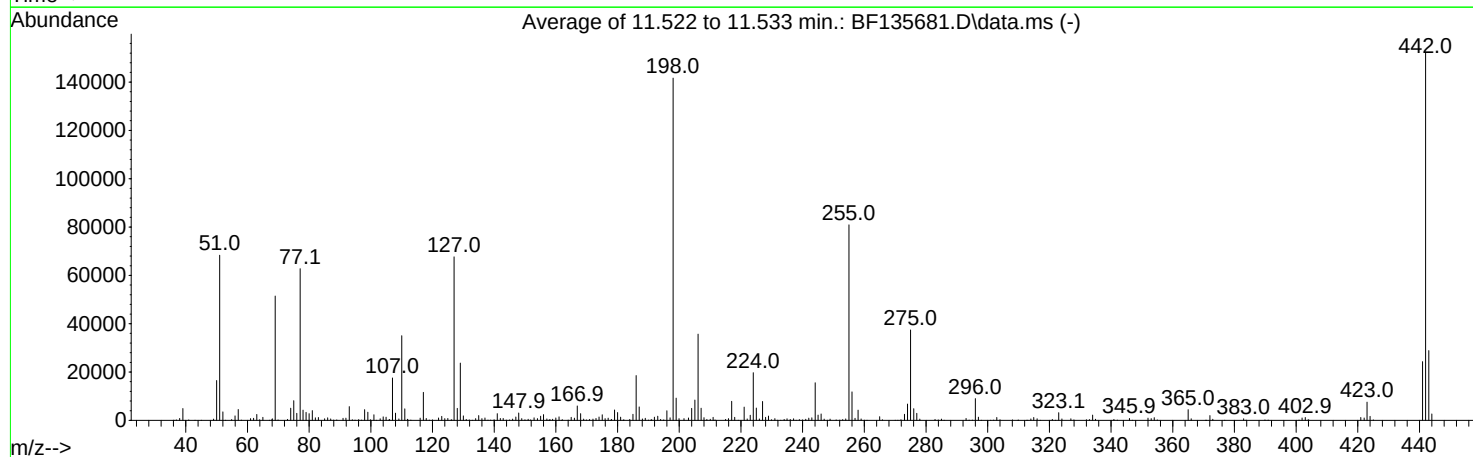


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
 Data File : BF135681.D
 Acq On : 10 Oct 2023 12:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 02:43:17 2023

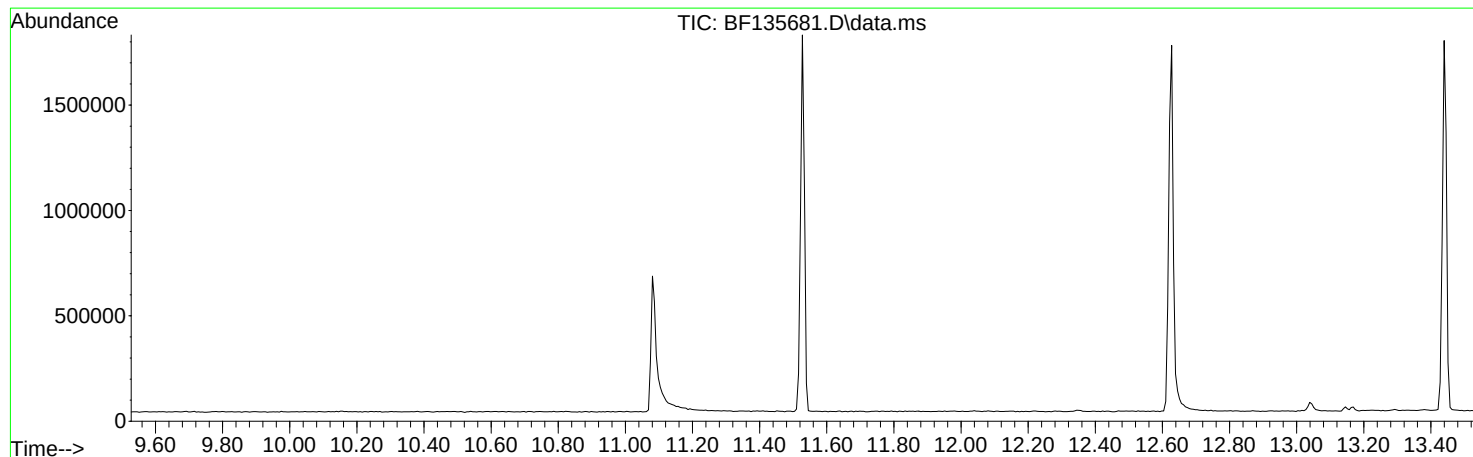




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	68336	PASS
68	69	0.00	2	1.3	648	PASS
69	198	0.00	100	36.3	51483	PASS
70	69	0.00	2	0.4	221	PASS
127	198	10	80	47.8	67648	PASS
197	198	0.00	2	0.7	1045	PASS
198	198	100	100	100.0	141659	PASS
199	198	5	9	6.5	9188	PASS
275	198	10	60	26.4	37411	PASS
365	198	1	100	3.1	4452	PASS
441	198	0.01	100	17.2	24309	PASS
442	442	50	100	100.0	152240	PASS
443	442	15	24	19.0	28894	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
Data File : BF135681.D
Acq On : 10 Oct 2023 12:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 13:19:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

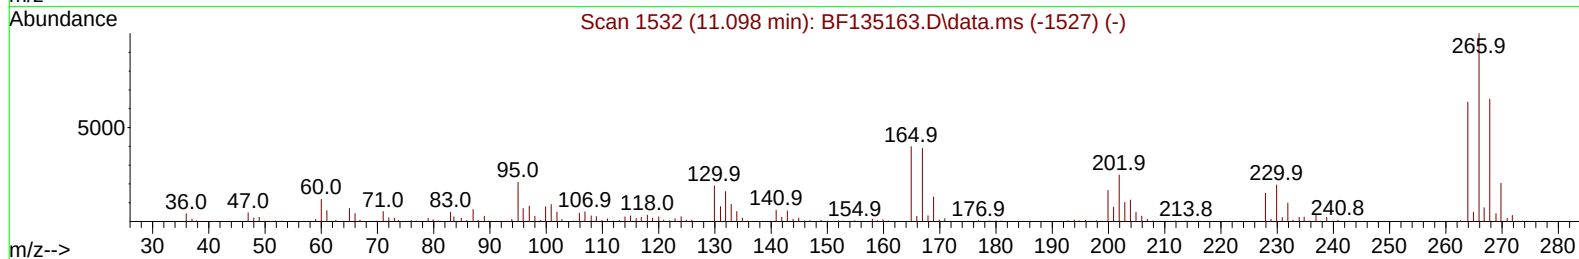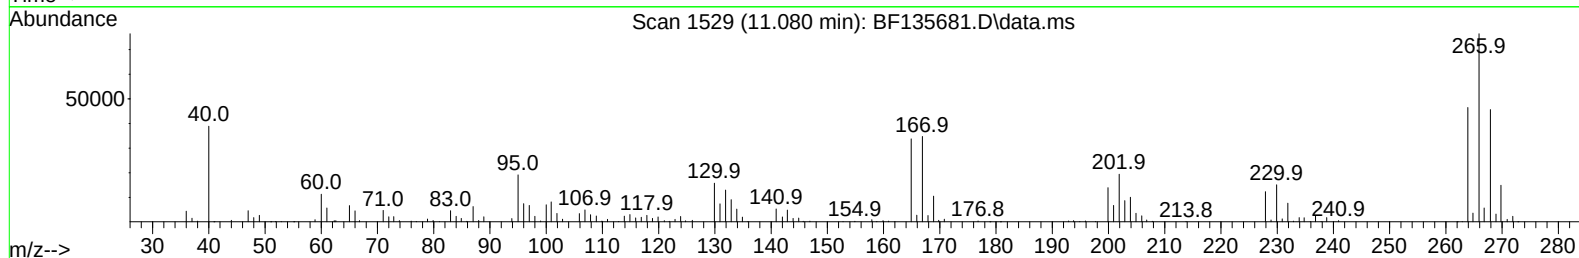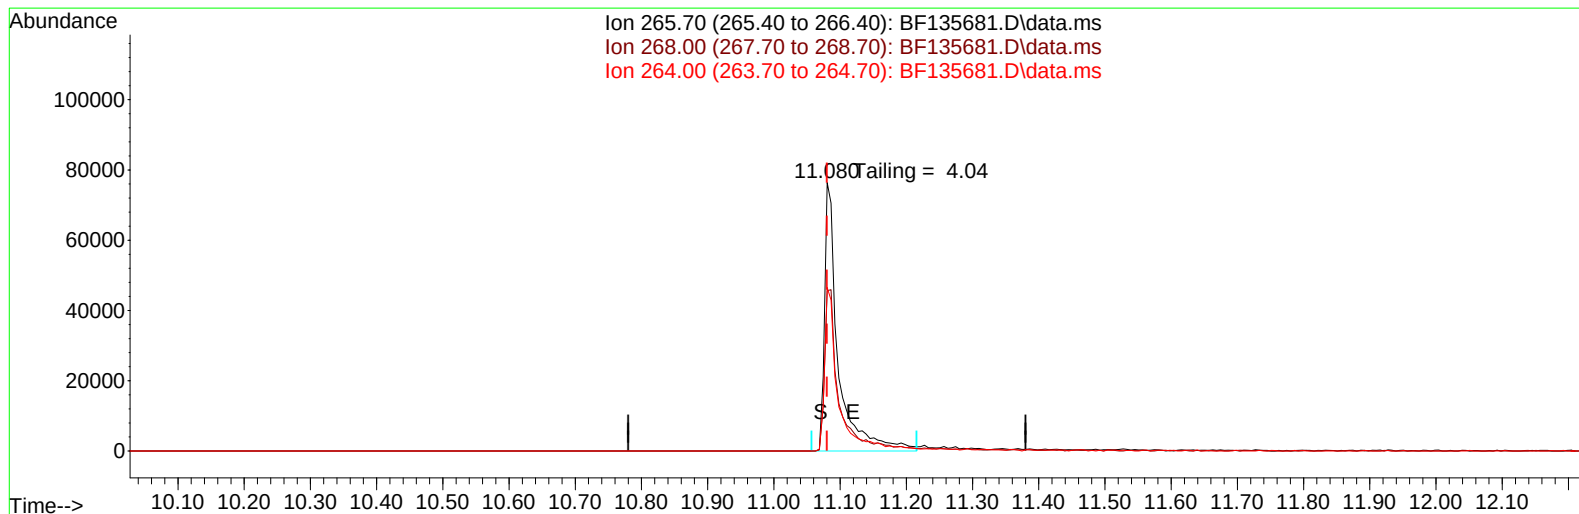

TIC: BF135681.D\data.ms

(70) Pentachlorophenol (C)

11.080min (+ 0.000) 28791.73 ng




response 110834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	59.74
264.00	63.50	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101023\
 Data File : BF135681.D
 Acq On : 10 Oct 2023 12:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 10 13:19:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 04 17:06:20 2023
 Response via : Initial Calibration

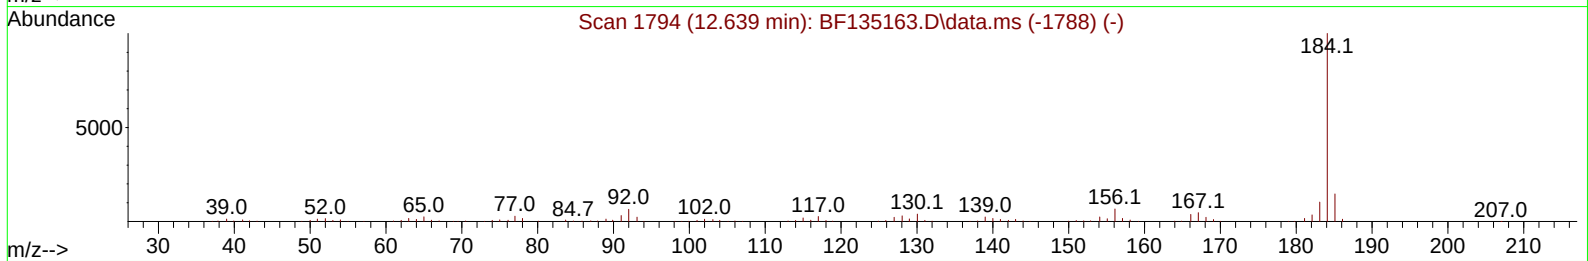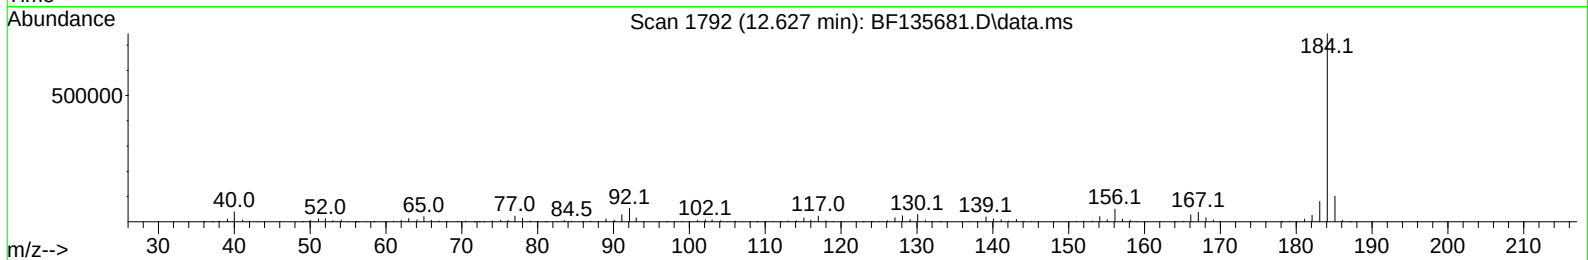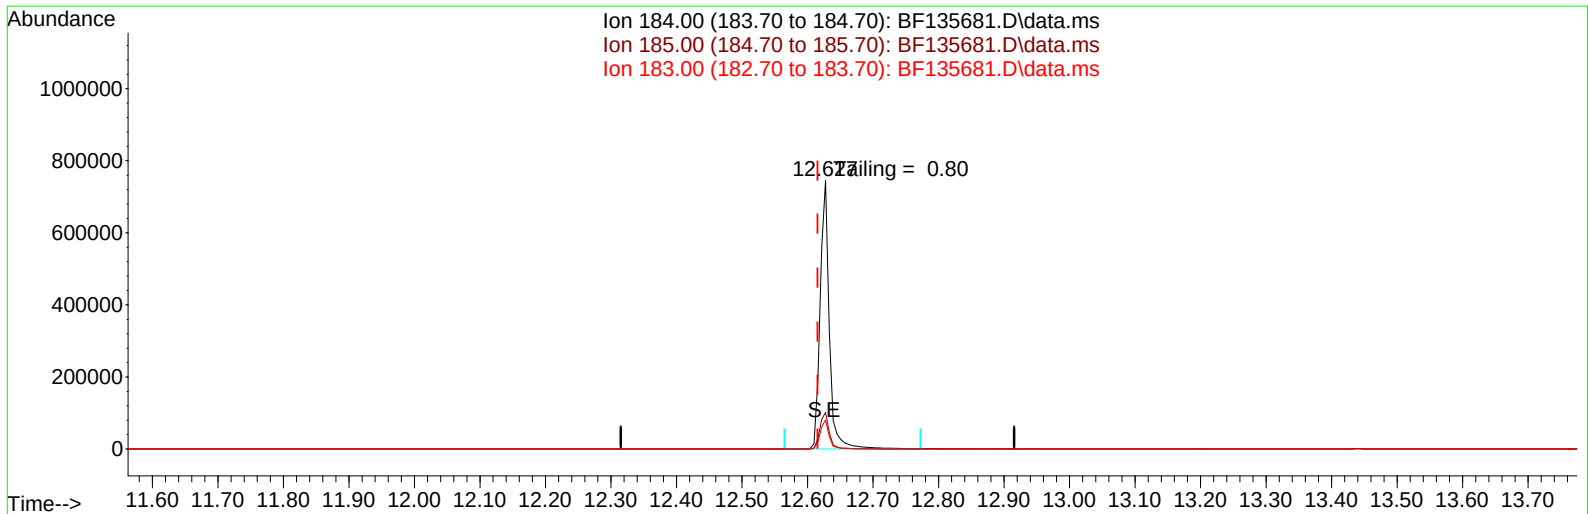

TIC: BF135681.D\data.ms

(77) Benzidine

12.627min (+ 0.012) 0.00 ng m

response 729928

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.66
183.00	10.30	10.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2023	BNA_F	<u>BF135681.D</u>
Compound Name	Response	Retention Time
DDT	309158	13.449
DDD	7897	13.145
DDE	239	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8136	317294	2.56

Instrument :
BNA_F
ClientSampleId :
DFTPP