
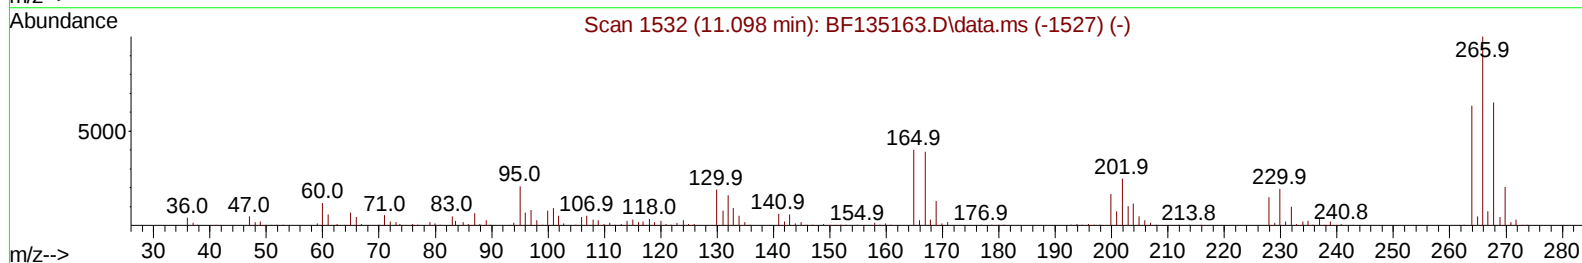
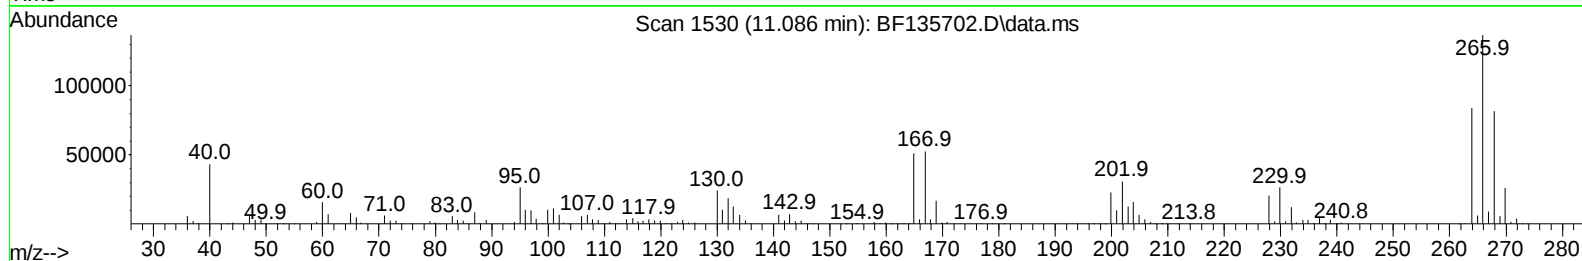


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135702.D
Acq On : 11 Oct 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 20:38:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

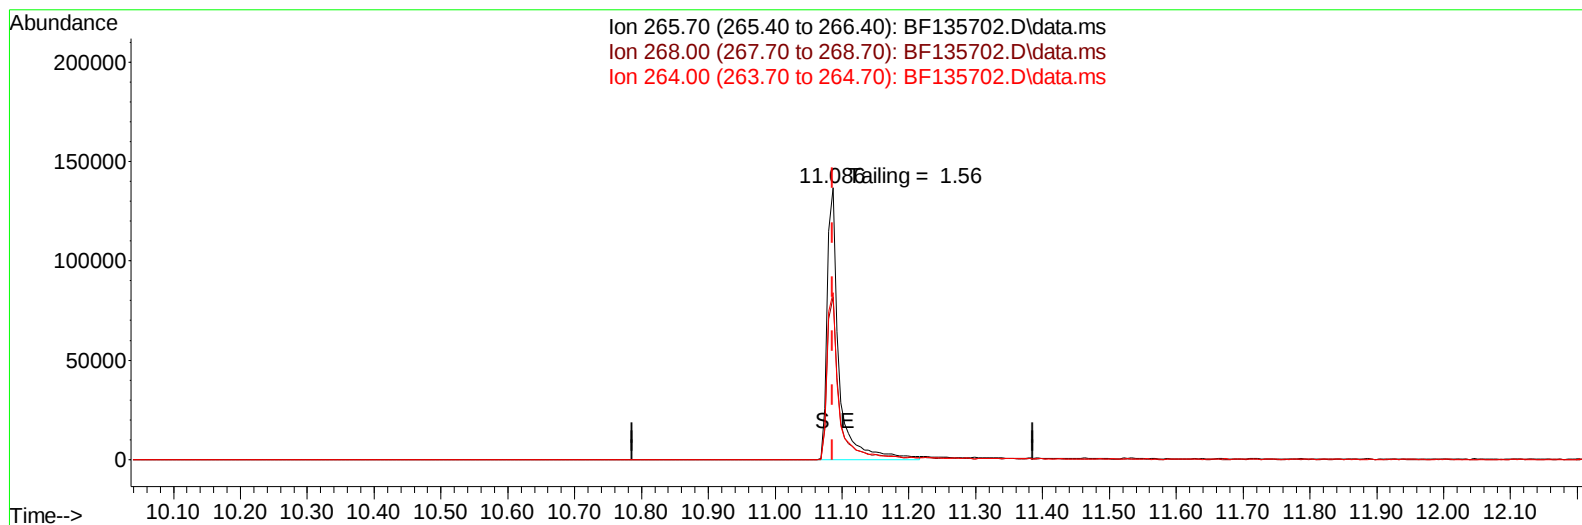




TIC: BF135702.D\data.ms

(70) Pentachlorophenol (C)**11.086min (-0.000) 35316.14 ng****response 163782**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	59.74
264.00	63.50	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135702.D
Acq On : 11 Oct 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 05:44:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

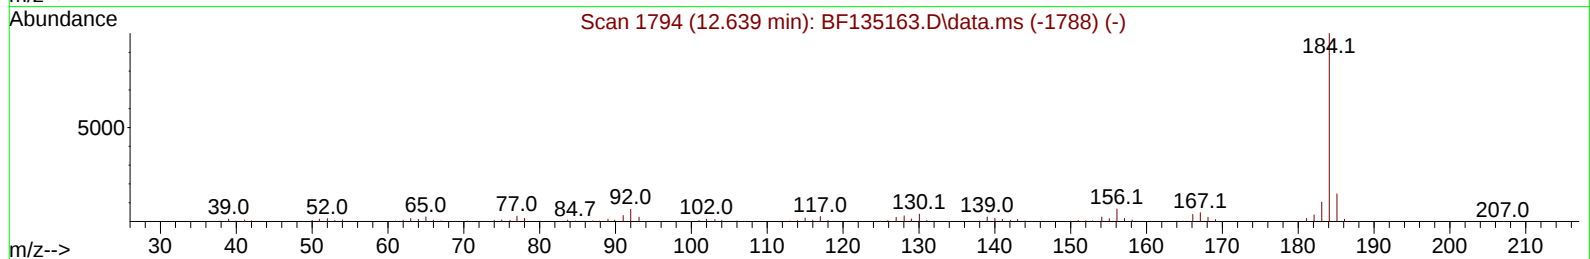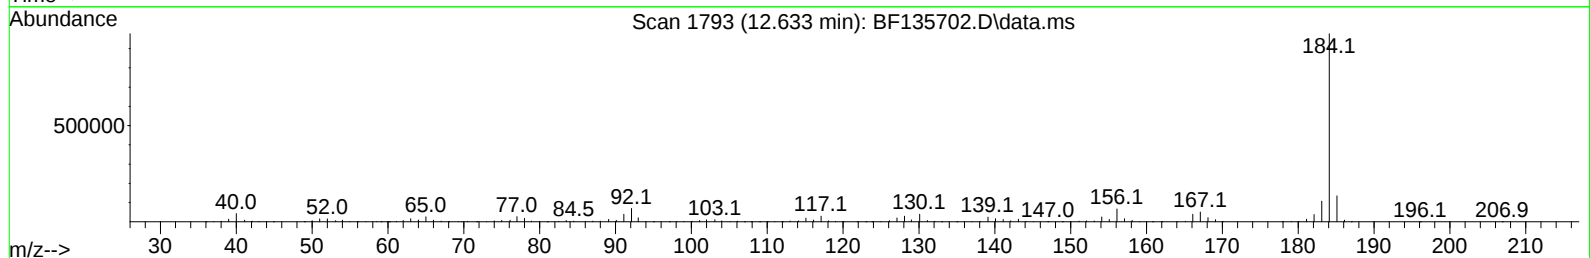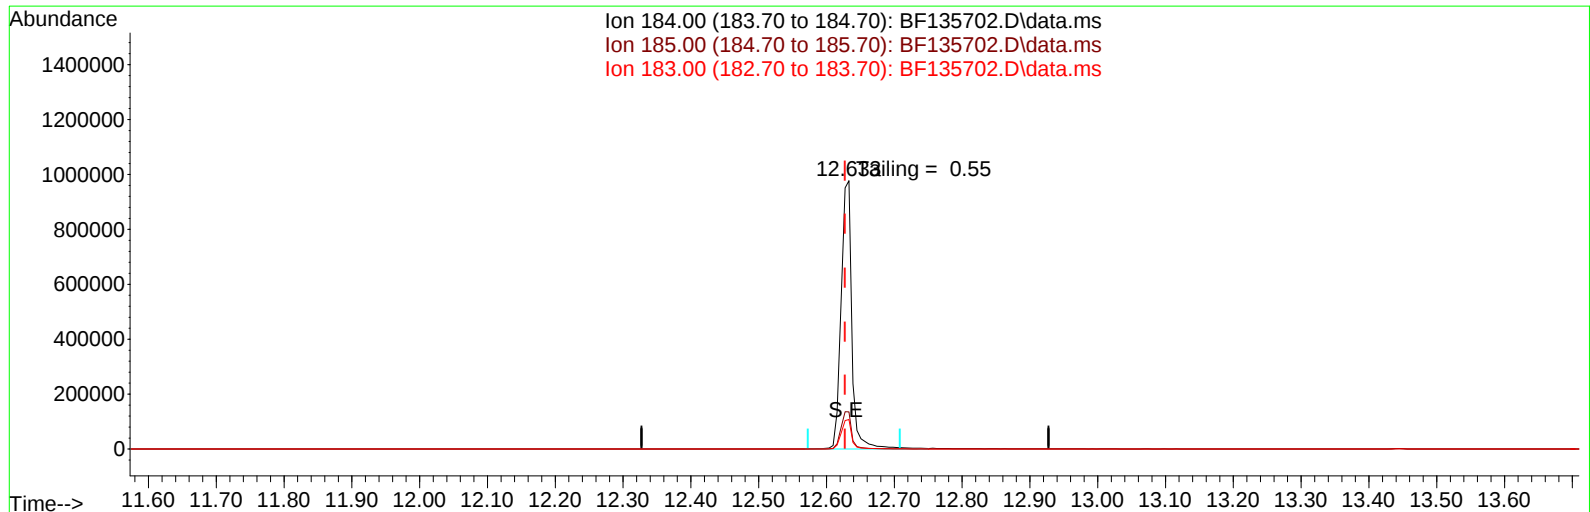

TIC: BF135702.D\data.ms

(77) Benzidine

12.633min (+ 0.006) 308718.61 ng m

response 1081518

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	10.30	11.01
0.00	0.00	0.00