

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
 Data File : BF135704.D
 Acq On : 11 Oct 2023 10:31
 Operator : CG\JU
 Sample : PB156020BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156020BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	557	560	586	rBV	3068142	3512253	89.15%	14.779%
2	6.392	728	732	752	rBV	3112049	3428450	87.03%	14.426%
3	6.739	787	791	797	rBV	673827	598448	15.19%	2.518%
4	7.310	883	888	901	rBV	1962442	2247255	57.04%	9.456%
5	8.016	1004	1008	1015	rBV	889391	812515	20.62%	3.419%
6	9.098	1186	1192	1195	rBV	3729923	3788975	96.18%	15.943%
7	9.775	1303	1307	1317	rVB	1035896	903466	22.93%	3.802%
8	10.574	1439	1443	1454	rBV	2248178	2234194	56.71%	9.401%
9	11.269	1558	1561	1569	rBV	950798	939844	23.86%	3.955%
10	12.874	1828	1834	1837	rBV	3613016	3939612	100.00%	16.577%
11	13.933	2011	2014	2025	rBV	747745	769379	19.53%	3.237%
12	15.409	2260	2265	2278	rBV	389743	591070	15.00%	2.487%




Sum of corrected areas: 23765461

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135704.D
Acq On : 11 Oct 2023 10:31
Operator : CG\JU
Sample : PB156020BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156020BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

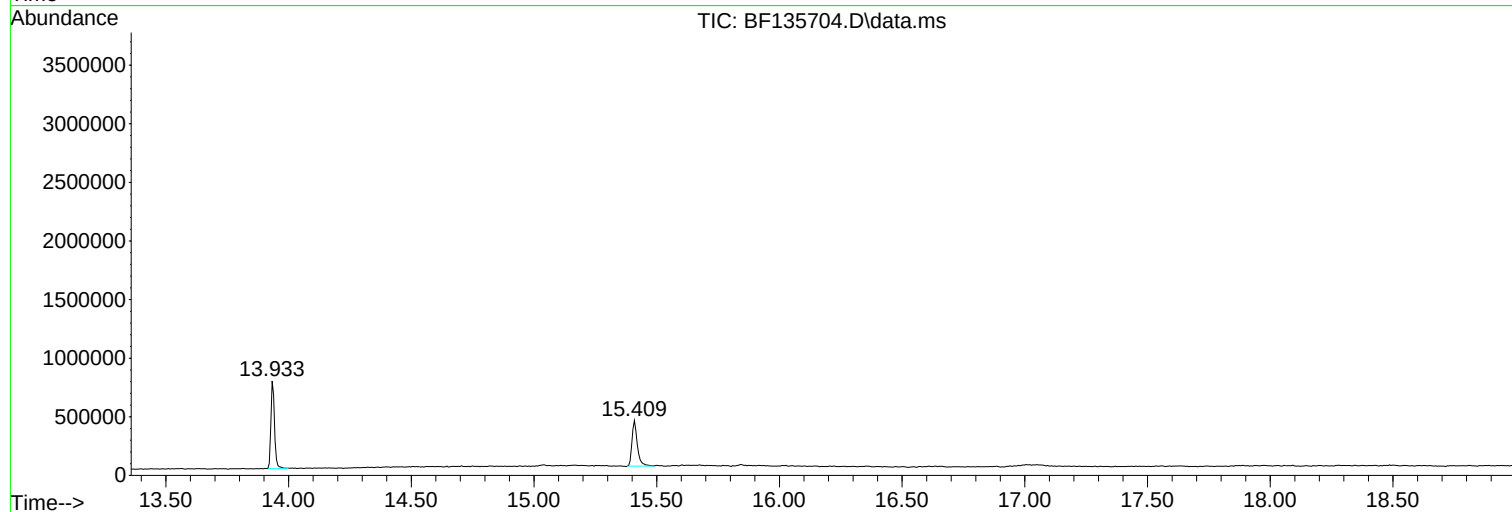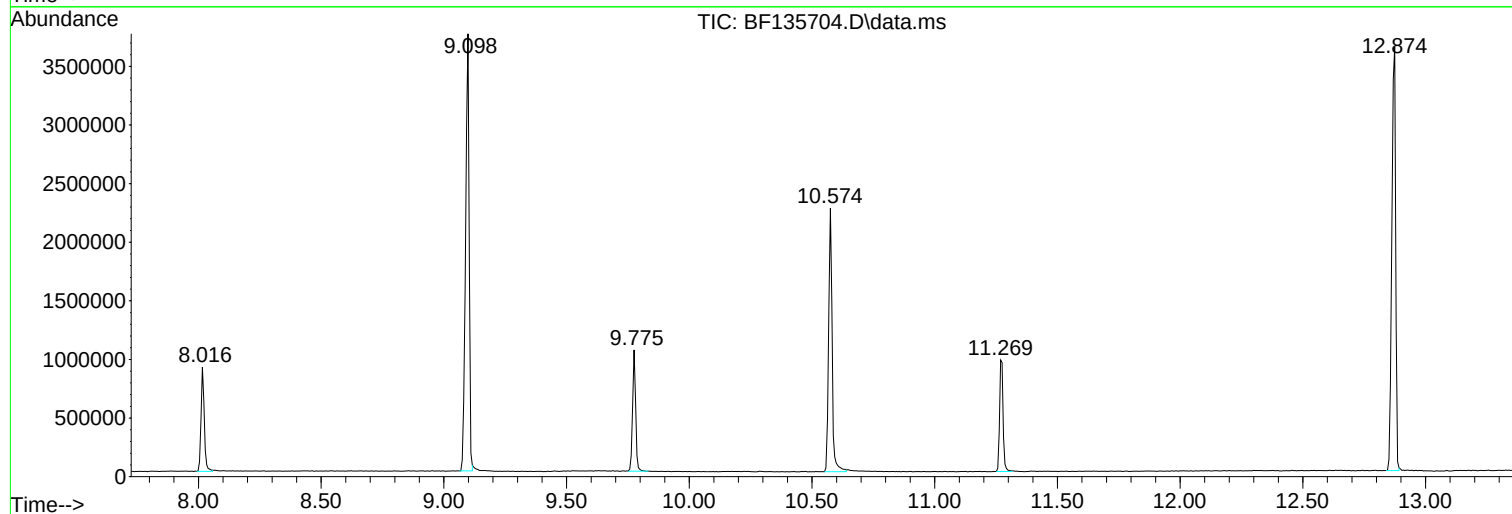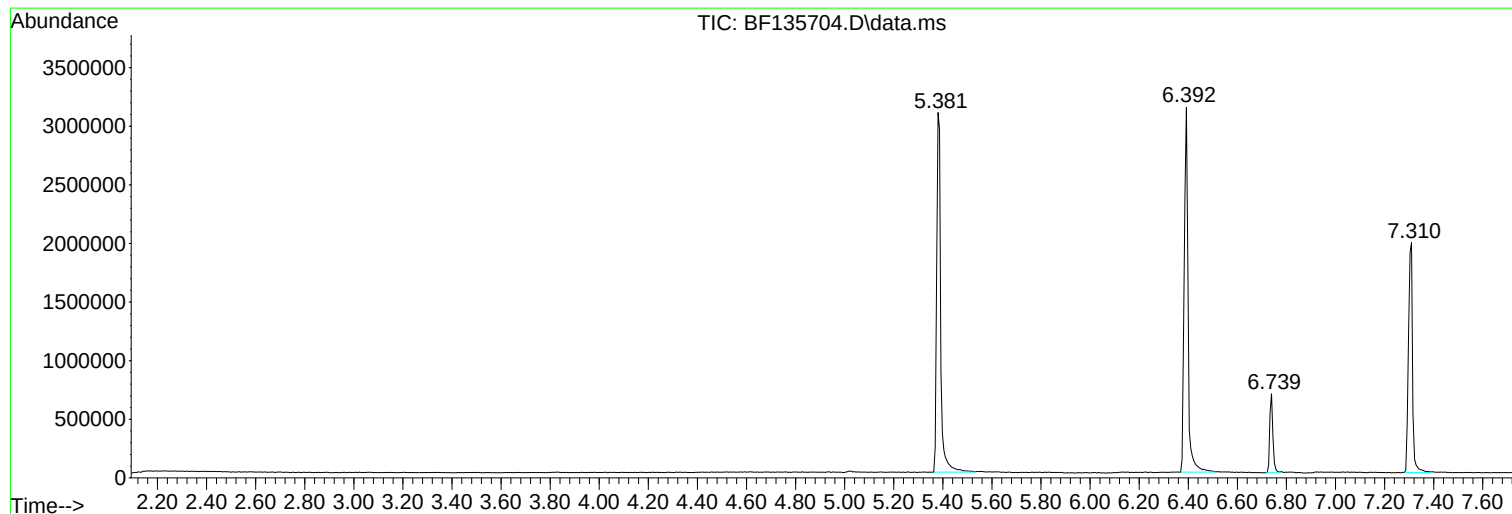

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135704.D
Acq On : 11 Oct 2023 10:31
Operator : CG\JU
Sample : PB156020BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156020BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135704.D
Acq On : 11 Oct 2023 10:31
Operator : CG\JU
Sample : PB156020BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156020BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------