


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
 Data File : BF135702.D
 Acq On : 11 Oct 2023 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 02:43:17 2023

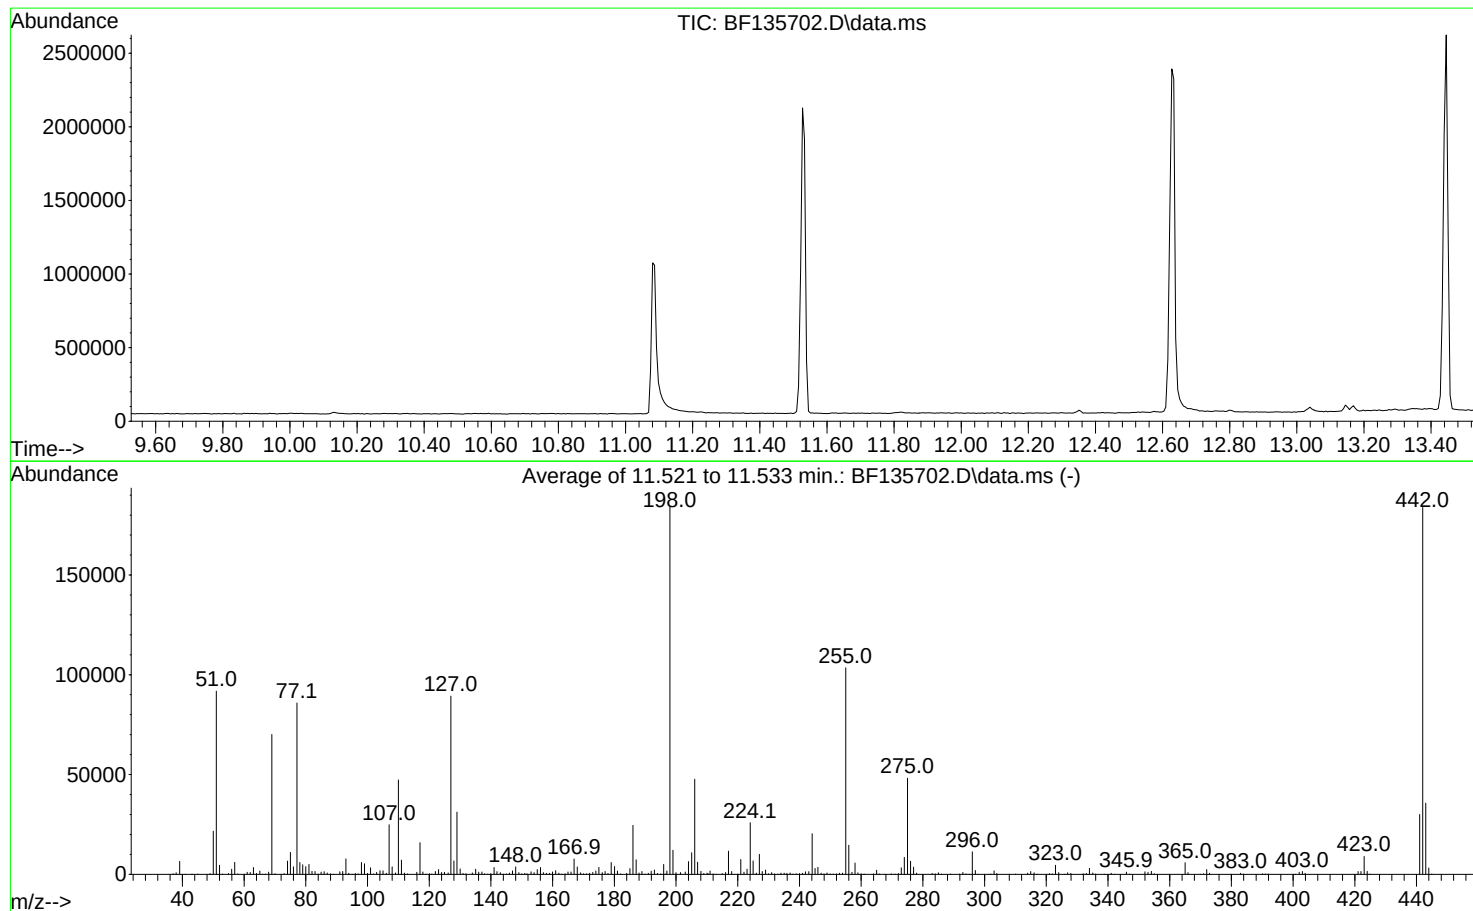




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.8	91829	PASS
68	69	0.00	2	1.6	1102	PASS
69	198	0.00	100	38.0	70037	PASS
70	69	0.00	2	0.4	295	PASS
127	198	10	80	48.5	89301	PASS
197	198	0.00	2	0.9	1676	PASS
198	198	100	100	100.0	184299	PASS
199	198	5	9	6.6	12145	PASS
275	198	10	60	26.1	48173	PASS
365	198	1	100	3.2	5838	PASS
441	198	0.01	100	16.3	30006	PASS
442	442	50	100	100.0	183843	PASS
443	442	15	24	19.4	35699	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135702.D
Acq On : 11 Oct 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 11 20:38:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

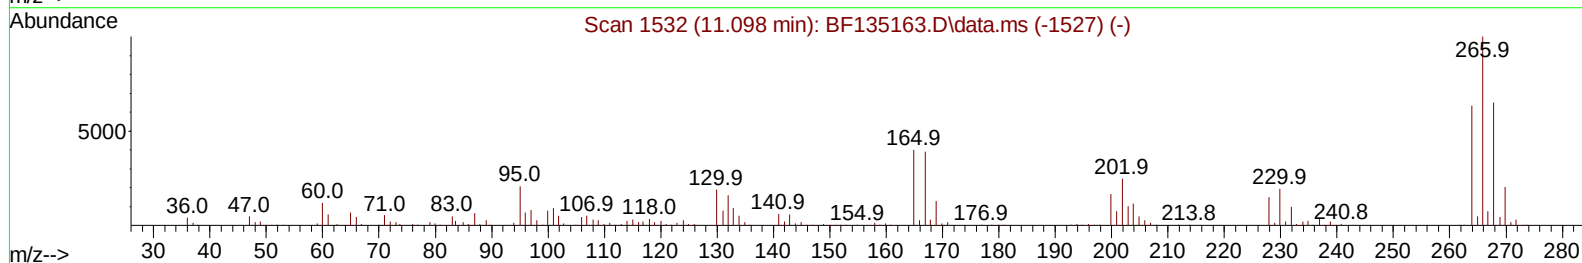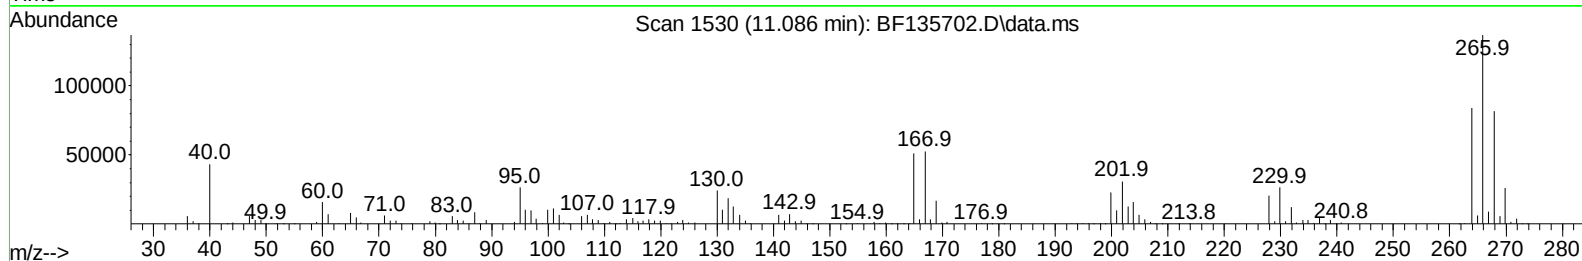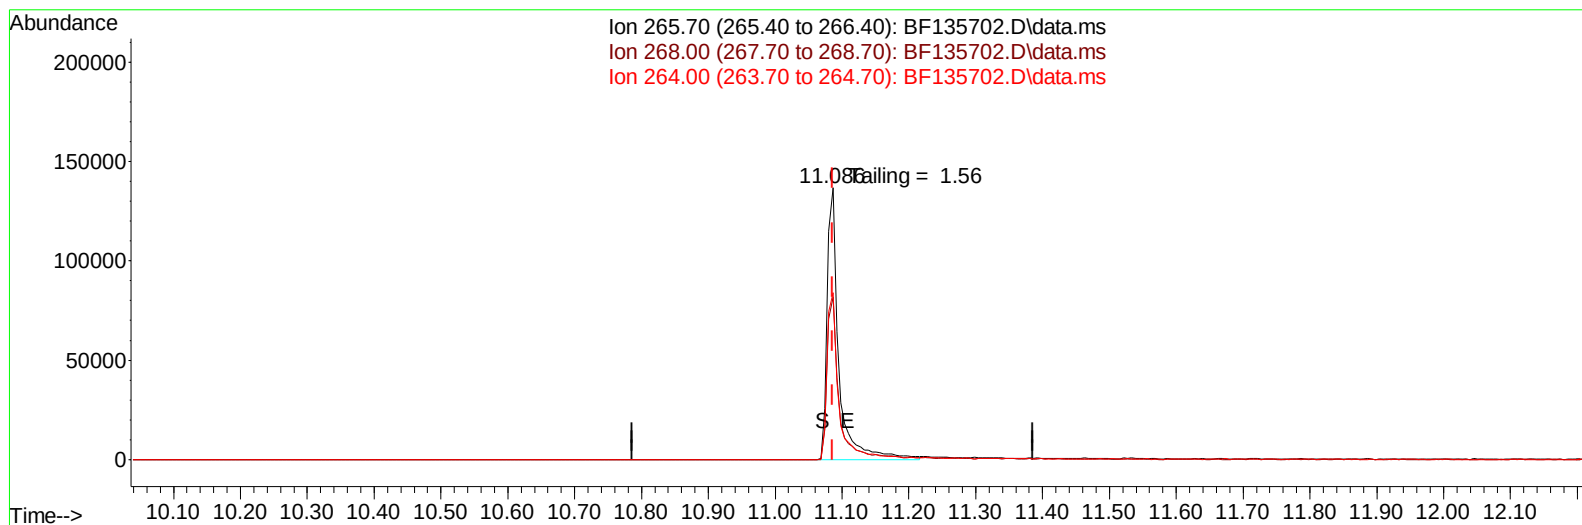

TIC: BF135702.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.000) 35316.14 ng




response 163782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	59.74
264.00	63.50	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101123\
Data File : BF135702.D
Acq On : 11 Oct 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 12 05:44:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

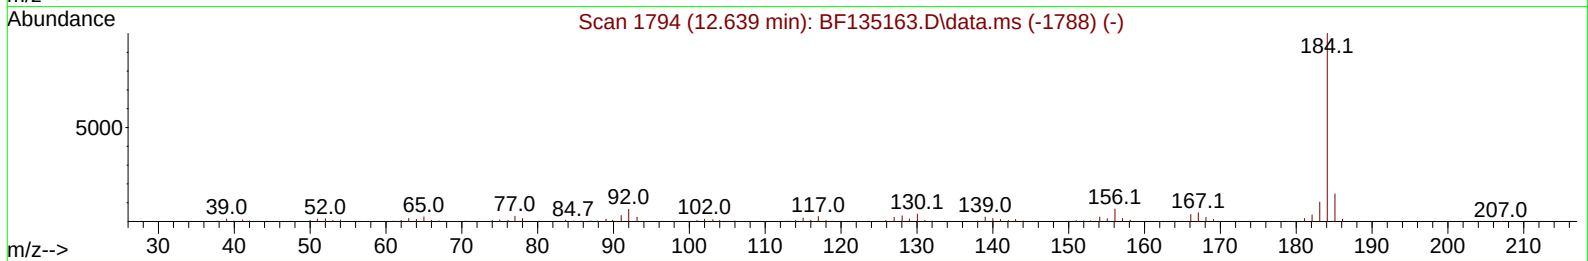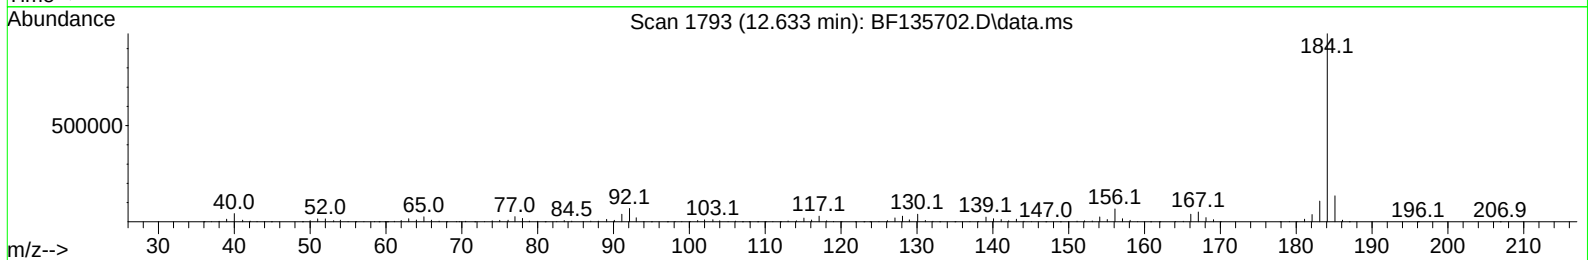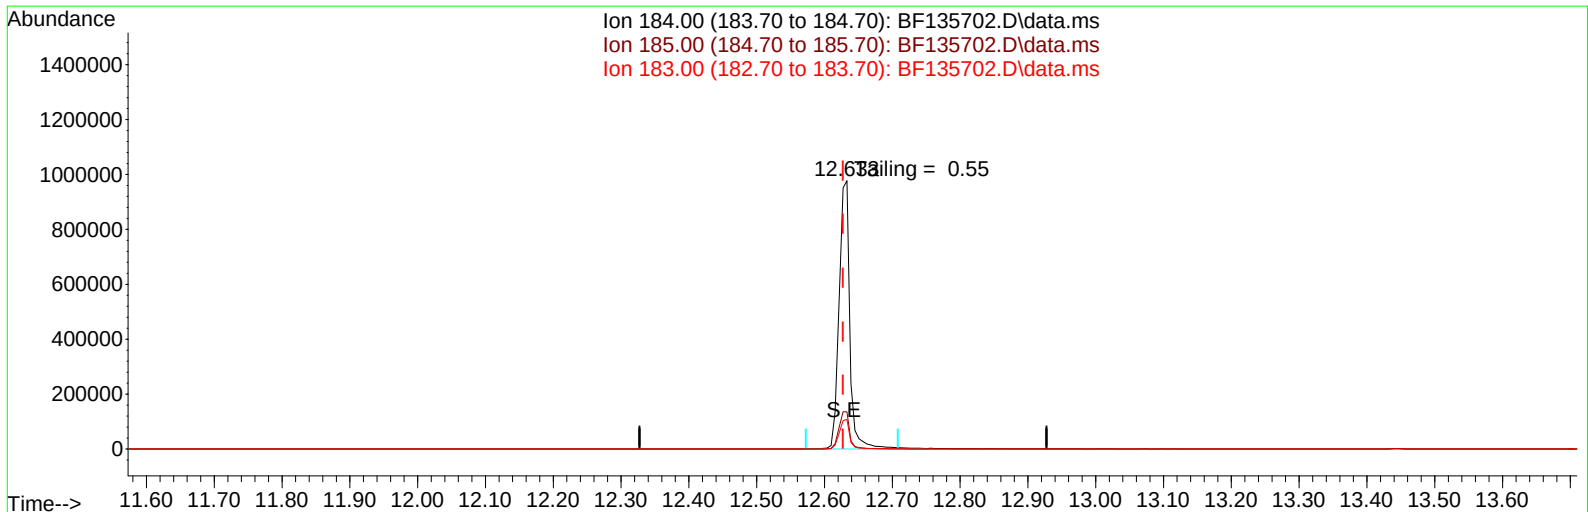

TIC: BF135702.D\data.ms

(77) Benzidine

12.633min (+ 0.006) 308718.61 ng m

response 1081518

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	10.30	11.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2023	BNA_F	<u>BF135702.D</u>
Compound Name	Response	Retention Time
DDT	462155	13.445
DDD	13142	13.145
DDE	1081	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14223	476378	2.99

Instrument :
BNA_F
ClientSampleId :
DFTPP