

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101219\
 Data File : BF117391.D
 Acq On : 13 Oct 2019 1:31
 Operator : JU
 Sample : K5323-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3

Quant Time: Oct 14 04:04:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:26:00 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	43011	20.00	ng	-0.01
21) Naphthalene-d8	8.08	136	173383	20.00	ng	0.00
39) Acenaphthene-d10	9.83	164	83692	20.00	ng	-0.01
64) Phenanthrene-d10	11.32	188	119105	20.00	ng	0.00
76) Chrysene-d12	13.96	240	88317	20.00	ng	-0.01
87) Perylene-d12	15.42	264	95917	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	271895	98.69	ng	0.00
7) Phenol-d6	6.44	99	361243	101.46	ng	-0.01
23) Nitrobenzene-d5	7.36	82	227843	69.05	ng	-0.01
42) 2,4,6-Tribromophenol	10.62	330	57428	82.10	ng	-0.01
45) 2-Fluorobiphenyl	9.15	172	352691	65.89	ng	-0.01
79) Terphenyl-d14	12.90	244	245855	52.04	ng	-0.01
Target Compounds						
10) Phenol	6.45	94	9752	2.485	ng	83
50) Dimethylphthalate	9.55	163	44403	7.493	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101219\
Data File : BF117391.D
Acq On : 13 Oct 2019 1:31
Operator : JU
Sample : K5323-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Time: Oct 14 04:04:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:26:00 2019
Response via : Initial Calibration

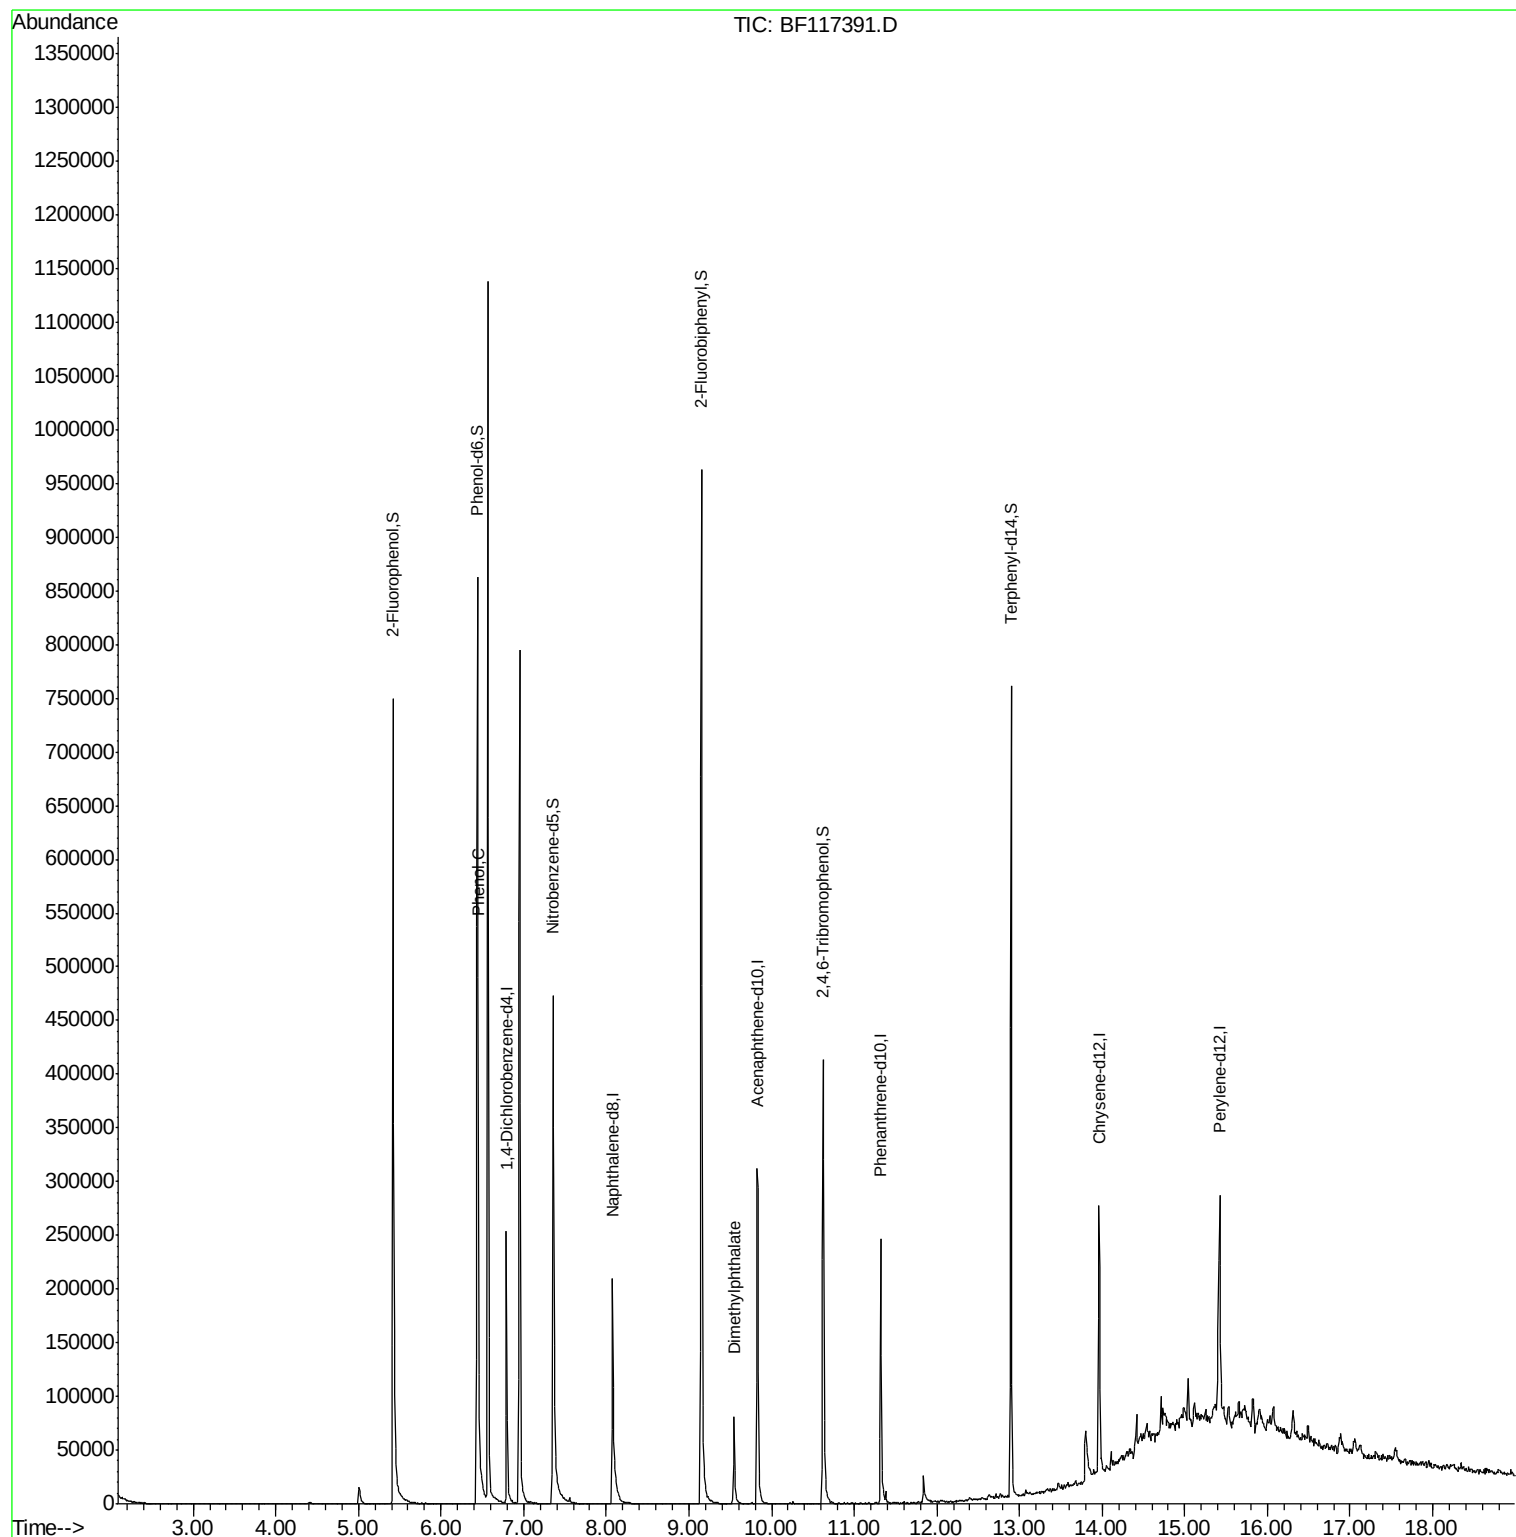

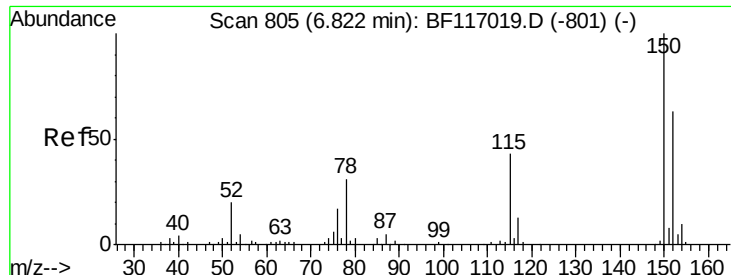


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 800
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31

Instrument :
BNA_F
ClientSampled :
TP-3

Tot Ion:152 Resp: 43011
Ion Ratio Lower Upper
152 100
150 161.1 127.5 191.3
115 68.0 55.0 82.4

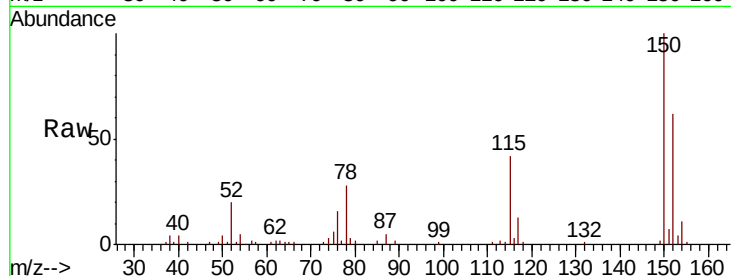


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

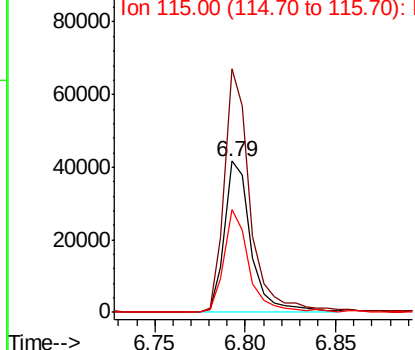



#5


2-Fluorophenol
Concen: 98.695 ng
RT: 5.42 min Scan# 567
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31

Tgt Ion:112 Resp: 271895
Ion Ratio Lower Upper
112 100
64 54.5 45.7 68.5
63 29.8 24.9 37.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

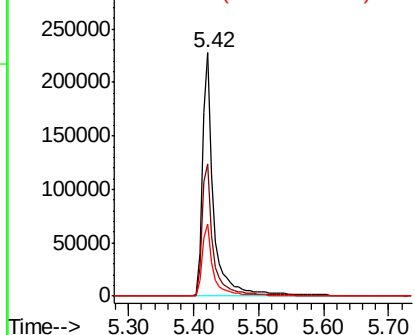

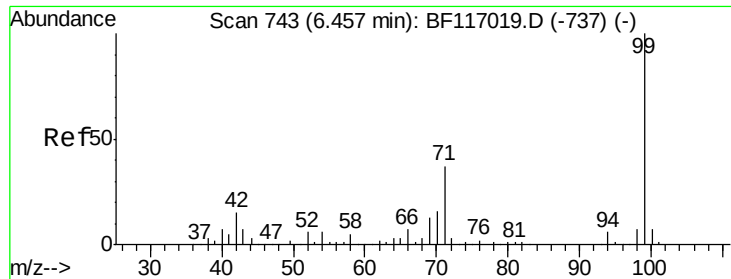

#7

Phenol-d6

Concen: 101.463 ng

RT: 6.44 min Scan# 740

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31

Instrument :

BNA_F

ClientSampleId :

TP-3


Tot Ion: 99 Resp: 361243

Ion Ratio Lower Upper




99 100

42 16.0 12.2 18.2

71 36.6 29.8 44.8

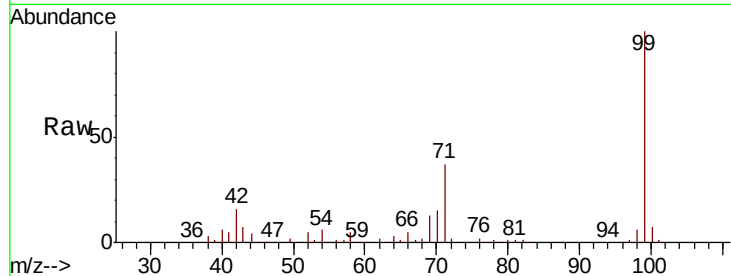

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

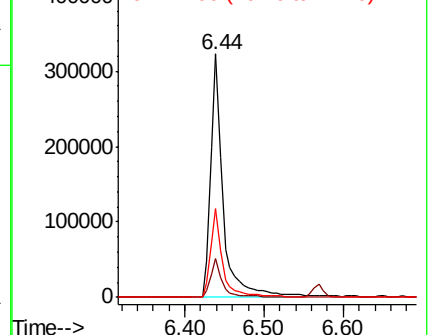

#10

Phenol

Concen: 2.485 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31


Tgt Ion: 94 Resp: 9752

Ion Ratio Lower Upper



94 100


65 32.4 12.5 52.5

66 68.6 28.9 68.9



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

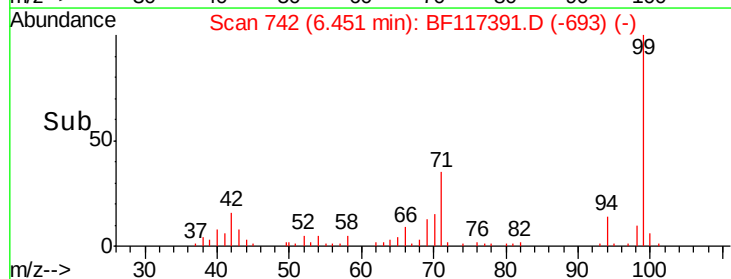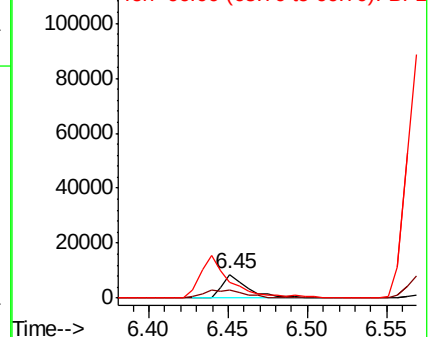

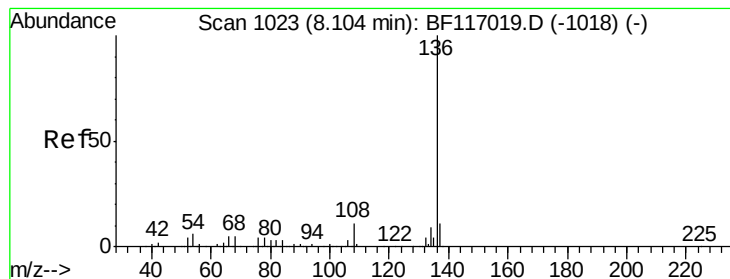

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.08 min Scan# 1019

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31

Instrument :

BNA_F

ClientSampleId :

TP-3

Tot Ion:136 Resp: 173383


Ion Ratio Lower Upper

136 100

137 10.5 9.0 13.4

54 5.2 4.5 6.7

68 4.7 4.0 6.0



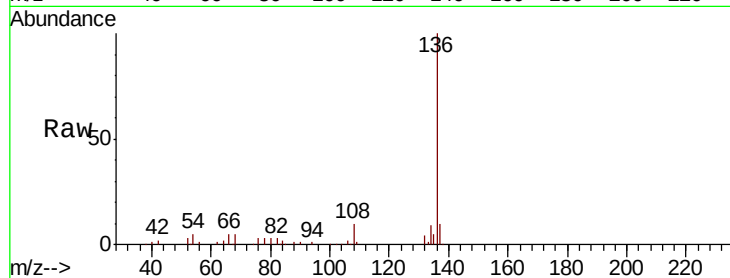


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

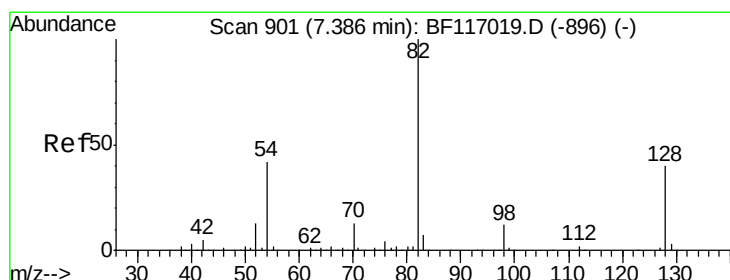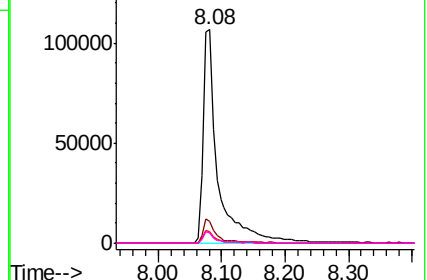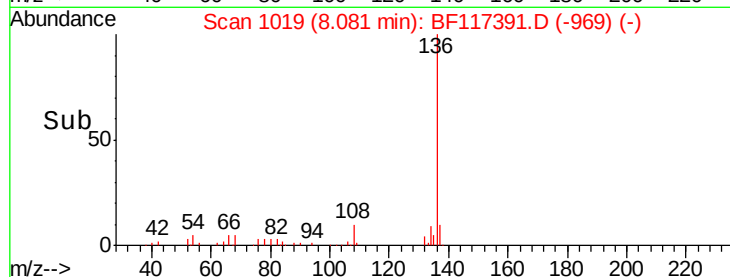

#23

Nitrobenzene-d5

Concen: 69.046 ng

RT: 7.36 min Scan# 896

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31


Tgt Ion: 82 Resp: 227843

Ion Ratio Lower Upper

82 100

128 40.1 32.3 48.5



54 42.4 33.3 49.9

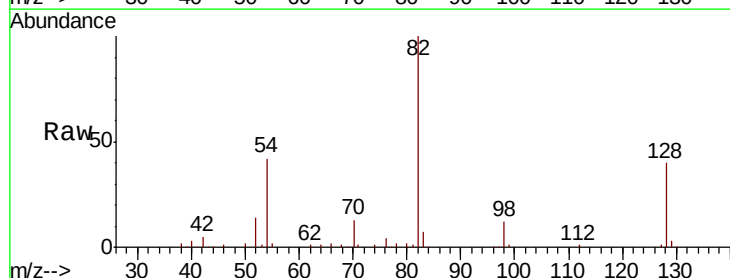


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

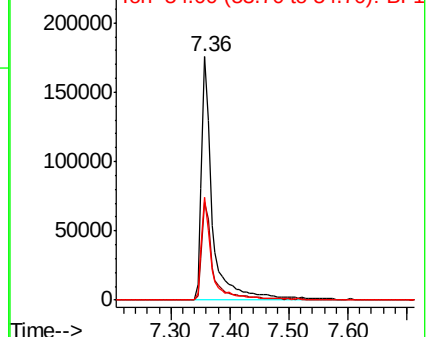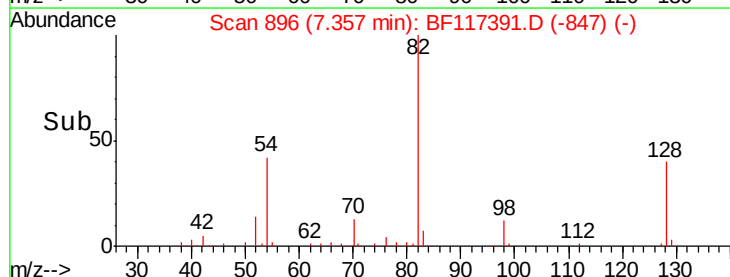



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.83 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31

Instrument :

BNA_F

ClientSampleId :

TP-3


Tot Ion:164 Resp: 83692

Ion Ratio Lower Upper

164 100

162 105.4 83.4 125.2




160 44.5 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

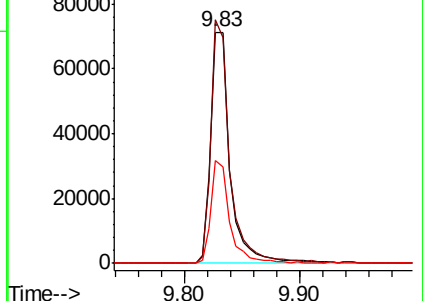

#42

2,4,6-Tribromophenol

Concen: 82.102 ng

RT: 10.62 min Scan# 1451

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31


Tgt Ion:330 Resp: 57428

Ion Ratio Lower Upper

330 100

332 93.6 78.0 117.0



141 44.5 35.8 53.6




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



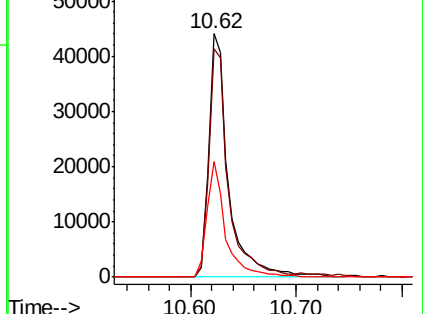



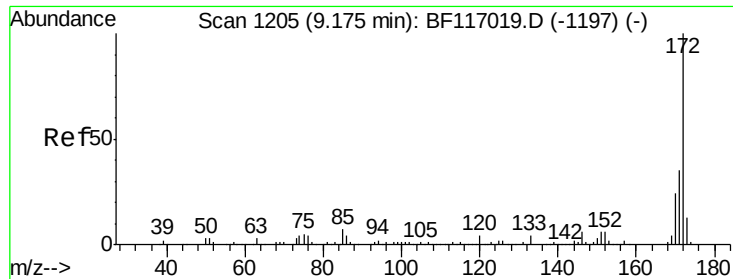

#45
2-Fluorobiphenyl
Concen: 65.891 ng
RT: 9.15 min Scan# 1201
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31




Instrument :
BNA_F
ClientSampleId :
TP-3


Tot Ion:172 Resp: 352691
Ion Ratio Lower Upper
172 100
171 35.3 28.2 42.2
170 23.1 18.9 28.3

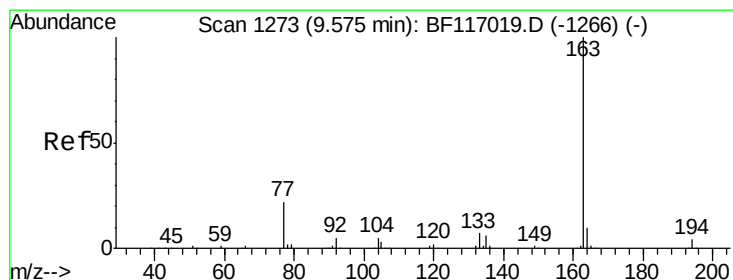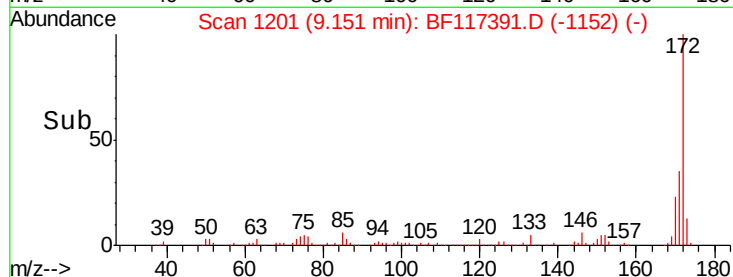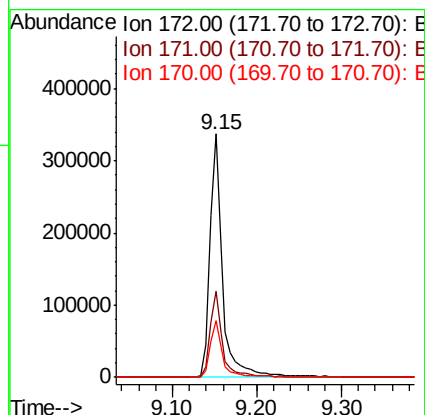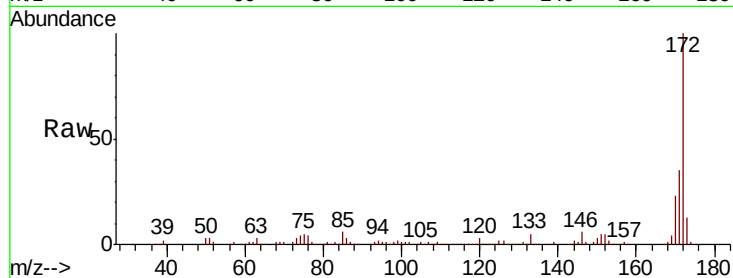

#50
Dimethylphthalate
Concen: 7.493 ng
RT: 9.55 min Scan# 1268
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31

Tgt Ion:163 Resp: 44403
Ion Ratio Lower Upper
163 100
194 3.6 2.9 4.3
164 9.8 8.2 12.4

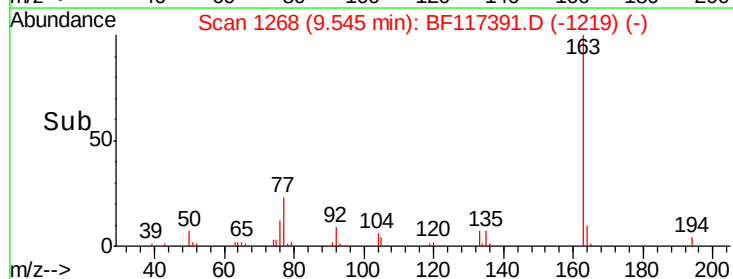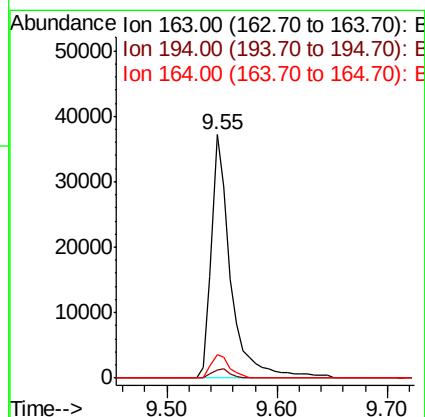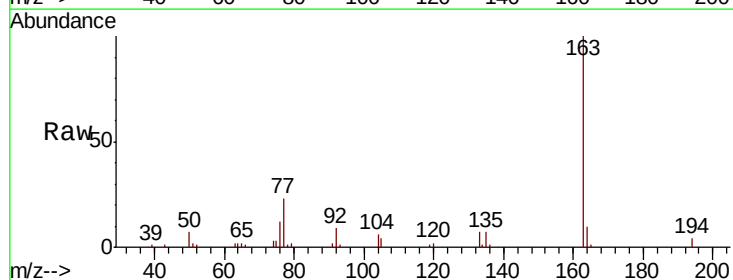







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1570
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31

Instrument :
BNA_F
ClientSampleId :
TP-3

Tot Ion:188 Resp: 119105
Ion Ratio Lower Upper
188 100
94 9.0 8.2 12.2
80 10.8 9.0 13.6

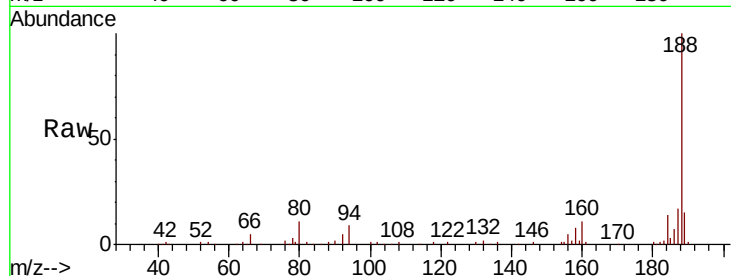


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


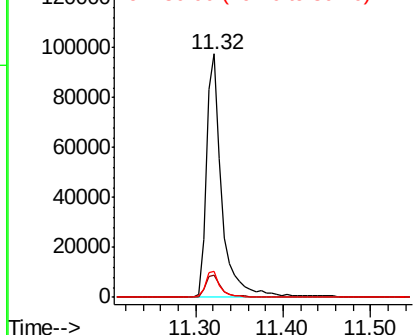



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.96 min Scan# 2019
Delta R.T. -0.01 min
Lab File: BF117391.D
Acq: 13 Oct 2019 1:31

Tgt Ion:240 Resp: 88317
Ion Ratio Lower Upper
240 100
120 11.0 8.3 12.5
236 25.5 20.3 30.5



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

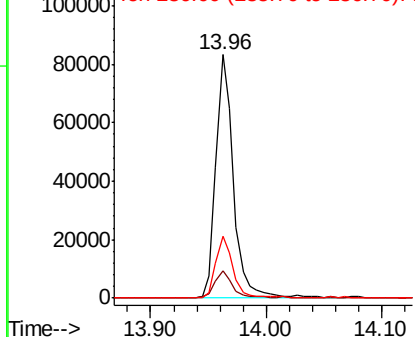



#79

Terphenyl-d14

Concen: 52.035 ng

RT: 12.90 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31

Instrument :


BNA_F

ClientSampleId :

TP-3

Tot Ion:244 Resp: 245855




Ion	Ratio	Lower	Upper
244	100		
212	6.4	5.8	8.8
122	13.2	11.3	16.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

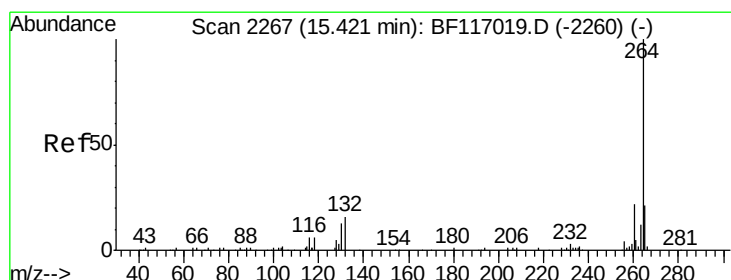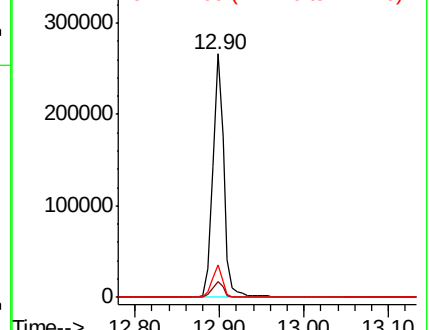

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.42 min Scan# 2267


Delta R.T. -0.01 min

Lab File: BF117391.D

Acq: 13 Oct 2019 1:31

Tgt Ion:264 Resp: 95917

Ion	Ratio	Lower	Upper
264	100		
260	22.8	17.6	26.4
265	21.5	16.6	24.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

