


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101219\
 Data File : BF117370.D
 Acq On : 12 Oct 2019 15:26
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:26:00 2019

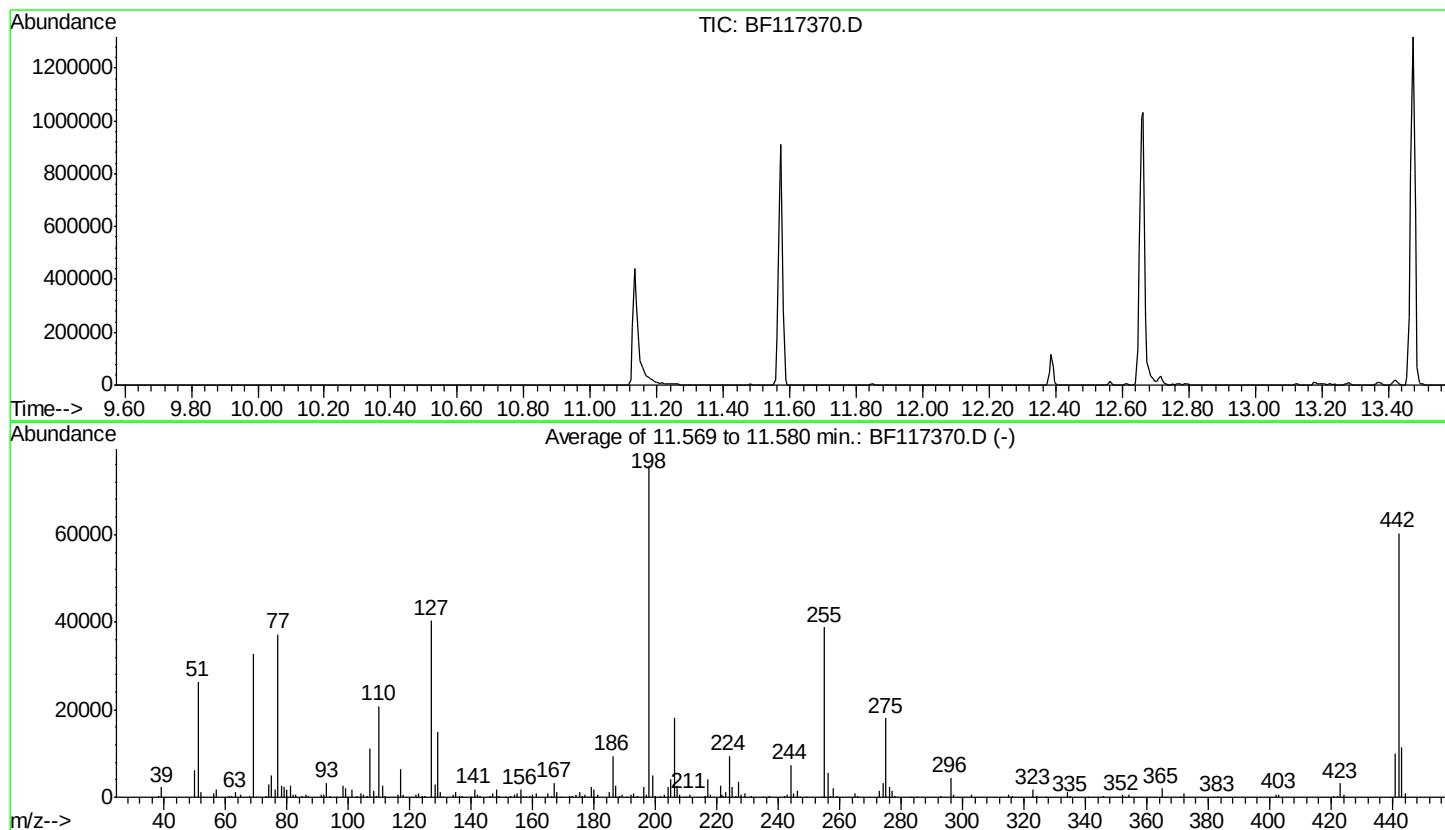

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	26394	PASS
68	69	0.00	2	1.3	433	PASS
69	198	0.00	100	43.1	32663	PASS
70	69	0.00	2	0.3	113	PASS
127	198	10	80	53.1	40257	PASS
197	198	0.00	2	0.7	523	PASS
198	198	100	100	100.0	75754	PASS
199	198	5	9	6.7	5067	PASS
275	198	10	60	23.9	18070	PASS
365	198	1	100	2.6	1951	PASS
441	198	0.01	100	13.3	10052	PASS
442	198	50	100	79.6	60317	PASS
443	442	15	24	18.8	11363	PASS