

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125812.D
 Acq On : 12 Oct 2021 20:39
 Operator : JU/CG
 Sample : M4158-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T8-COMP-(1-4)

Quant Time: Oct 13 09:47:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	187442	20.000	ng	0.00
21) Naphthalene-d8	8.122	136	669043	20.000	ng	# 0.00
39) Acenaphthene-d10	9.875	164	299407	20.000	ng	0.00
64) Phenanthrene-d10	11.369	188	399297	20.000	ng	# 0.00
76) Chrysene-d12	14.004	240	412921	20.000	ng	0.01
86) Perylene-d12	15.451	264	343592	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	957808	83.477	ng	0.00
7) Phenol-d6	6.463	99	1077654	72.958	ng	-0.01
23) Nitrobenzene-d5	7.398	82	629949	58.528	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	233648	79.040	ng	0.00
45) 2-Fluorobiphenyl	9.198	172	1146153	66.028	ng	0.00
79) Terphenyl-d14	12.957	244	1023301	37.749	ng	0.01
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.398	70	78001	10.003	ng	# 52
25) Isophorone	7.398	82	627380	32.902	ng	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125812.D
Acq On : 12 Oct 2021 20:39
Operator : JU/CG
Sample : M4158-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)

Quant Time: Oct 13 09:47:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration




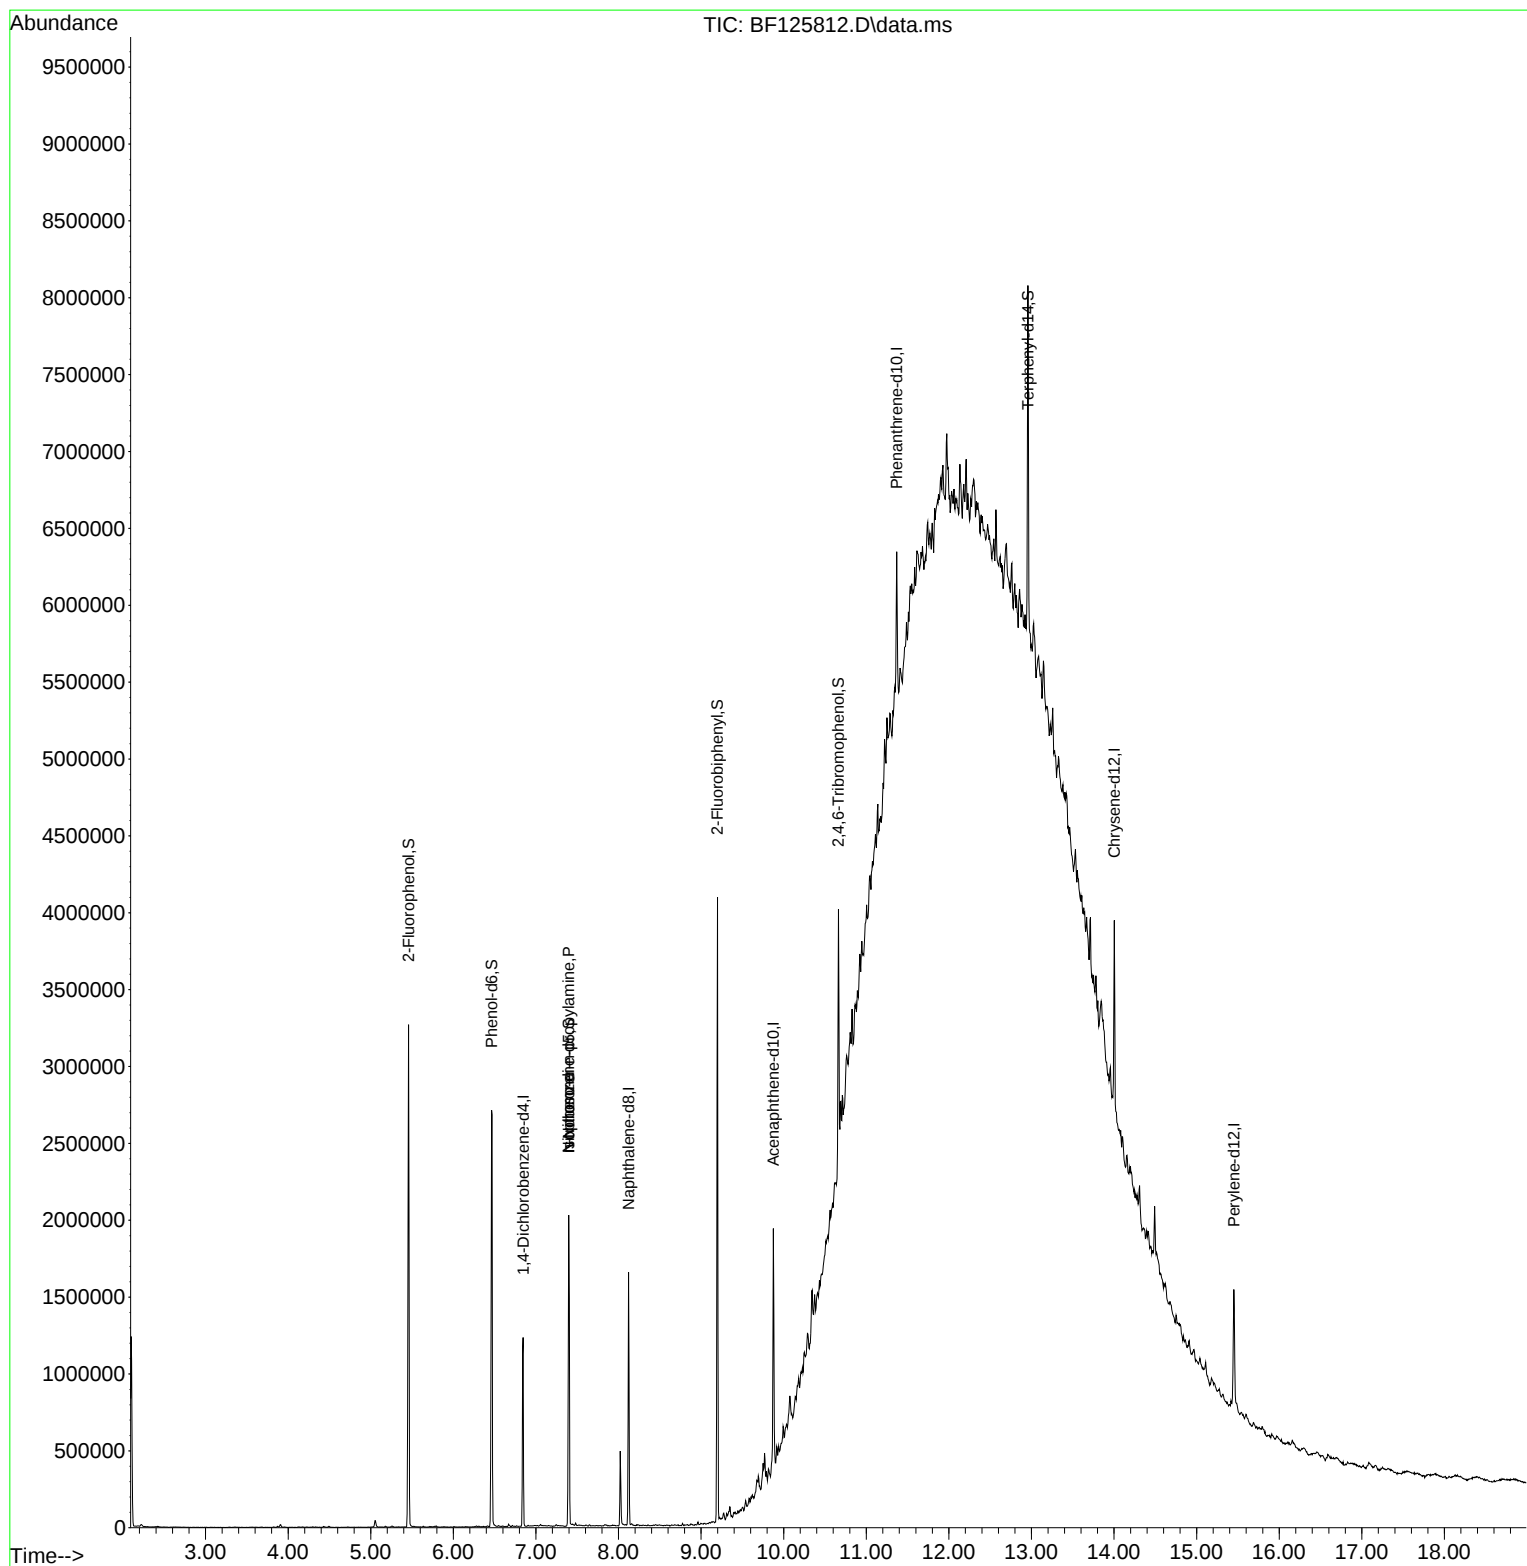


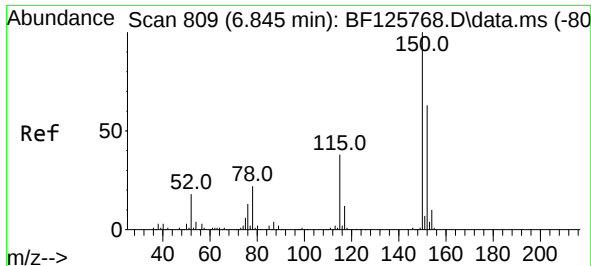

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 809
Delta R.T. 0.000 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39




Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)


Tgt Ion:152 Resp: 187442
Ion Ratio Lower Upper
152 100
150 158.8 117.6 176.4
115 58.6 47.1 70.7

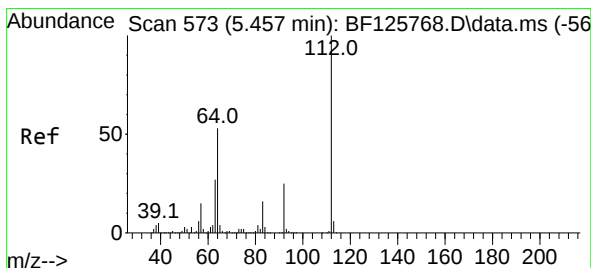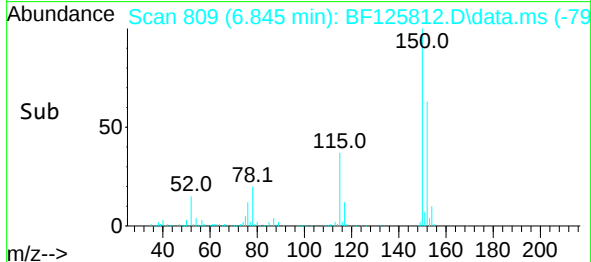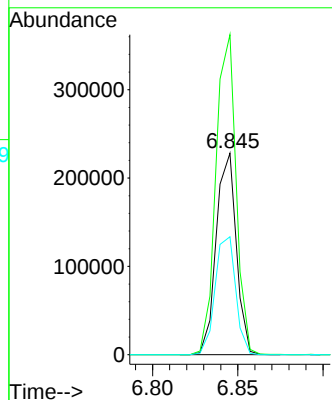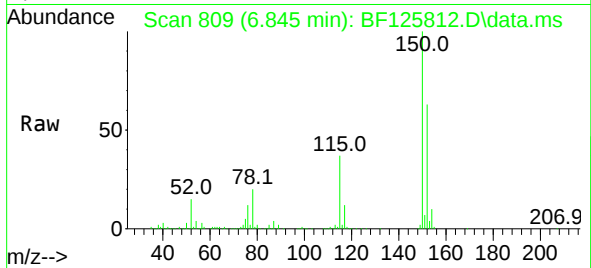

#5
2-Fluorophenol
Concen: 83.477 ng
RT: 5.457 min Scan# 573
Delta R.T. 0.000 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39

Tgt Ion:112 Resp: 957808
Ion Ratio Lower Upper
112 100
64 53.0 44.2 66.2
63 25.7 26.2 39.2#


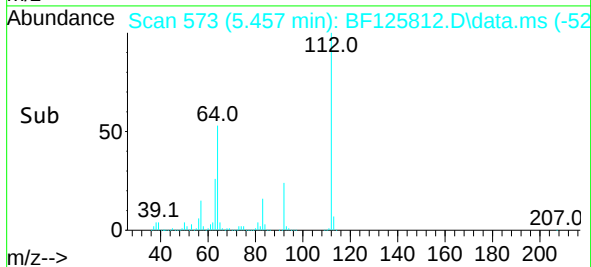
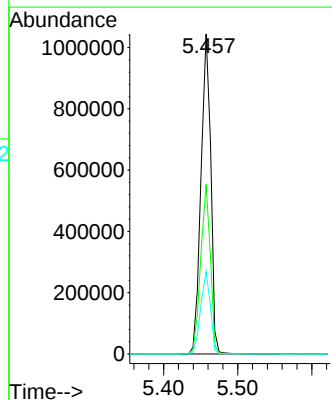
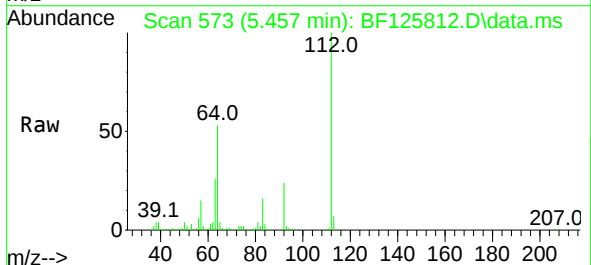


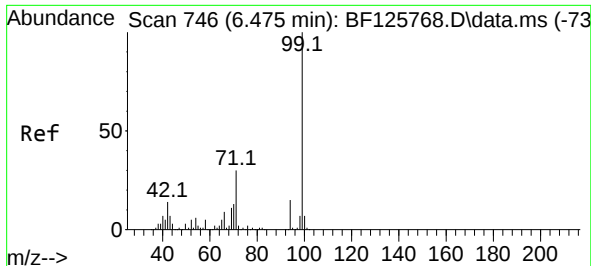

#7
Phenol-d6
Concen: 72.958 ng
RT: 6.463 min Scan# 744
Delta R.T. -0.012 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39




Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)


Tgt Ion: 99 Resp: 1077654
Ion Ratio Lower Upper
99 100
42 14.2 23.5 35.3#
71 29.5 25.6 38.4

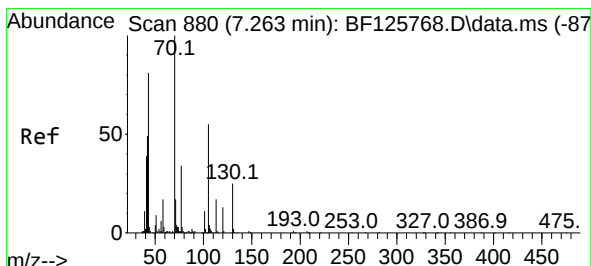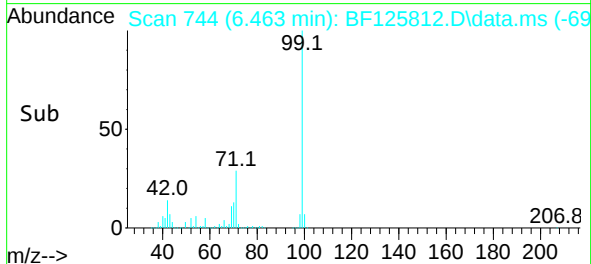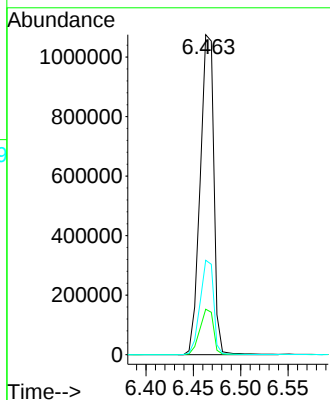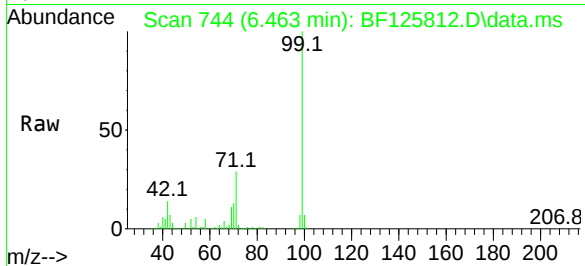

#19
n-Nitroso-di-n-propylamine
Concen: 10.003 ng
RT: 7.398 min Scan# 903
Delta R.T. 0.135 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39

Tgt Ion: 70 Resp: 78001
Ion Ratio Lower Upper
70 100
42 42.6 72.2 108.2#
101 0.0 7.8 11.8#
130 2.5 21.8 32.6#


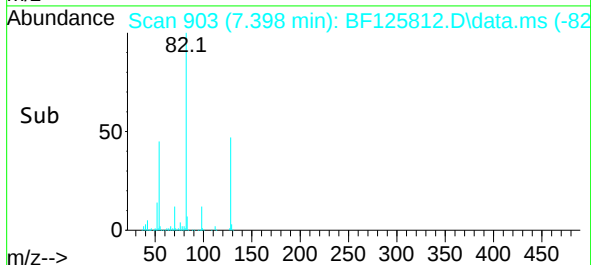
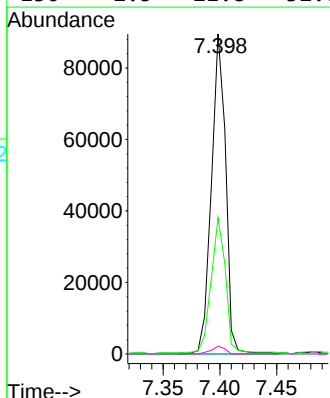
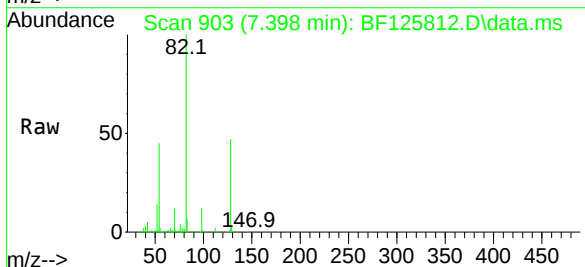


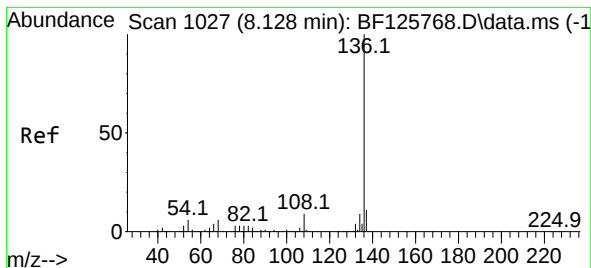

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39




Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)


Tgt Ion:	136	Resp:	669043
Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.8	14.6
54	6.7	6.4	9.6
68	6.2	3.3	4.9

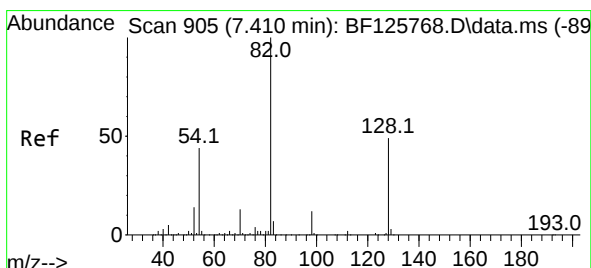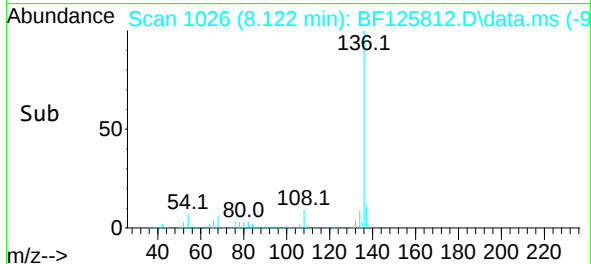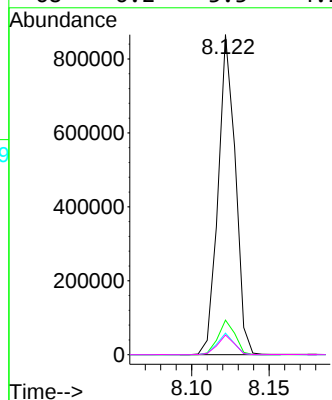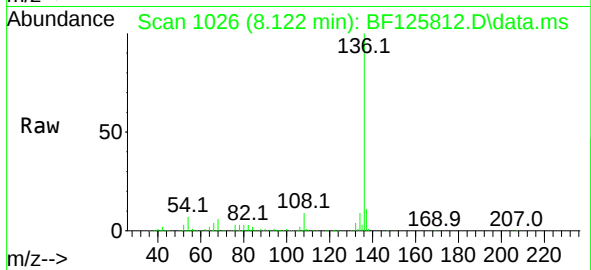

#23
Nitrobenzene-d5
Concen: 58.528 ng
RT: 7.398 min Scan# 903
Delta R.T. -0.012 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39

Tgt Ion:	82	Resp:	629949
Ion	Ratio	Lower	Upper
82	100		
128	46.7	40.6	60.8
54	45.3	49.6	74.4


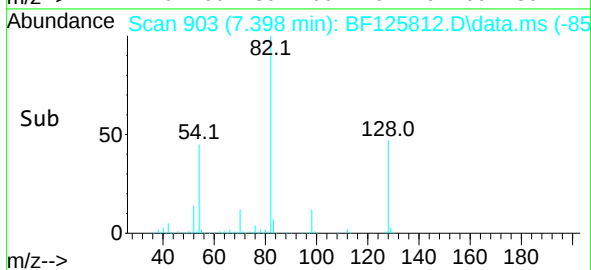
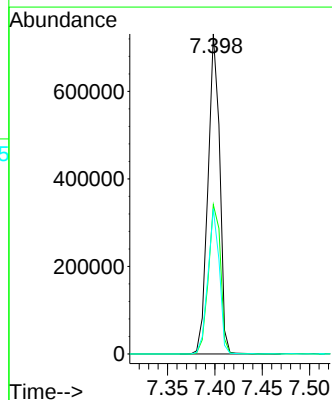
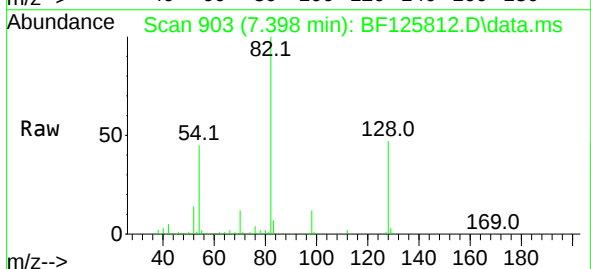


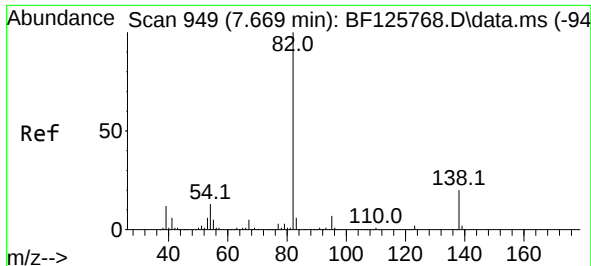

#25
Isophorone
Concen: 32.902 ng
RT: 7.398 min Scan# 903
Delta R.T. -0.270 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39




Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)


Tgt Ion: 82 Resp: 627380
Ion Ratio Lower Upper
82 100
95 0.0 6.5 9.7#
138 0.0 18.4 27.6#

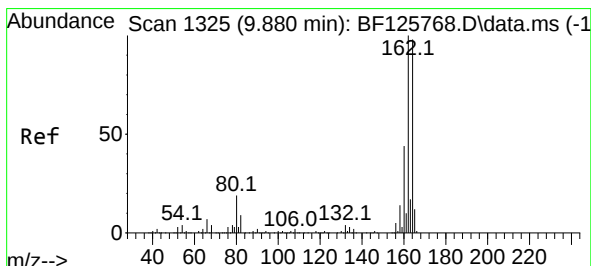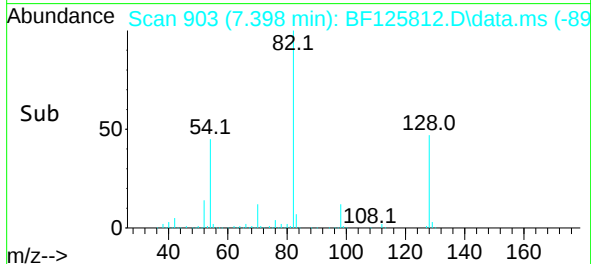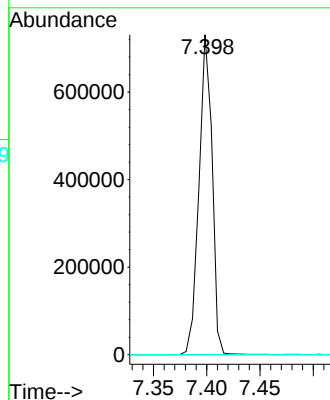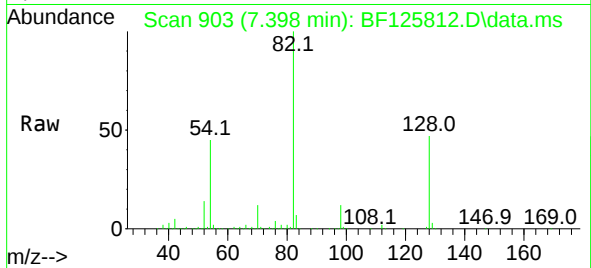

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.875 min Scan# 1324
Delta R.T. -0.006 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39

Tgt Ion: 164 Resp: 299407
Ion Ratio Lower Upper
164 100
162 102.0 81.3 121.9
160 43.1 38.0 57.0


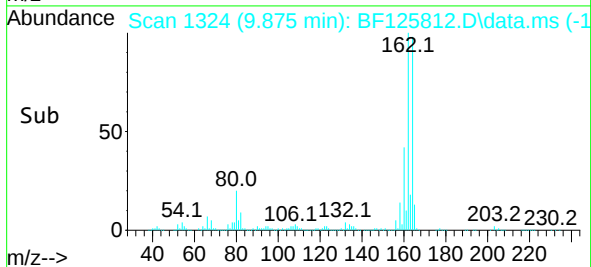
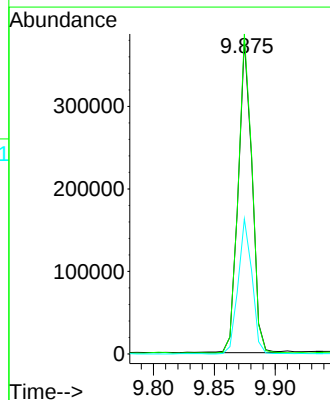
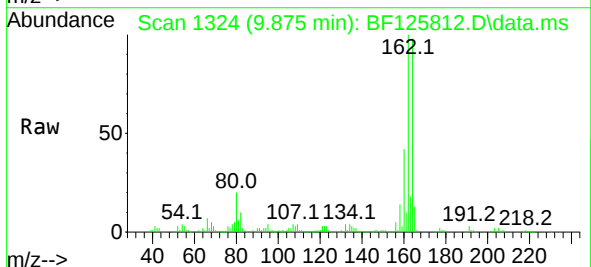


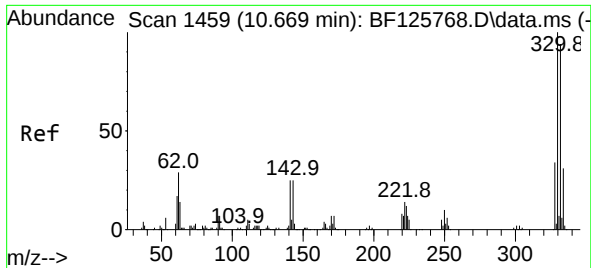

#42
 2,4,6-Tribromophenol
 Concen: 79.040 ng
 RT: 10.663 min Scan# 1458
 Delta R.T. -0.006 min
 Lab File: BF125812.D
 Acq: 12 Oct 2021 20:39




Instrument :
 BNA_F
 ClientSampleId :
 T8-COMP-(1-4)


Tgt Ion:330 Resp: 233648
 Ion Ratio Lower Upper
 330 100
 332 94.7 76.2 114.4
 141 31.9 44.6 66.8#

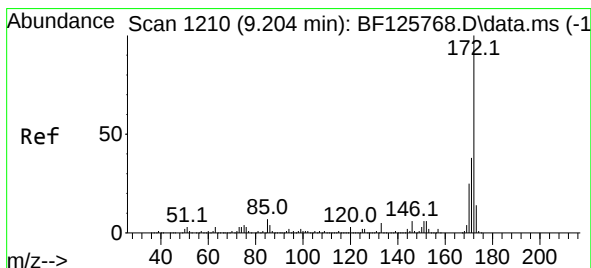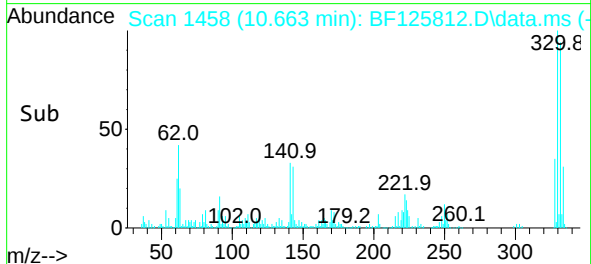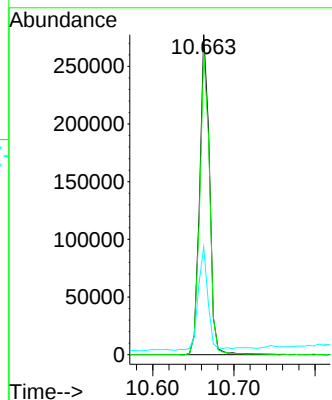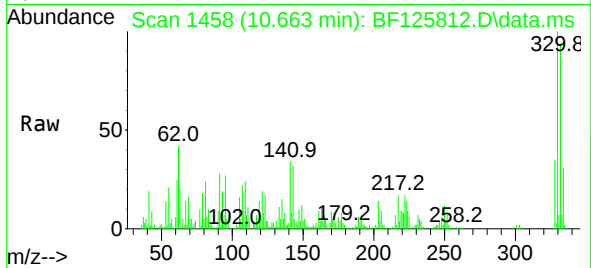

#45
 2-Fluorobiphenyl
 Concen: 66.028 ng
 RT: 9.198 min Scan# 1209
 Delta R.T. -0.006 min
 Lab File: BF125812.D
 Acq: 12 Oct 2021 20:39

Tgt Ion:172 Resp: 1146153
 Ion Ratio Lower Upper
 172 100
 171 35.5 26.5 39.7
 170 23.7 18.8 28.2


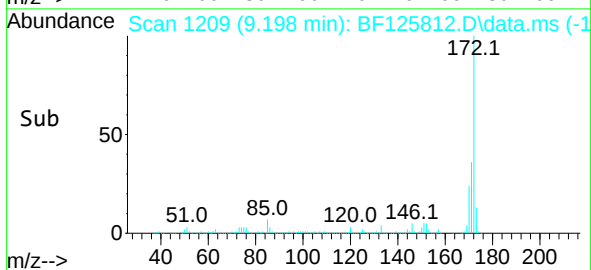
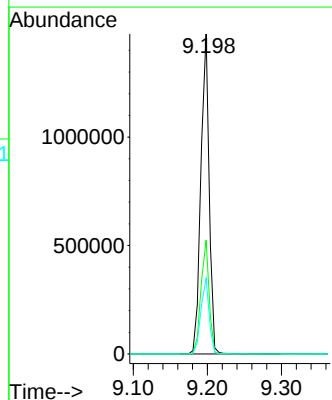
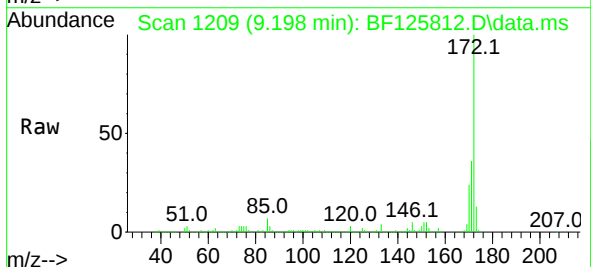


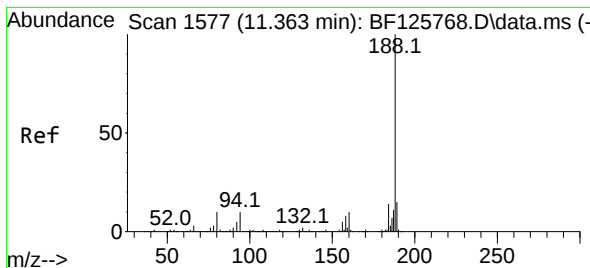

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.369 min Scan# 1578
Delta R.T. 0.006 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39




Instrument :
BNA_F
ClientSampleId :
T8-COMP-(1-4)


Tgt Ion:188 Resp: 399297
Ion Ratio Lower Upper
188 100
94 15.8 6.7 10.1#
80 13.7 7.5 11.3#

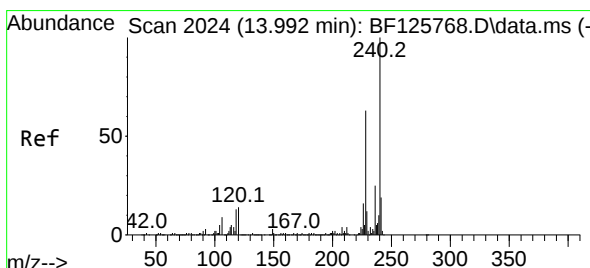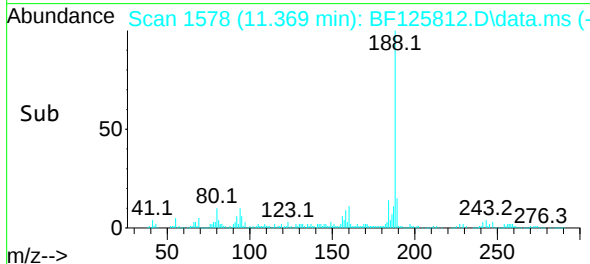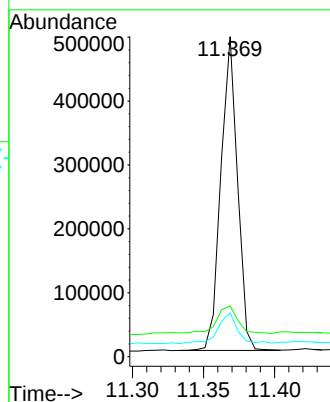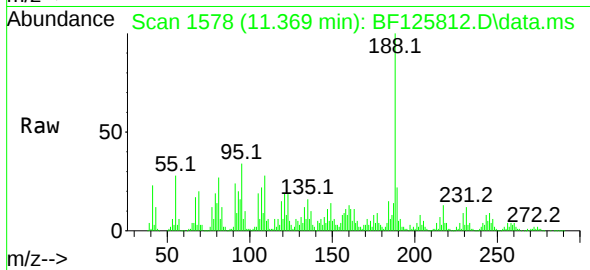

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.004 min Scan# 2026
Delta R.T. 0.012 min
Lab File: BF125812.D
Acq: 12 Oct 2021 20:39

Tgt Ion:240 Resp: 412921
Ion Ratio Lower Upper
240 100
120 13.5 10.8 16.2
236 25.5 21.6 32.4


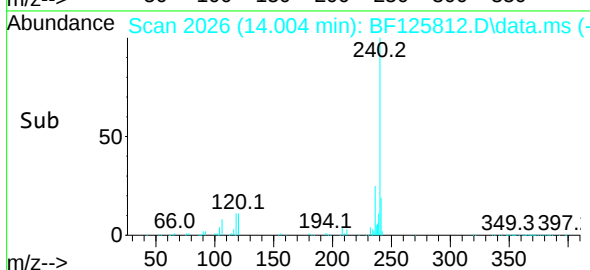
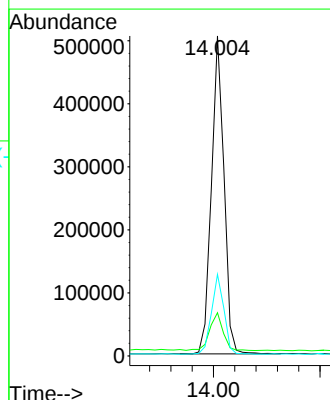
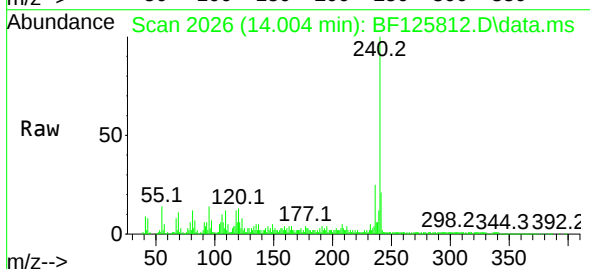


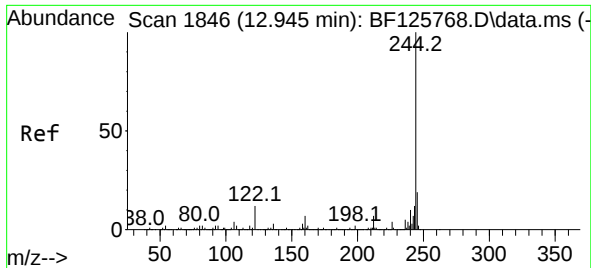

#79
 Terphenyl-d14
 Concen: 37.749 ng
 RT: 12.957 min Scan# 1848
 Delta R.T. 0.012 min
 Lab File: BF125812.D
 Acq: 12 Oct 2021 20:39

Instrument :
 BNA_F
 ClientSampleId :
 T8-COMP-(1-4)

Tgt Ion:244 Resp: 1023301
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.9 8.9
 122 12.7 9.0 13.4

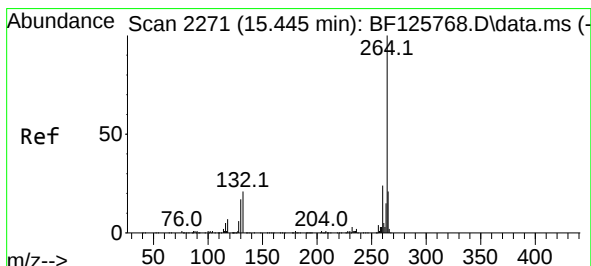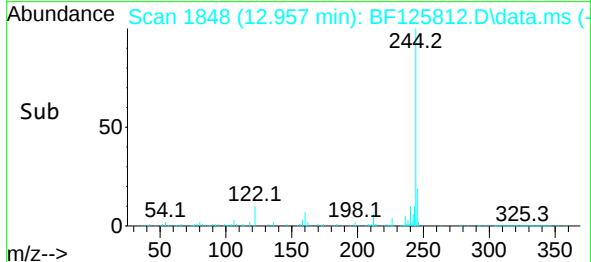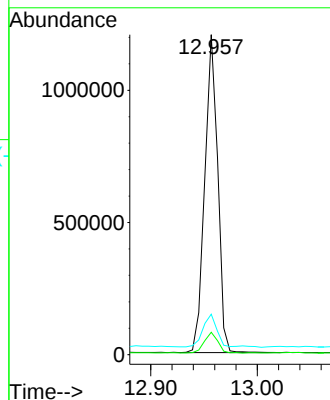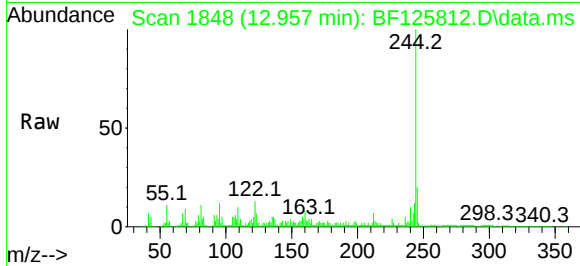

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.451 min Scan# 2272
 Delta R.T. 0.006 min
 Lab File: BF125812.D
 Acq: 12 Oct 2021 20:39

Tgt Ion:264 Resp: 343592
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.6 29.4
 265 21.2 17.2 25.8

