
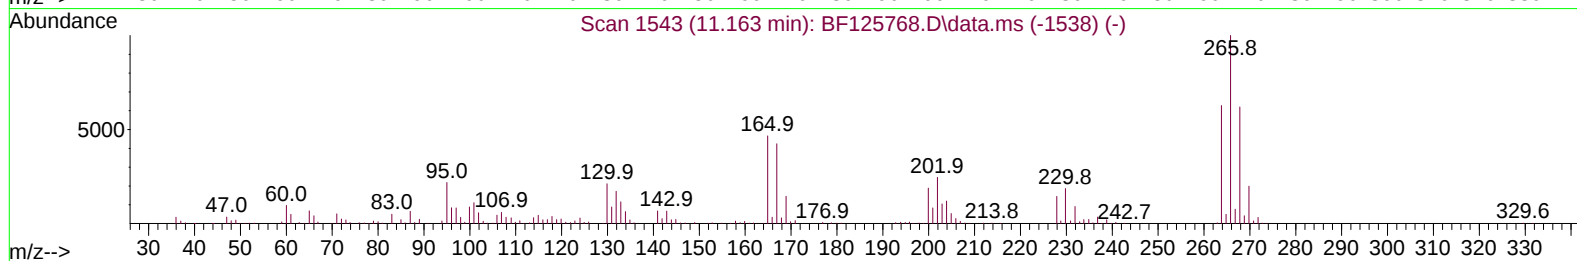
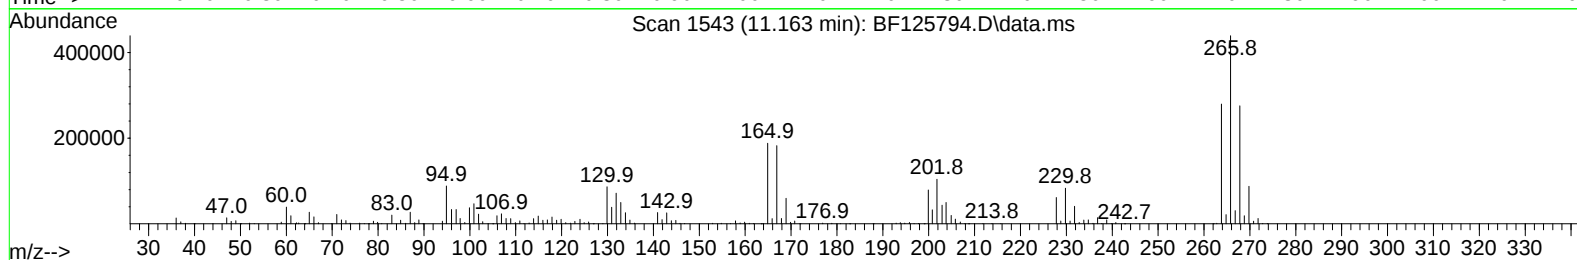


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125794.D
 Acq On : 12 Oct 2021 10:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:13:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

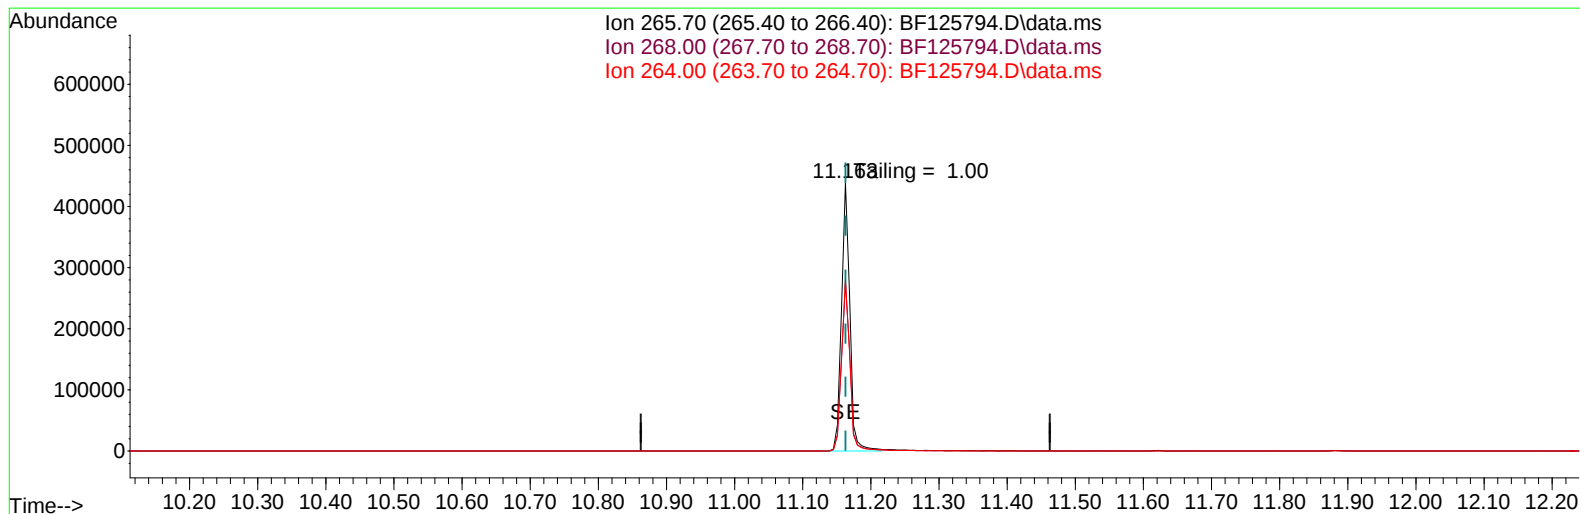

TIC: BF125794.D\data.ms

(70) Pentachlorophenol (C)




11.163min (0.000) 458254.10 ng

response 378157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.79
264.00	69.90	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125794.D
 Acq On : 12 Oct 2021 10:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:13:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

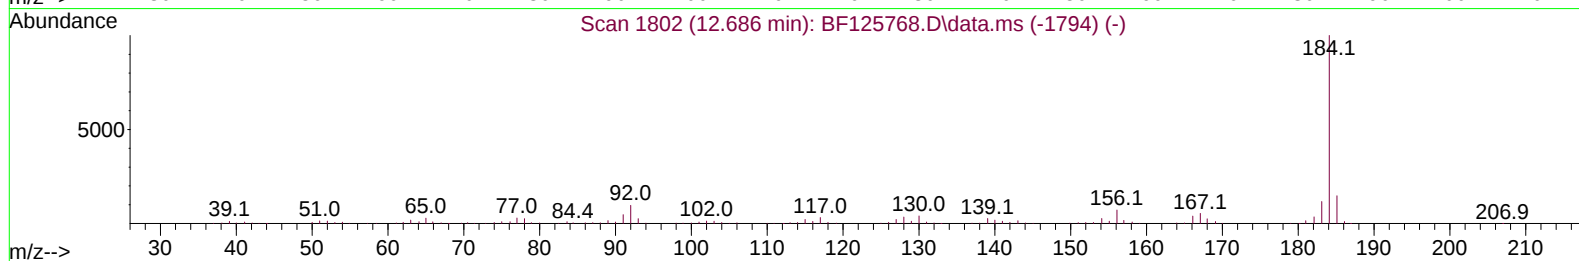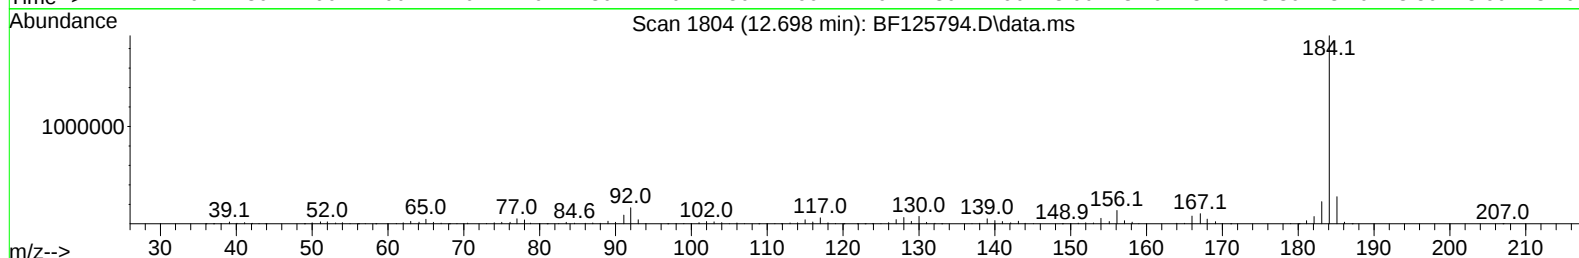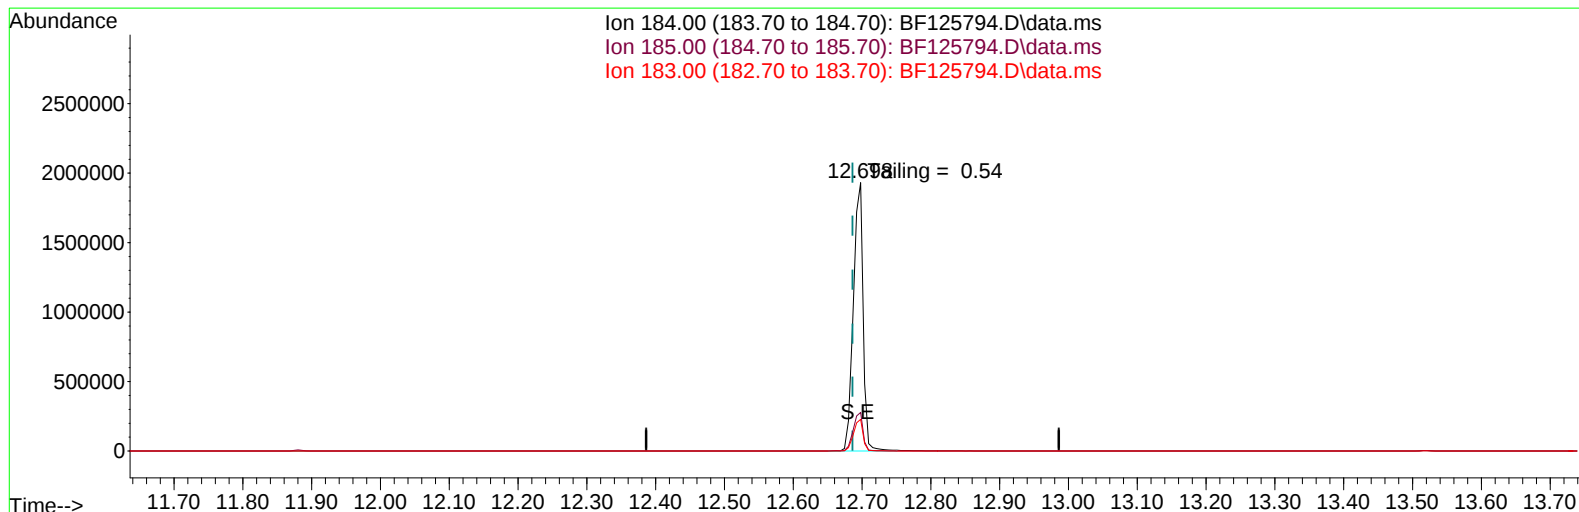

TIC: BF125794.D\data.ms

(77) Benzidine

12.698min (+ 0.012) 4896.67 ng m

response 1900688

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.38
183.00	10.10	11.80
0.00	0.00	0.00