

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125798.D
 Acq On : 12 Oct 2021 13:08
 Operator : JU/CG
 Sample : M4112-04RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1-FLOORRE

Quant Time: Oct 12 16:26:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.839	152	157947	20.00	ng	0.00
21) Naphthalene-d8	8.122	136	558066	20.00	ng	# 0.00
39) Acenaphthene-d10	9.875	164	255452	20.00	ng	0.00
64) Phenanthrene-d10	11.357	188	462894	20.00	ng	# 0.00
76) Chrysene-d12	14.033	240	374611	20.00	ng	0.04
86) Perylene-d12	15.474	264	284569	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	650513	67.28	ng	0.00
7) Phenol-d6	6.463	99	856335	68.80	ng	-0.01
23) Nitrobenzene-d5	7.398	82	511016	56.92	ng	-0.01
42) 2,4,6-Tribromophenol	10.657	330	121081	48.01	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	945046	63.81	ng	0.00
79) Terphenyl-d14	12.945	244	1128473	45.89	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.386	77	69258	10.25	ng	94
15) Benzyl Alcohol	6.986	79	584096	70.81	ng	91
74) Di-n-butylphthalate	11.921	149	469438	18.47	ng	99
75) Fluoranthene	12.580	202	53498	2.39	ng	78
80) Butylbenzylphthalate	13.586	149	29477385	2416.40	ng	# 81
84) Bis(2-ethylhexyl)phtha...	14.033	149	103774	7.82	ng	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125798.D
Acq On : 12 Oct 2021 13:08
Operator : JU/CG
Sample : M4112-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1-FLOORRE

Quant Time: Oct 12 16:26:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration




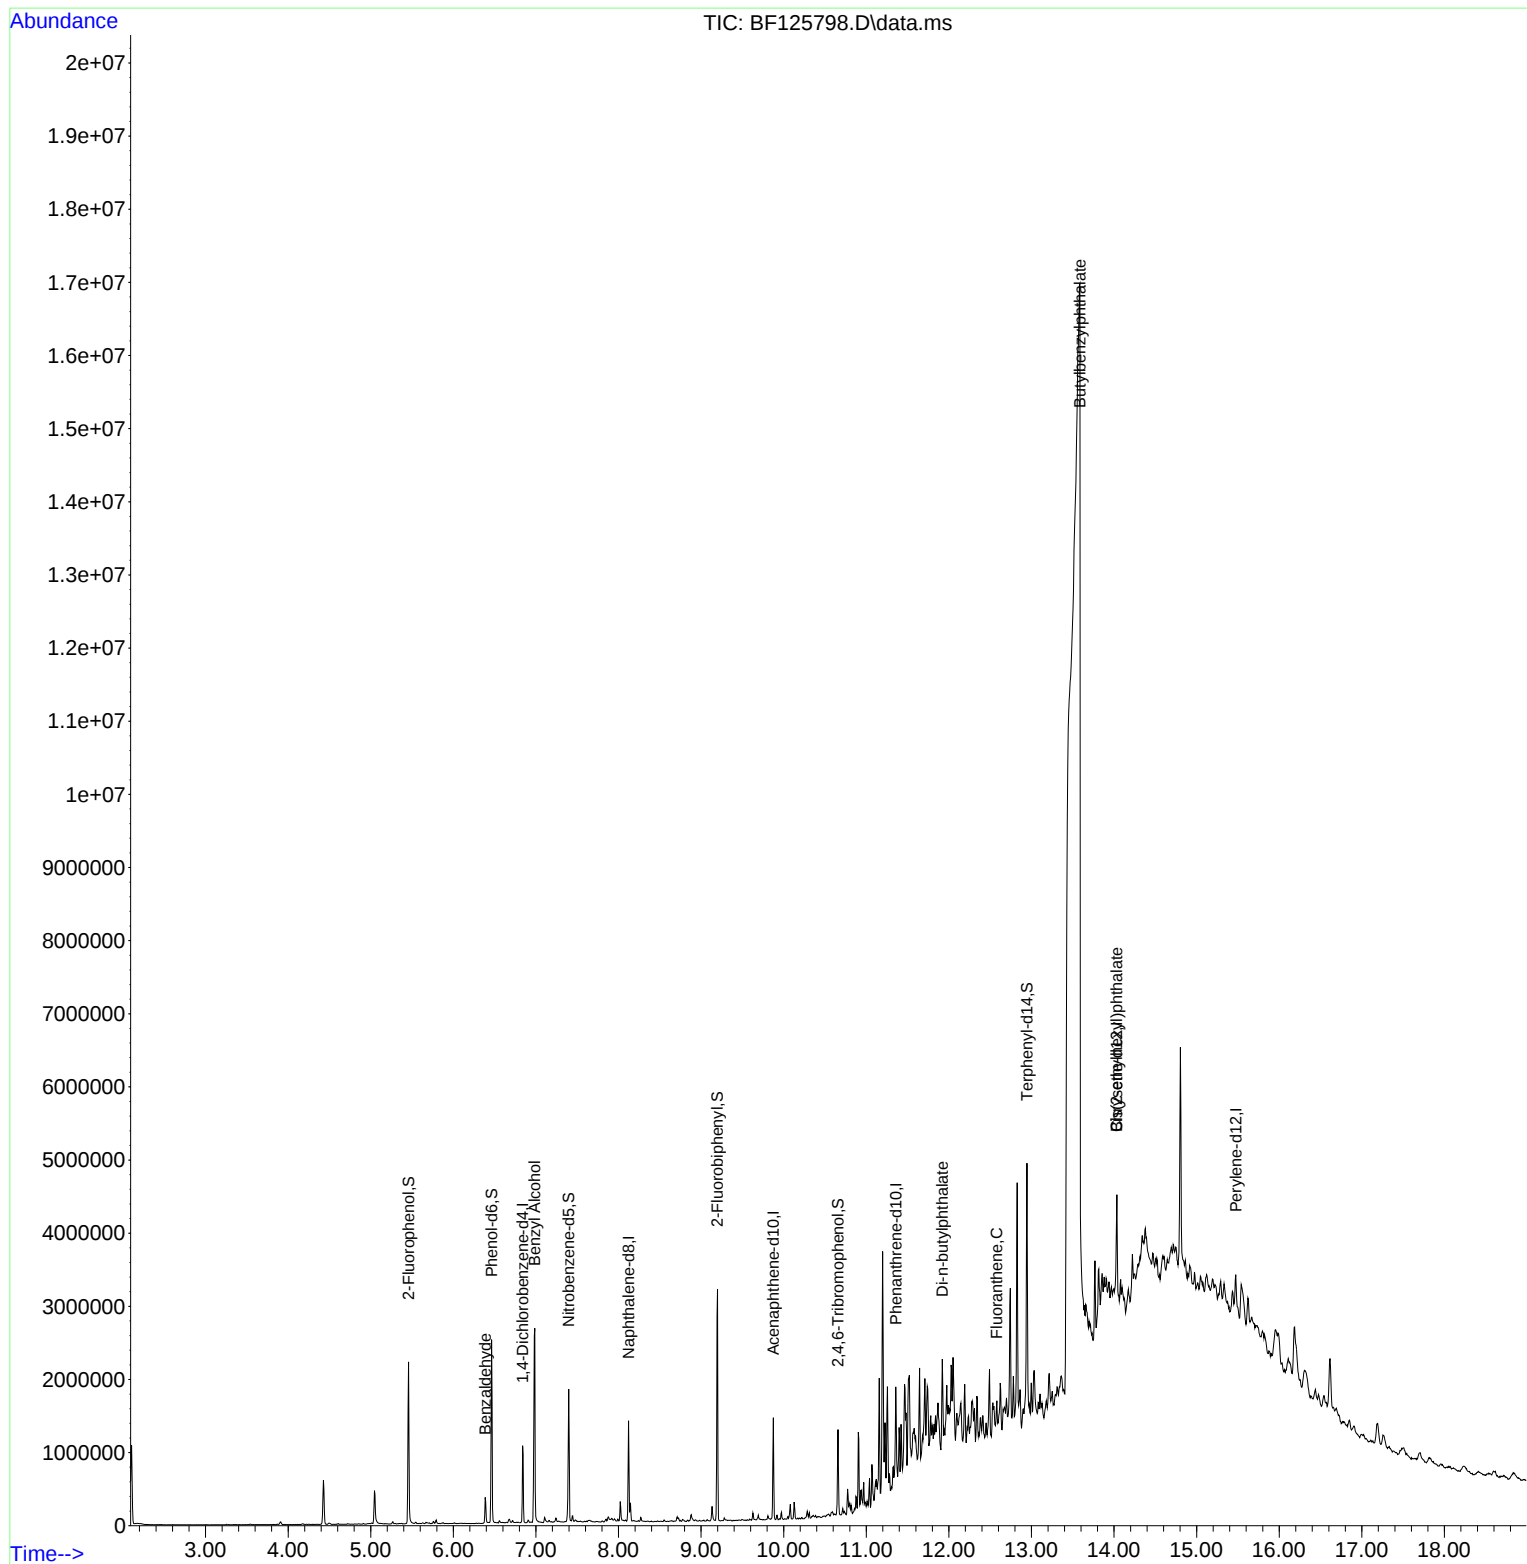


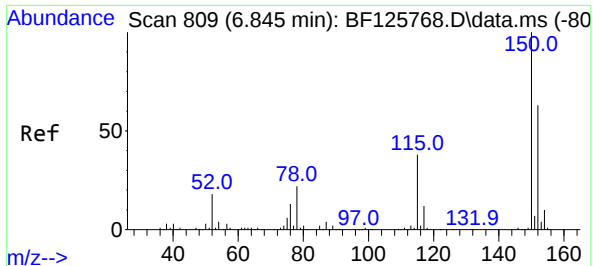

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.839 min Scan# 808
Delta R.T. -0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampleId :
1-FLOORRE


Tgt Ion:152 Resp: 157947
Ion Ratio Lower Upper
152 100
150 162.1 117.6 176.4
115 61.4 47.1 70.7

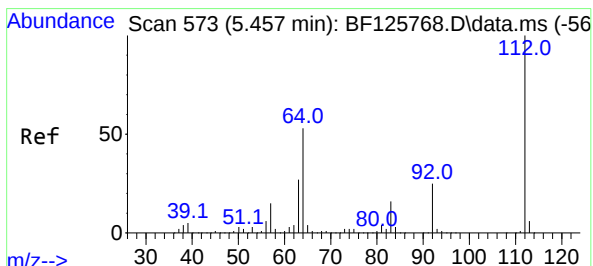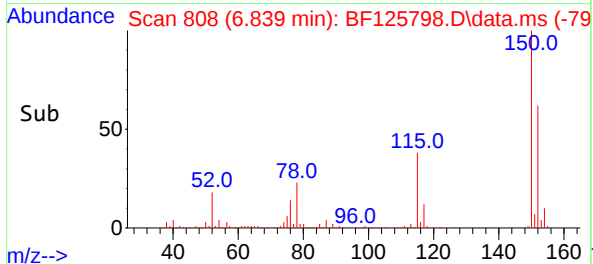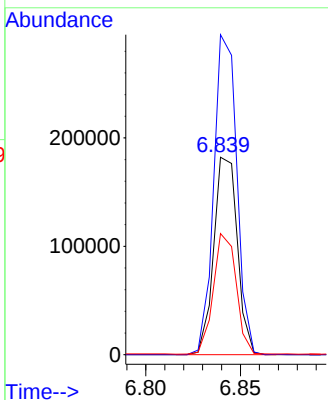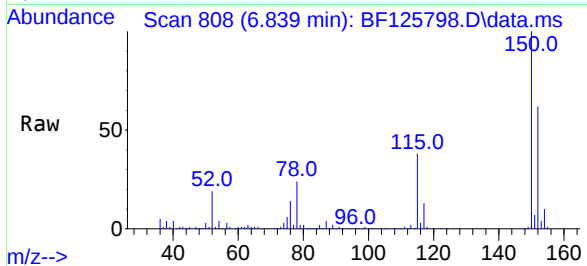

#5
2-Fluorophenol
Concen: 67.28 ng
RT: 5.457 min Scan# 573
Delta R.T. 0.000 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:112 Resp: 650513
Ion Ratio Lower Upper
112 100
64 52.0 44.2 66.2
63 25.9 26.2 39.2#


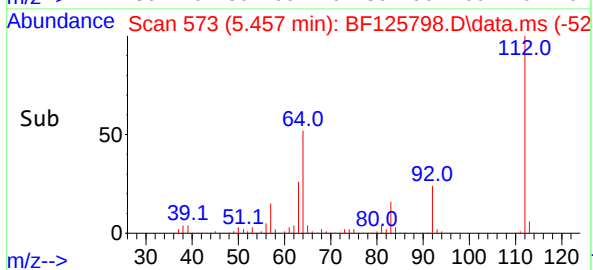
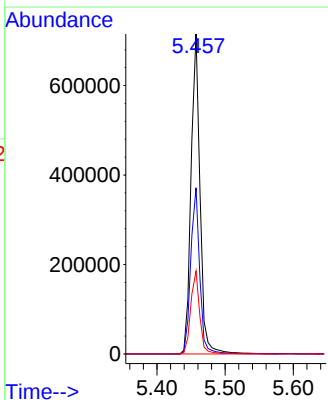
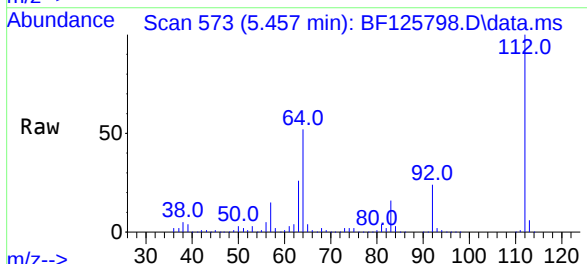


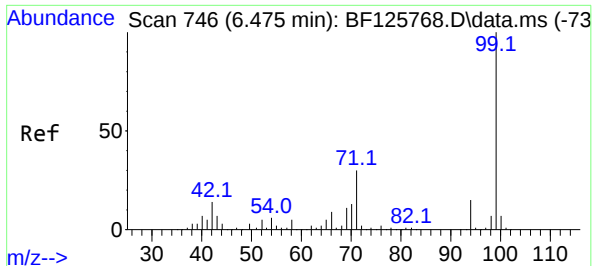

#7
Phenol-d6
Concen: 68.80 ng
RT: 6.463 min Scan# 744
Delta R.T. -0.012 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampleId :
1-FLOORRE


Tgt Ion: 99 Resp: 856335
Ion Ratio Lower Upper
99 100
42 14.7 23.5 35.3#
71 30.1 25.6 38.4

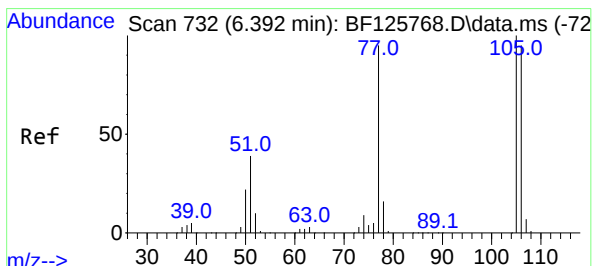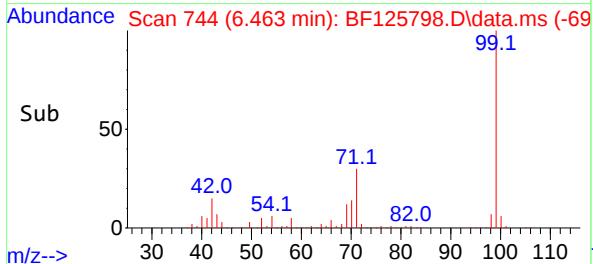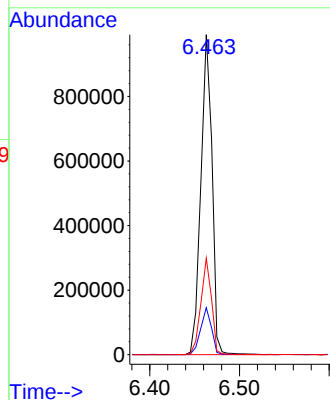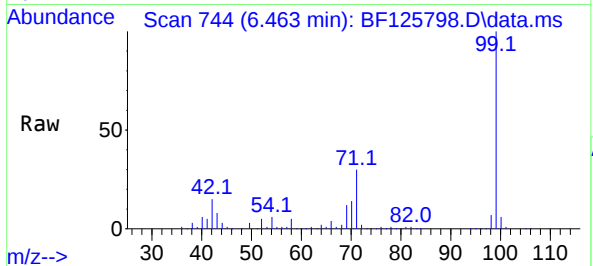

#9
Benzaldehyde
Concen: 10.25 ng
RT: 6.386 min Scan# 731
Delta R.T. -0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion: 77 Resp: 69258
Ion Ratio Lower Upper
77 100
105 106.4 75.9 115.9
106 105.8 84.0 124.0

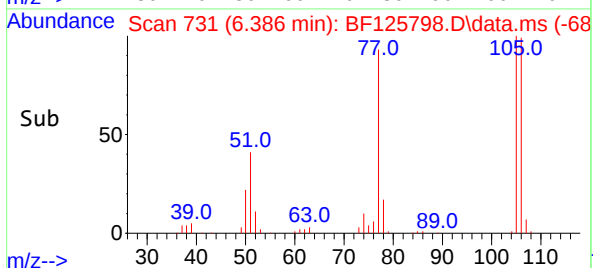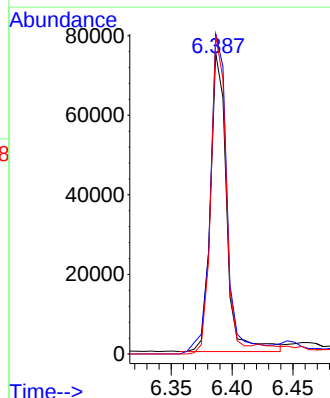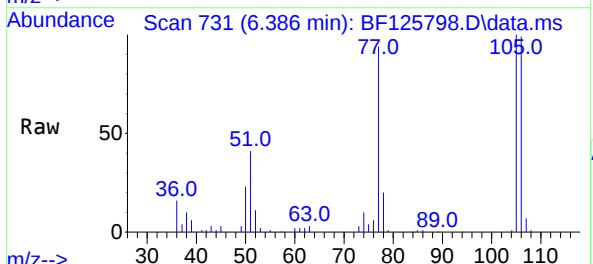







#15
Benzyl Alcohol
Concen: 70.81 ng
RT: 6.986 min Scan# 833
Delta R.T. 0.000 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Instrument :
BNA_F
ClientSampleId :
1-FLOORRE

Tgt Ion: 79 Resp: 584096




Ion	Ratio	Lower	Upper
79	100		
108	87.3	60.4	90.6
77	62.2	51.5	77.3

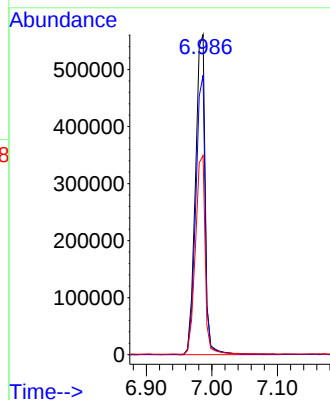


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion: 136 Resp: 558066

Ion	Ratio	Lower	Upper
136	100		
137	10.7	9.8	14.6
54	6.3	6.4	9.6#
68	6.4	3.3	4.9#

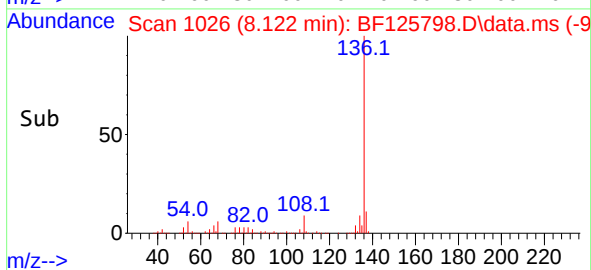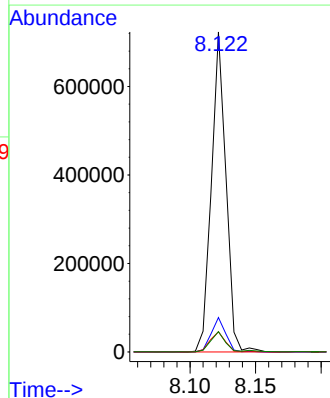



#23

Nitrobenzene-d5

Concen: 56.92 ng

RT: 7.398 min Scan# 903

Delta R.T. -0.012 min

Lab File: BF125798.D

Acq: 12 Oct 2021 13:08

Instrument :

BNA_F

ClientSampleId :

1-FLOORRE





Tgt Ion: 82 Resp: 511016

Ion Ratio Lower Upper

82 100

128 47.7 40.6 60.8

54 43.7 49.6 74.4#

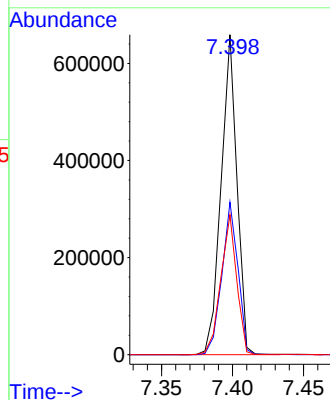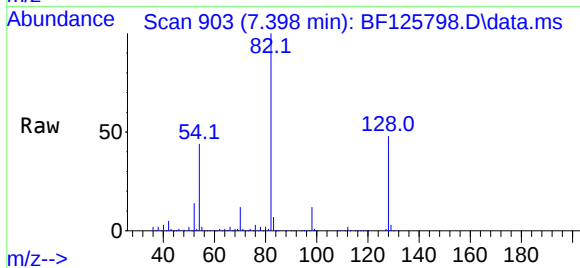

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.875 min Scan# 1324

Delta R.T. -0.006 min

Lab File: BF125798.D

Acq: 12 Oct 2021 13:08




Tgt Ion: 164 Resp: 255452


Ion Ratio Lower Upper

164 100

162 102.2 81.3 121.9

160 43.5 38.0 57.0


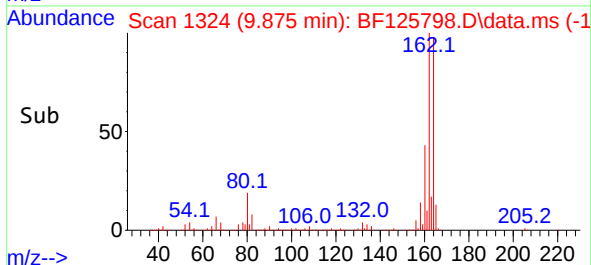
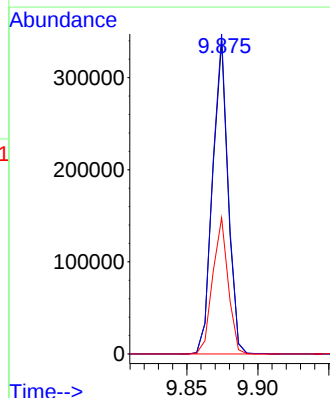
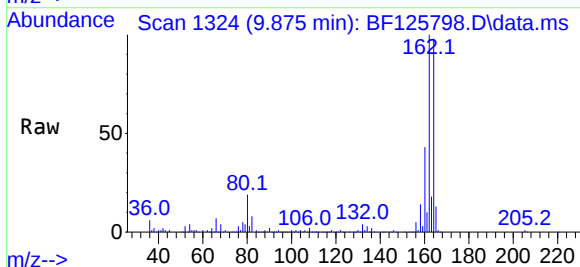




#42
2,4,6-Tribromophenol
Concen: 48.01 ng
RT: 10.657 min Scan# 1457
Delta R.T. -0.012 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampled :
1-FLOORRE


Tgt Ion:330 Resp: 121081
Ion Ratio Lower Upper
330 100
332 96.7 76.2 114.4
141 34.6 44.6 66.8#

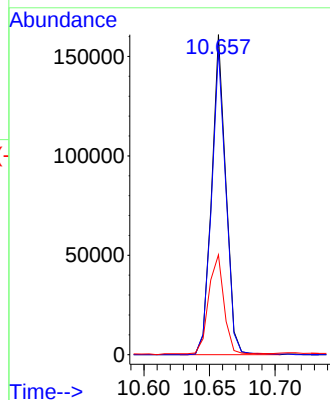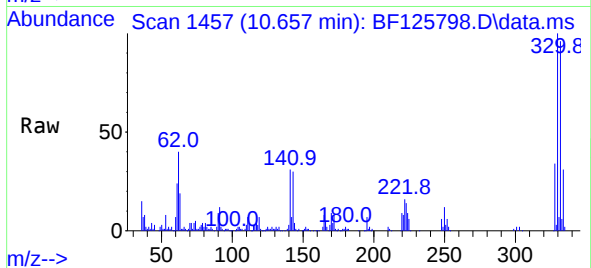

#45
2-Fluorobiphenyl
Concen: 63.81 ng
RT: 9.198 min Scan# 1209
Delta R.T. -0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:172 Resp: 945046
Ion Ratio Lower Upper
172 100
171 35.6 26.5 39.7
170 22.8 18.8 28.2


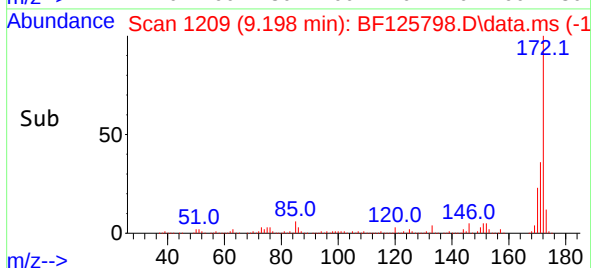
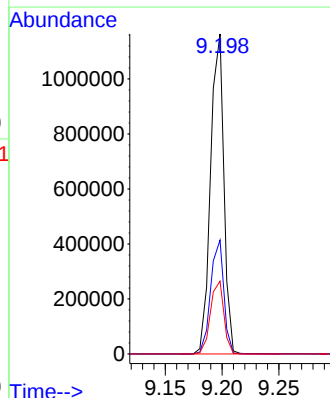





#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.357 min Scan# 1576
Delta R.T. -0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampleId :
1-FLOORRE


Tgt Ion:188 Resp: 462894
Ion Ratio Lower Upper
188 100
94 10.6 6.7 10.1#
80 10.9 7.5 11.3

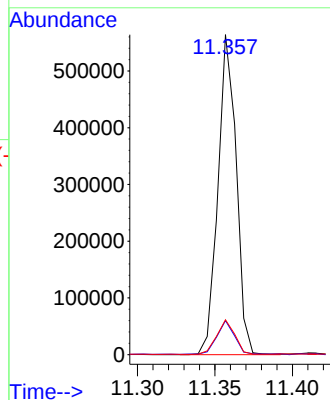

#74
Di-n-butylphthalate
Concen: 18.47 ng
RT: 11.921 min Scan# 1672
Delta R.T. 0.000 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:149 Resp: 469438
Ion Ratio Lower Upper
149 100
150 9.0 7.4 11.2
104 5.6 4.1 6.1


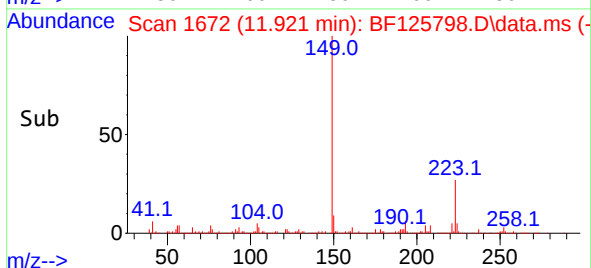
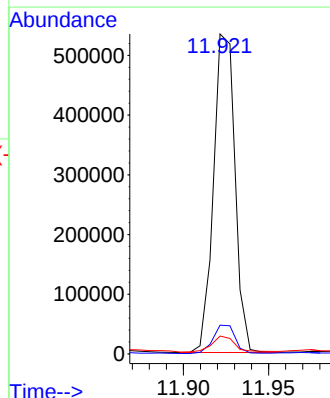





#75
Fluoranthene
Concen: 2.39 ng
RT: 12.580 min Scan# 1784
Delta R.T. 0.006 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampleId :
1-FLOORRE


Tgt Ion:202 Resp: 53498
Ion Ratio Lower Upper
202 100
101 17.1 0.0 30.7
203 26.9 0.0 36.3

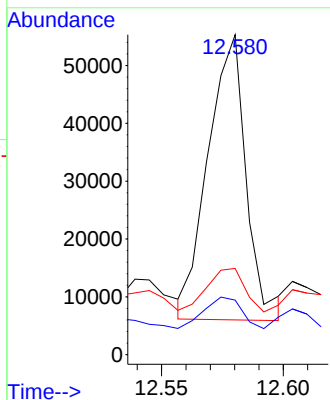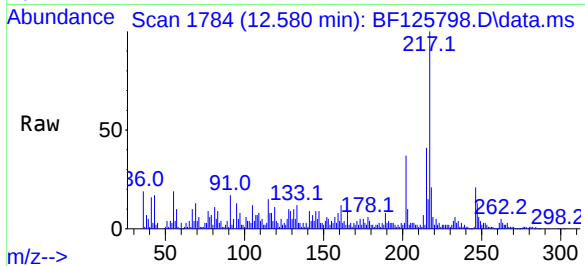

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.033 min Scan# 2031
Delta R.T. 0.041 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:240 Resp: 374611
Ion Ratio Lower Upper
240 100
120 14.6 10.8 16.2
236 25.5 21.6 32.4


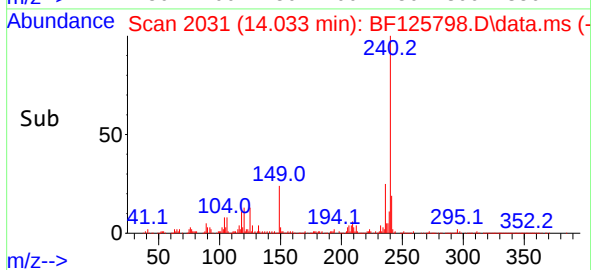
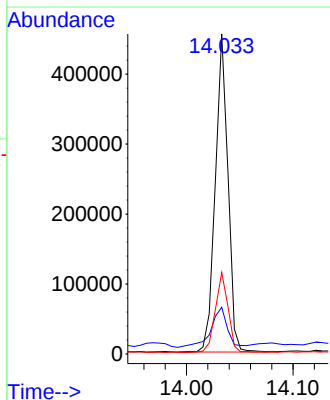
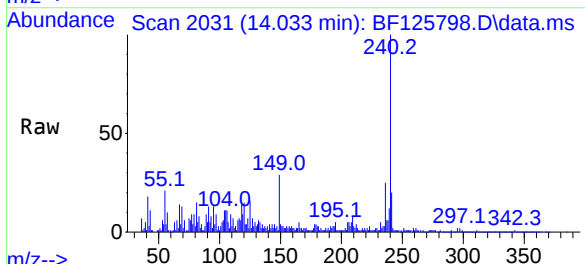




#79
Terphenyl-d14
Concen: 45.89 ng
RT: 12.945 min Scan# 1846
Delta R.T. 0.000 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08




Instrument :
BNA_F
ClientSampleId :
1-FLOORRE


Tgt Ion:244 Resp: 1128473
Ion Ratio Lower Upper
244 100
212 6.8 5.9 8.9
122 12.2 9.0 13.4

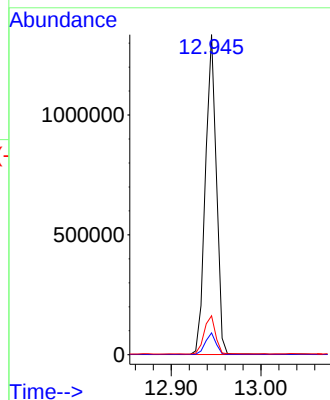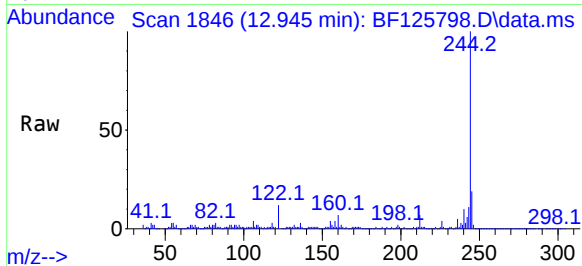

#80
Butylbenzylphthalate
Concen: 2416.40 ng
RT: 13.586 min Scan# 1955
Delta R.T. 0.171 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:149 Resp:29477385
Ion Ratio Lower Upper
149 100
91 74.7 51.8 77.8
206 37.2 14.5 21.7#


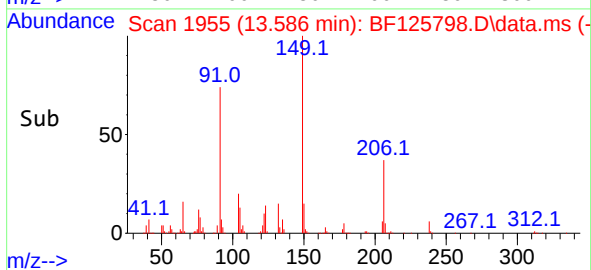
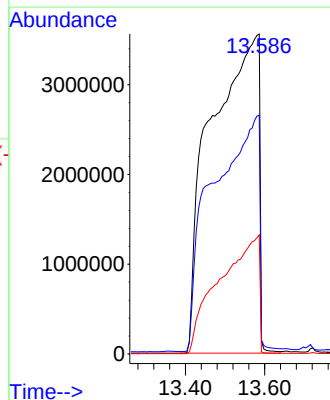
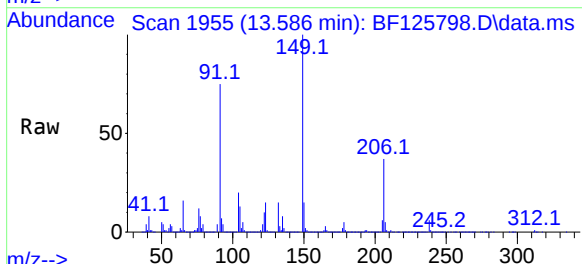




#84
Bis(2-ethylhexyl)phthalate
Concen: 7.82 ng
RT: 14.033 min Scan# 2031
Delta R.T. 0.053 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Instrument :
BNA_F
ClientSampled :
1-FLOORRE

Tgt Ion:149 Resp: 103774
Ion Ratio Lower Upper
149 100
167 8.0 21.4 32.0#
279 1.5 2.6 4.0#

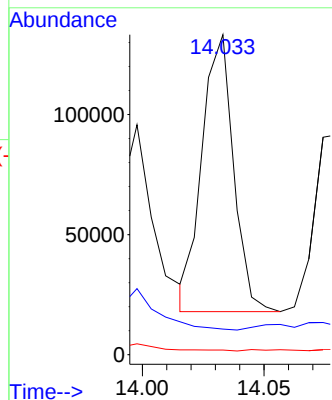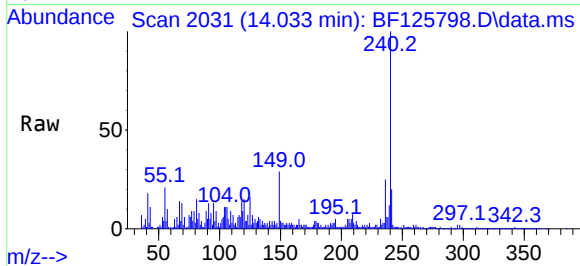

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.474 min Scan# 2276
Delta R.T. 0.029 min
Lab File: BF125798.D
Acq: 12 Oct 2021 13:08

Tgt Ion:264 Resp: 284569
Ion Ratio Lower Upper
264 100
260 24.8 19.6 29.4
265 22.3 17.2 25.8

