

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125807.D
 Acq On : 12 Oct 2021 17:59
 Operator : JU/CG
 Sample : M4159-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T10-COMP-(1-4)

Quant Time: Oct 13 09:44:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.840	152	186260	20.00	ng	0.00
21) Naphthalene-d8	8.122	136	691402	20.00	ng	# 0.00
39) Acenaphthene-d10	9.875	164	322385	20.00	ng	0.00
64) Phenanthrene-d10	11.357	188	520687	20.00	ng	0.00
76) Chrysene-d12	13.992	240	447138	20.00	ng	0.00
86) Perylene-d12	15.445	264	361790	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.463	112	1276576	111.96	ng	0.00
7) Phenol-d6	6.469	99	1520557	103.60	ng	0.00
23) Nitrobenzene-d5	7.398	82	924196	83.09	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	353457	111.05	ng	0.00
45) 2-Fluorobiphenyl	9.198	172	1671662	89.44	ng	0.00
79) Terphenyl-d14	12.945	244	1716111	58.46	ng	0.00
Target Compounds						
75) Fluoranthene	12.563	202	55968	2.23	ng	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125807.D
Acq On : 12 Oct 2021 17:59
Operator : JU/CG
Sample : M4159-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)

Quant Time: Oct 13 09:44:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration




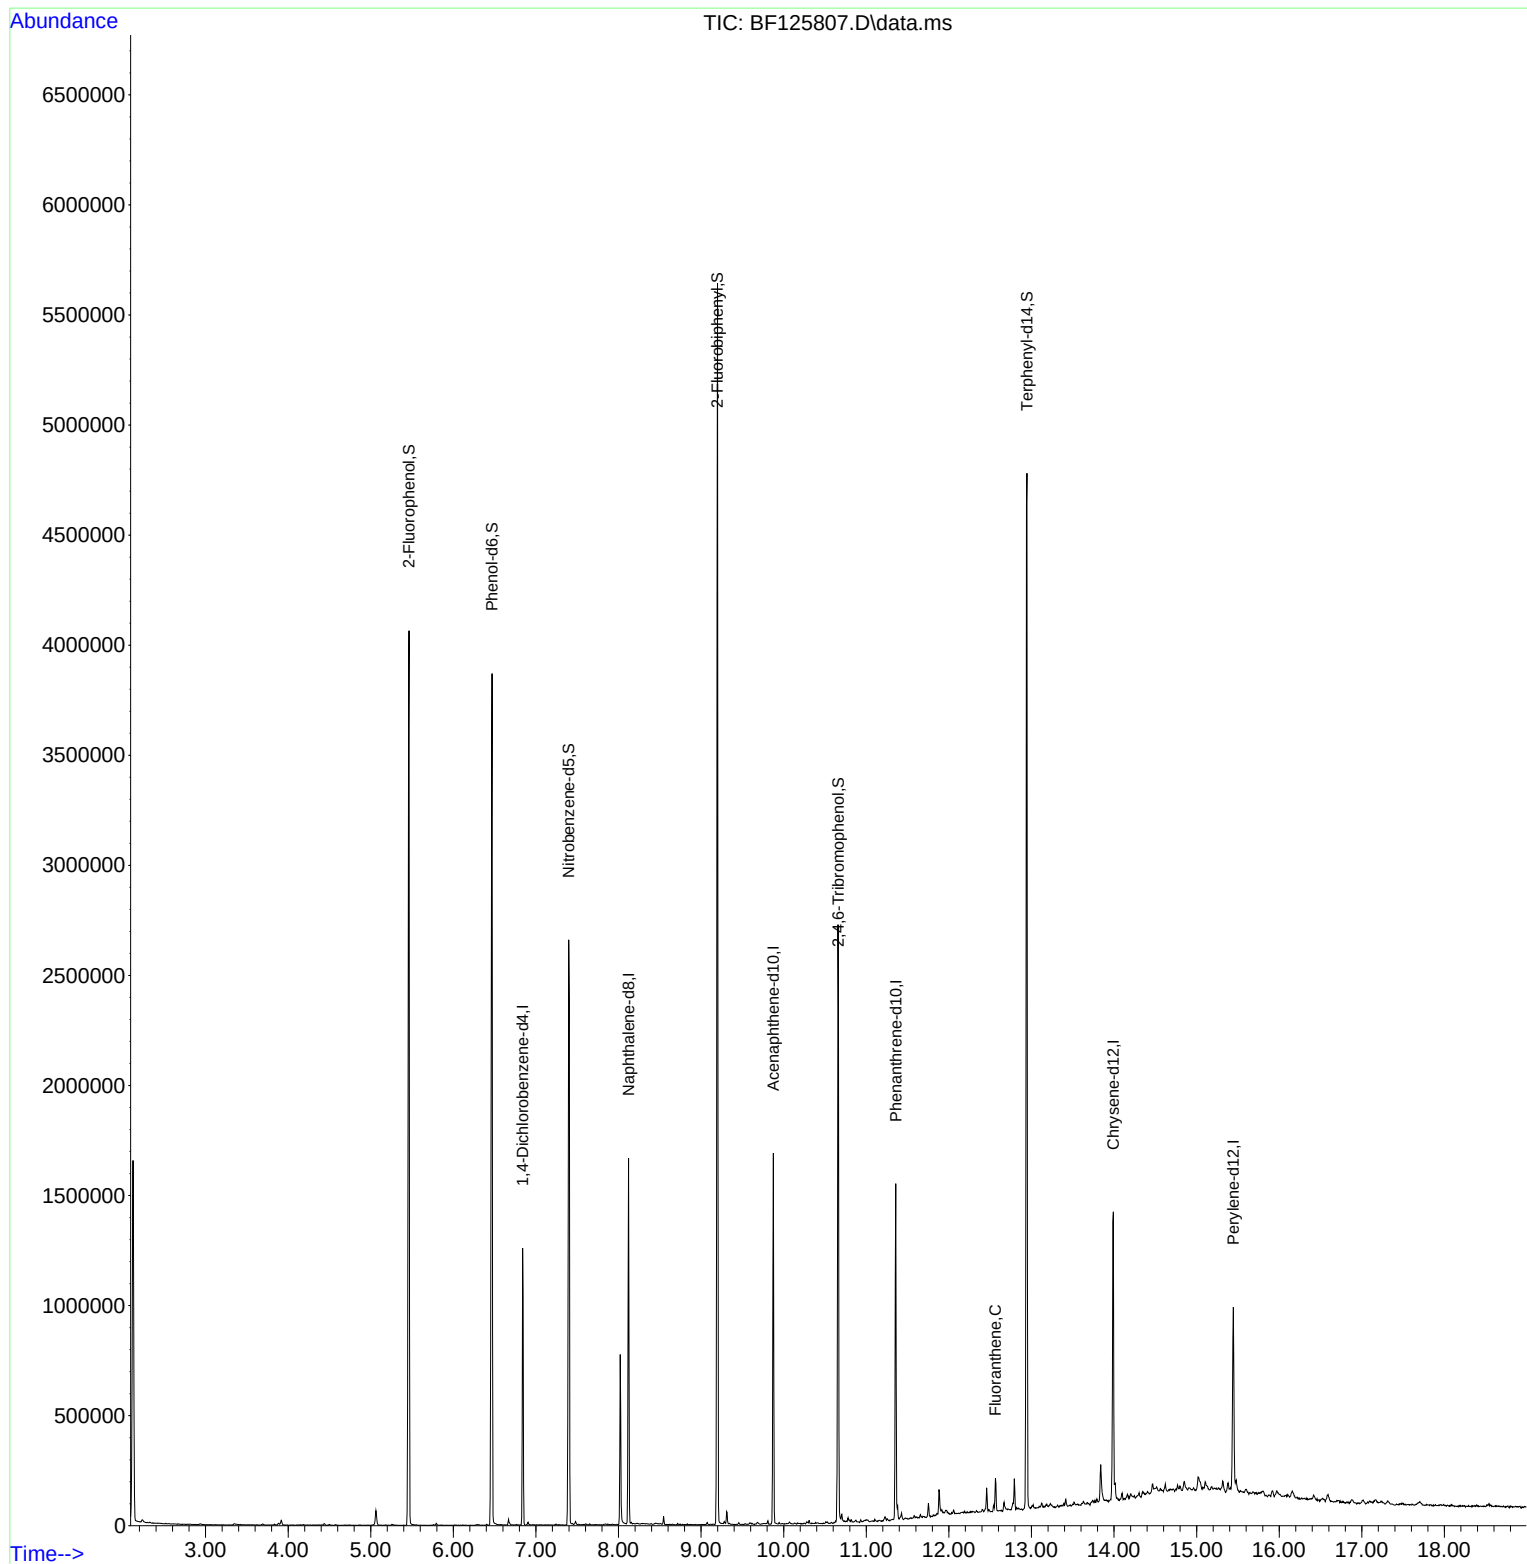


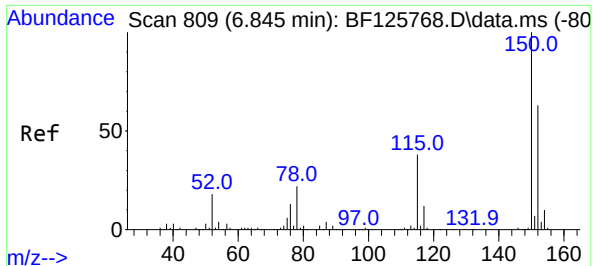

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.840 min Scan# 808
Delta R.T. -0.005 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion:152 Resp: 186260
Ion Ratio Lower Upper
152 100
150 161.8 117.6 176.4
115 61.7 47.1 70.7

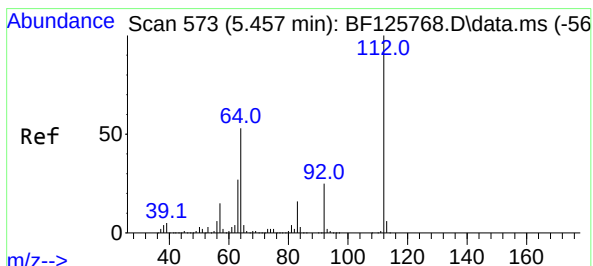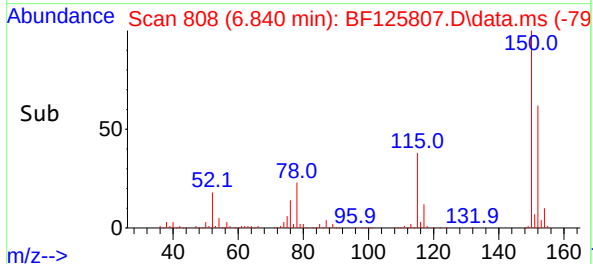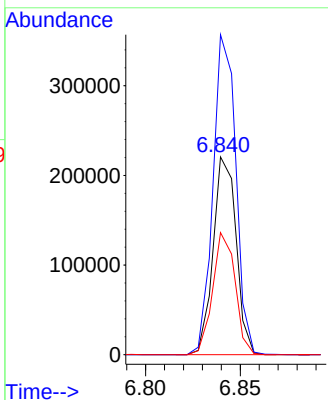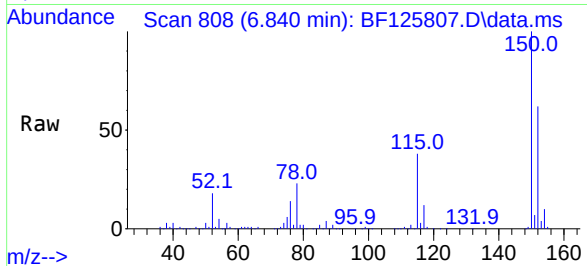

#5
2-Fluorophenol
Concen: 111.96 ng
RT: 5.463 min Scan# 574
Delta R.T. 0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion:112 Resp: 1276576
Ion Ratio Lower Upper
112 100
64 51.5 44.2 66.2
63 25.1 26.2 39.2#


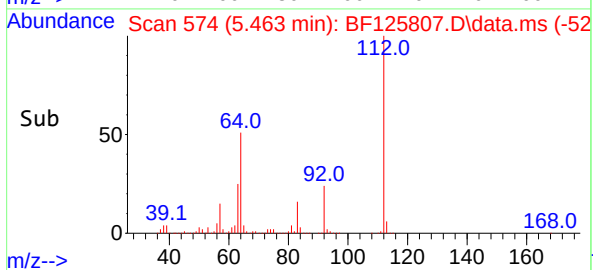
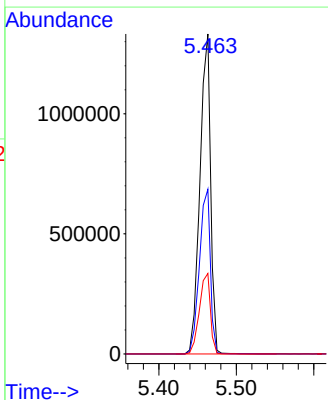
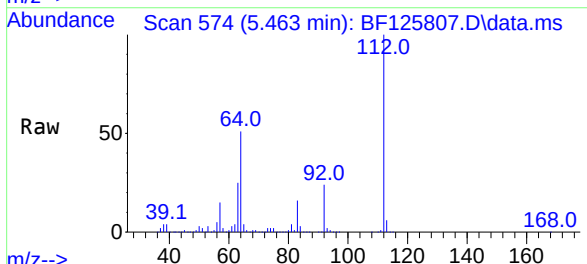


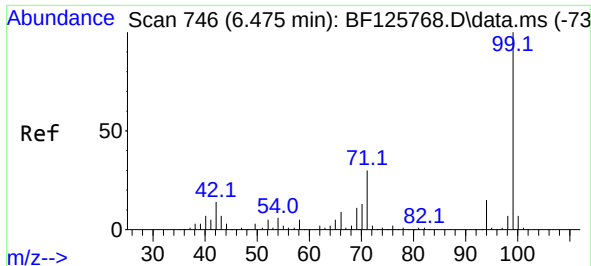

#7
Phenol-d6
Concen: 103.60 ng
RT: 6.469 min Scan# 745
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion: 99 Resp: 1520557
Ion Ratio Lower Upper
99 100
42 14.2 23.5 35.3#
71 29.2 25.6 38.4

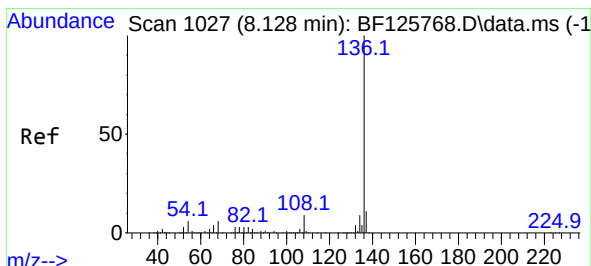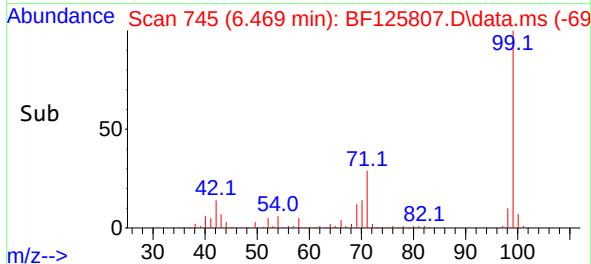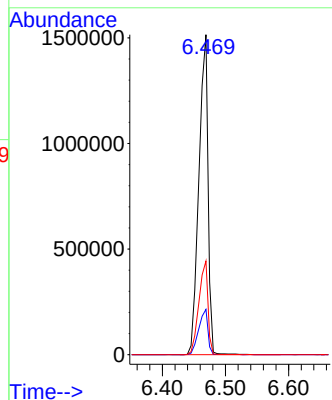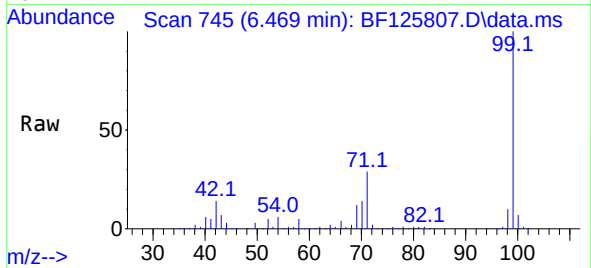

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion: 136 Resp: 691402
Ion Ratio Lower Upper
136 100
137 10.6 9.8 14.6
54 6.5 6.4 9.6
68 5.7 3.3 4.9#


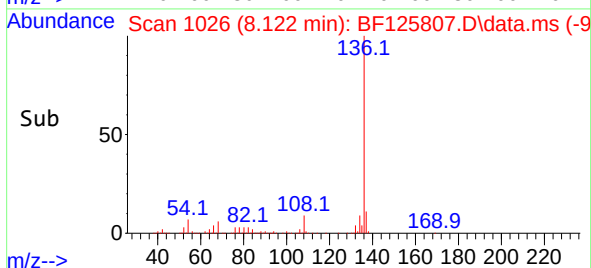
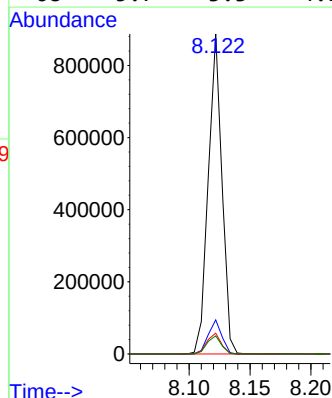
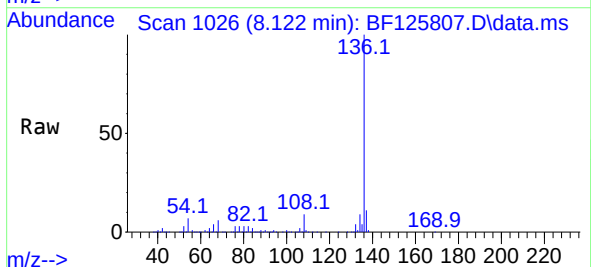


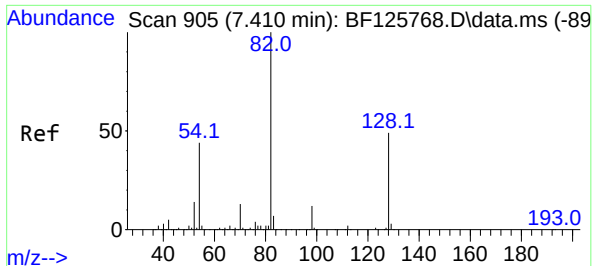

#23
Nitrobenzene-d5
Concen: 83.09 ng
RT: 7.398 min Scan# 903
Delta R.T. -0.012 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion: 82 Resp: 924196
Ion Ratio Lower Upper
82 100
128 46.9 40.6 60.8
54 44.7 49.6 74.4#

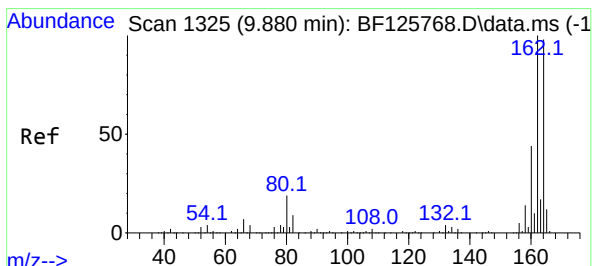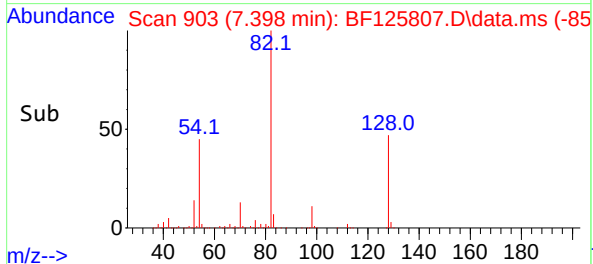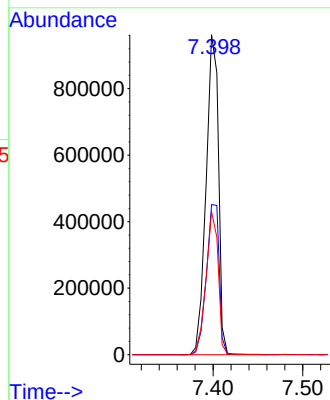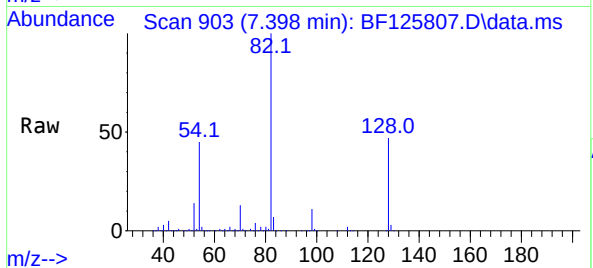

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.875 min Scan# 1324
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion: 164 Resp: 322385
Ion Ratio Lower Upper
164 100
162 100.1 81.3 121.9
160 43.4 38.0 57.0


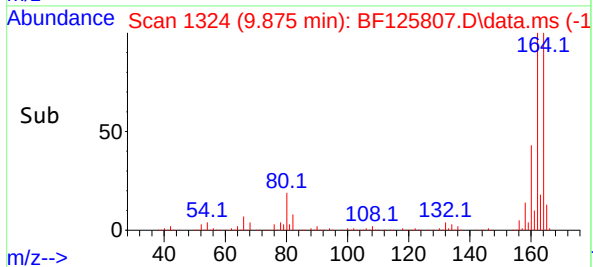
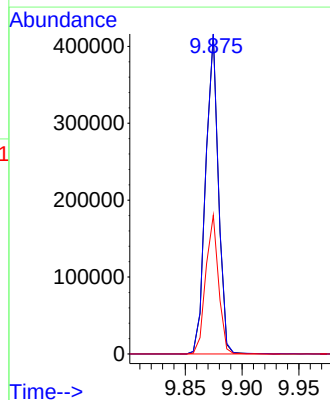
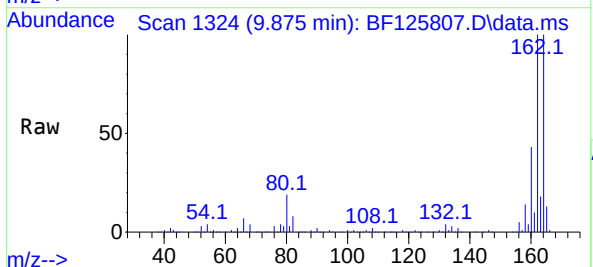


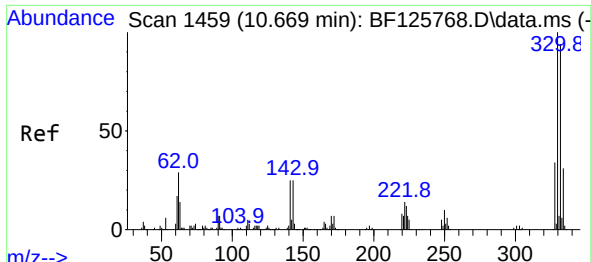

#42
2,4,6-Tribromophenol
Concen: 111.05 ng
RT: 10.663 min Scan# 1458
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion:330 Resp: 353457
Ion Ratio Lower Upper
330 100
332 96.0 76.2 114.4
141 31.6 44.6 66.8#

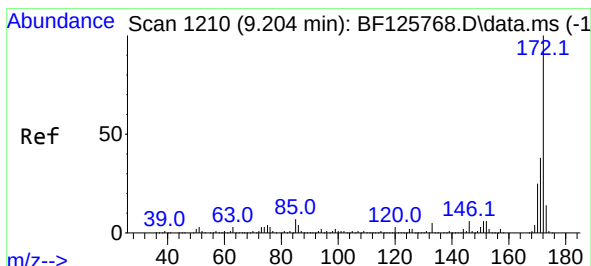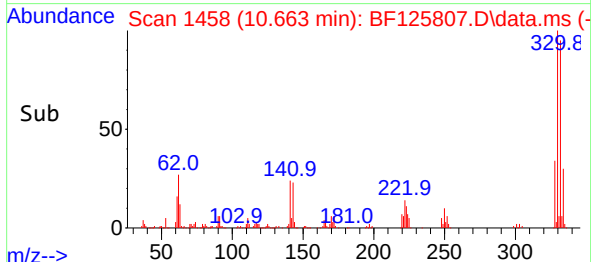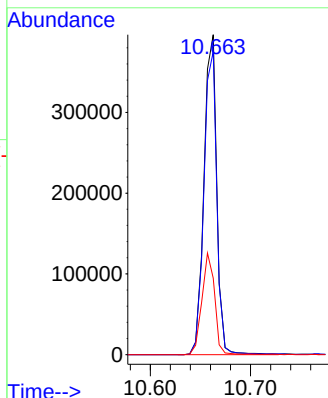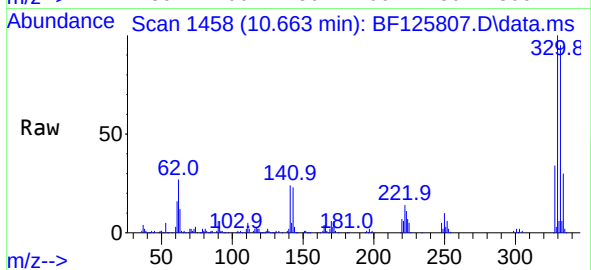

#45
2-Fluorobiphenyl
Concen: 89.44 ng
RT: 9.198 min Scan# 1209
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion:172 Resp: 1671662
Ion Ratio Lower Upper
172 100
171 36.3 26.5 39.7
170 24.5 18.8 28.2


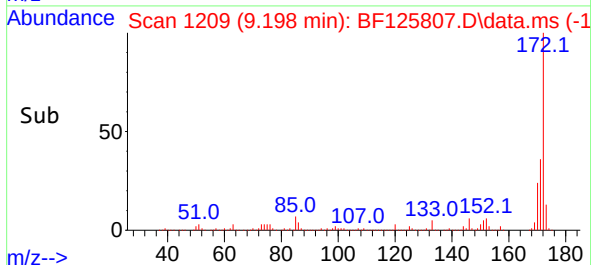
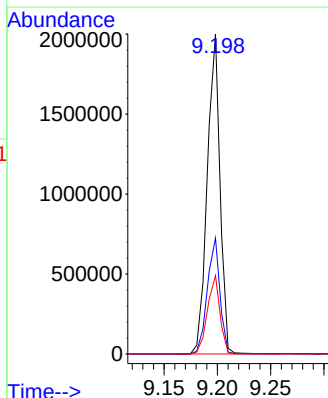
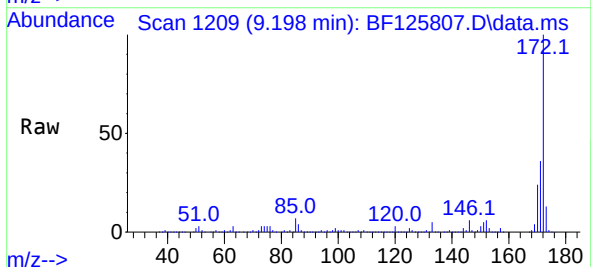


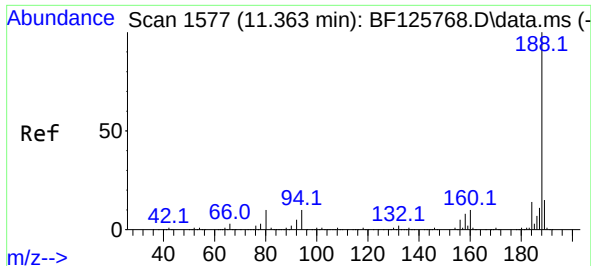

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.357 min Scan# 1576
Delta R.T. -0.006 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion:188 Resp: 520687
Ion Ratio Lower Upper
188 100
94 9.9 6.7 10.1
80 10.2 7.5 11.3

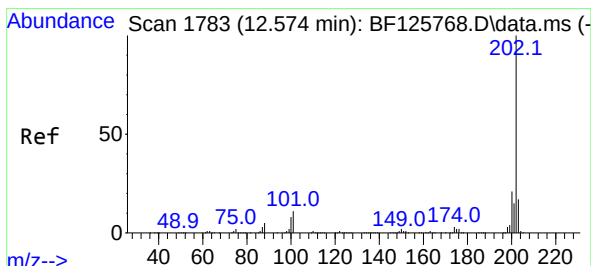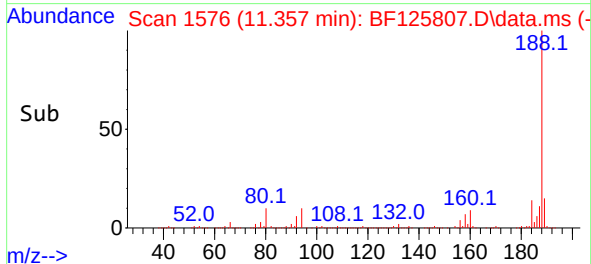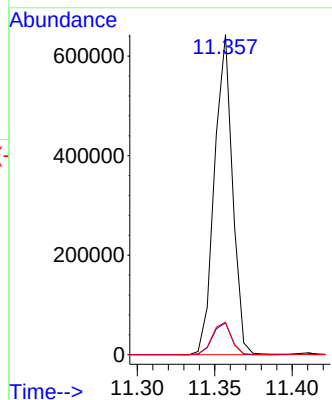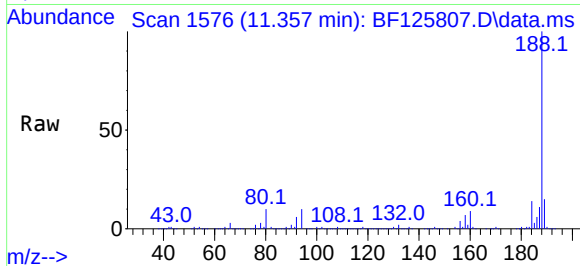

#75
Fluoranthene
Concen: 2.23 ng
RT: 12.563 min Scan# 1781
Delta R.T. -0.012 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion:202 Resp: 55968
Ion Ratio Lower Upper
202 100
101 14.8 0.0 30.7
203 18.1 0.0 36.3


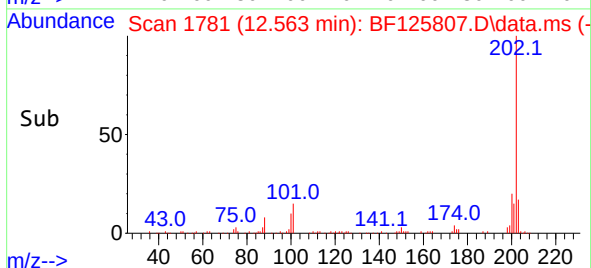
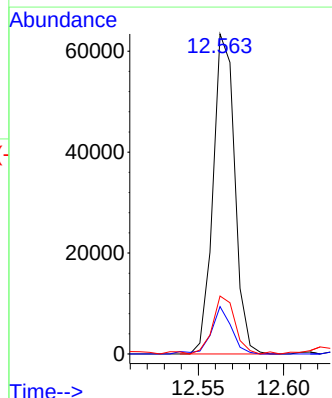
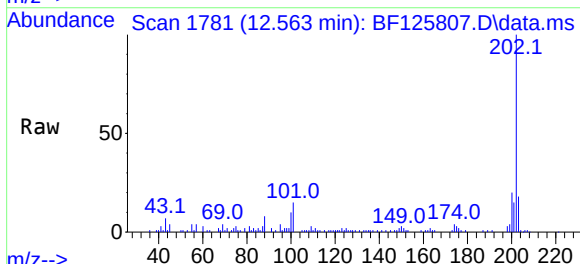


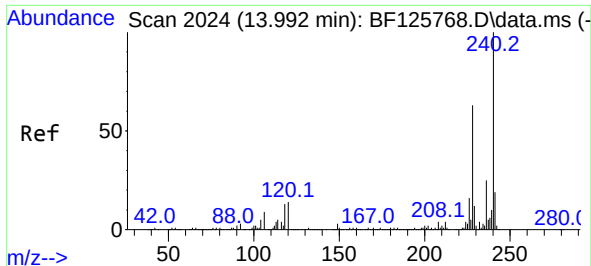

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.992 min Scan# 2024
Delta R.T. 0.000 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59




Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)


Tgt Ion:240 Resp: 447138
Ion Ratio Lower Upper
240 100
120 11.6 10.8 16.2
236 24.8 21.6 32.4

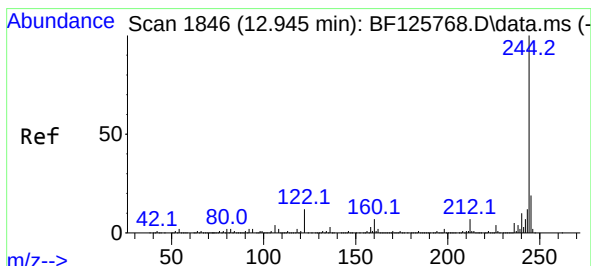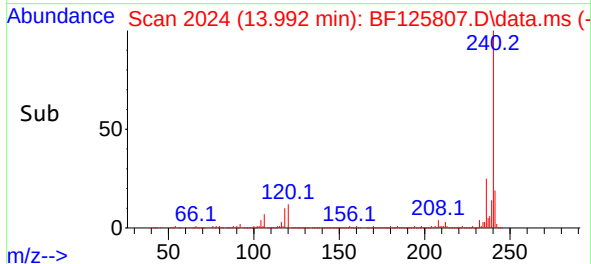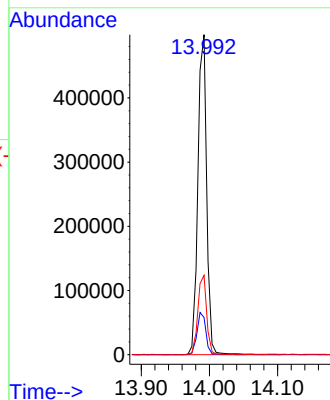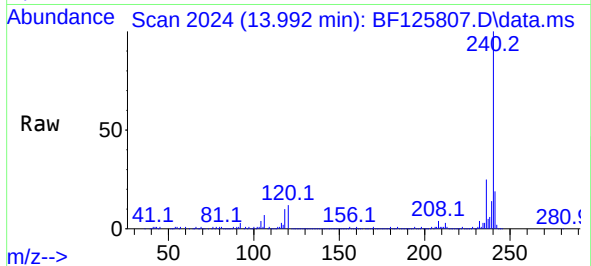

#79
Terphenyl-d14
Concen: 58.46 ng
RT: 12.945 min Scan# 1846
Delta R.T. 0.000 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Tgt Ion:244 Resp: 1716111
Ion Ratio Lower Upper
244 100
212 6.6 5.9 8.9
122 11.2 9.0 13.4

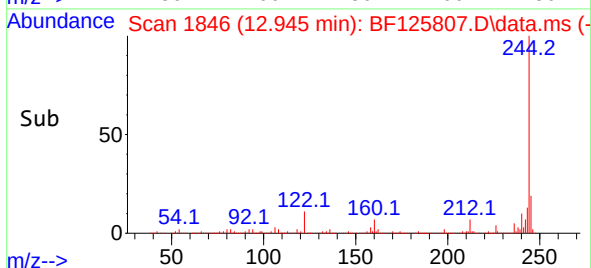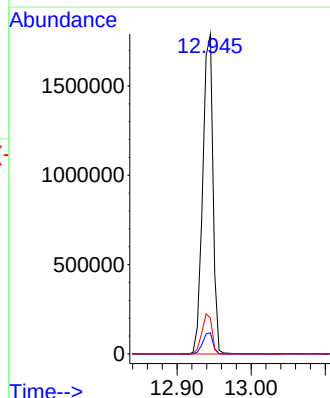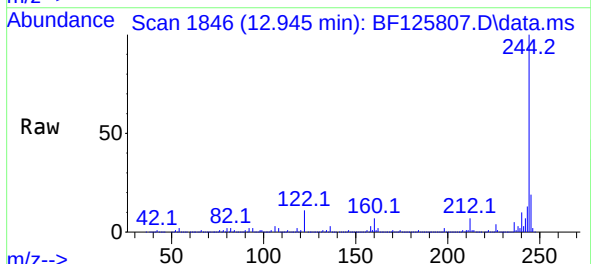

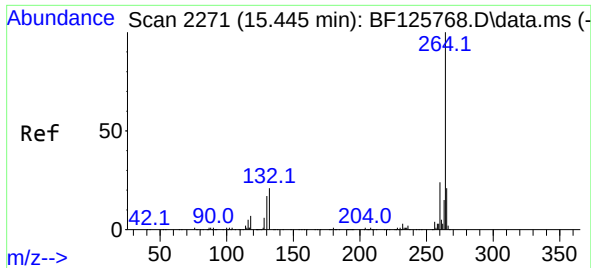

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.445 min Scan# 2271
Delta R.T. 0.000 min
Lab File: BF125807.D
Acq: 12 Oct 2021 17:59

Instrument :
BNA_F
ClientSampleId :
T10-COMP-(1-4)

Tgt Ion:264 Resp: 361790

Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.6	29.4
265	21.7	17.2	25.8

