

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101221\  
 Data File : BF125813.D  
 Acq On : 12 Oct 2021 21:11  
 Operator : JU/CG  
 Sample : M4117-01 5X  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SB-1(1.5-2.0)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF100721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125813.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.893       | 302           | 307         | 312          | rVB      | 15049          | 20614         | 1.61%           | 0.192%        |
| 2         | 5.451       | 568           | 572         | 581          | rBV      | 698846         | 657608        | 51.24%          | 6.118%        |
| 3         | 6.457       | 740           | 743         | 747          | rBV      | 740151         | 626155        | 48.79%          | 5.825%        |
| 4         | 6.845       | 805           | 809         | 812          | rBV      | 1201367        | 1052299       | 82.00%          | 9.790%        |
| 5         | 7.398       | 899           | 903         | 906          | rBV      | 472837         | 383563        | 29.89%          | 3.569%        |
| 6         | 8.022       | 1006          | 1009        | 1014         | rBV      | 54085          | 54240         | 4.23%           | 0.505%        |
| 7         | 8.122       | 1023          | 1026        | 1030         | rBV      | 1691472        | 1283264       | 100.00%         | 11.939%       |
| 8         | 9.192       | 1205          | 1208        | 1212         | rBV      | 859662         | 746351        | 58.16%          | 6.944%        |
| 9         | 9.875       | 1320          | 1324        | 1328         | rBV      | 1664799        | 1263292       | 98.44%          | 11.753%       |
| 10        | 10.657      | 1453          | 1457        | 1463         | rBV      | 498408         | 409164        | 31.88%          | 3.807%        |
| 11        | 11.357      | 1572          | 1576        | 1580         | rBV      | 1547125        | 1254968       | 97.79%          | 11.676%       |
| 12        | 11.886      | 1662          | 1666        | 1668         | rBV2     | 39599          | 41562         | 3.24%           | 0.387%        |
| 13        | 12.569      | 1779          | 1782        | 1784         | rBV      | 29987          | 28297         | 2.21%           | 0.263%        |
| 14        | 12.669      | 1797          | 1799        | 1803         | rBV5     | 21994          | 30406         | 2.37%           | 0.283%        |
| 15        | 12.939      | 1841          | 1845        | 1848         | rBV      | 988125         | 803377        | 62.60%          | 7.474%        |
| 16        | 13.992      | 2020          | 2024        | 2027         | rBV      | 1426915        | 1226846       | 95.60%          | 11.414%       |
| 17        | 15.451      | 2268          | 2272        | 2276         | rVB      | 714537         | 866550        | 67.53%          | 8.062%        |




Sum of corrected areas: 10748556

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101221\  
Data File : BF125813.D  
Acq On : 12 Oct 2021 21:11  
Operator : JU/CG  
Sample : M4117-01 5X  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB-1(1.5-2.0)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF100721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

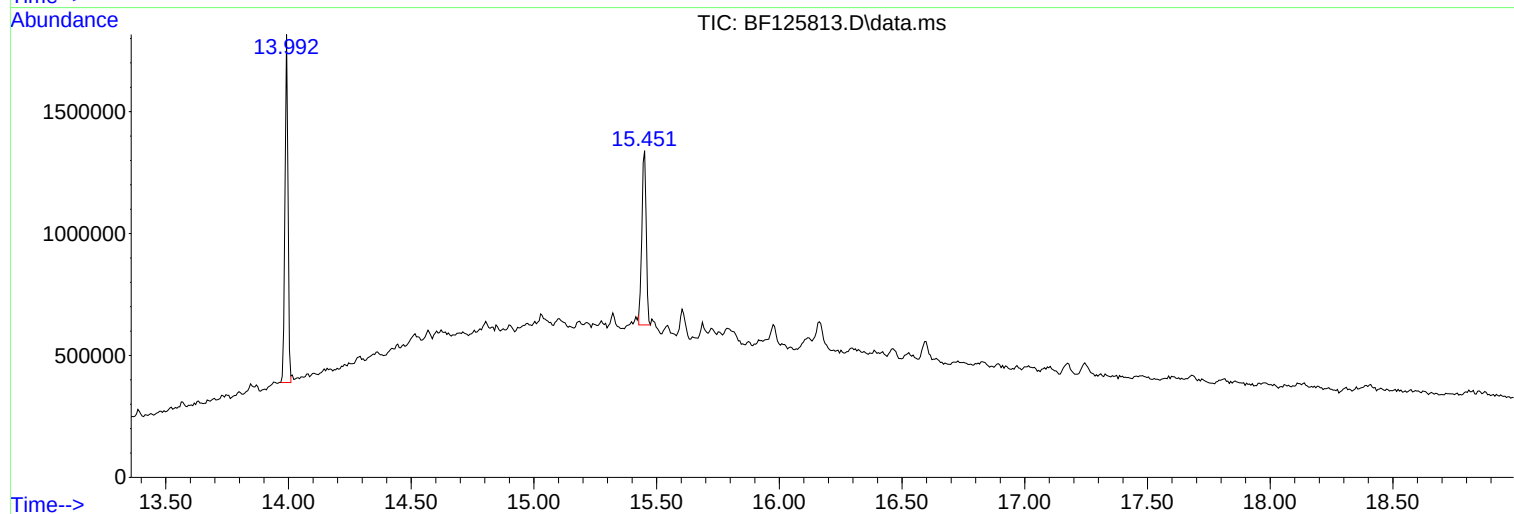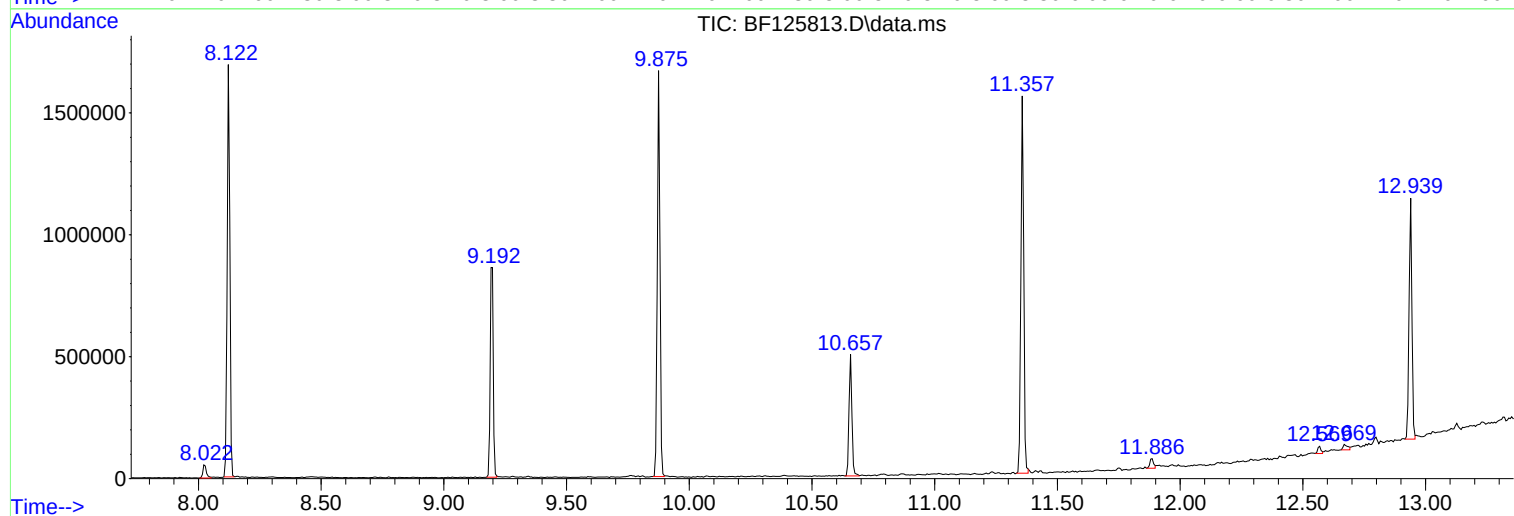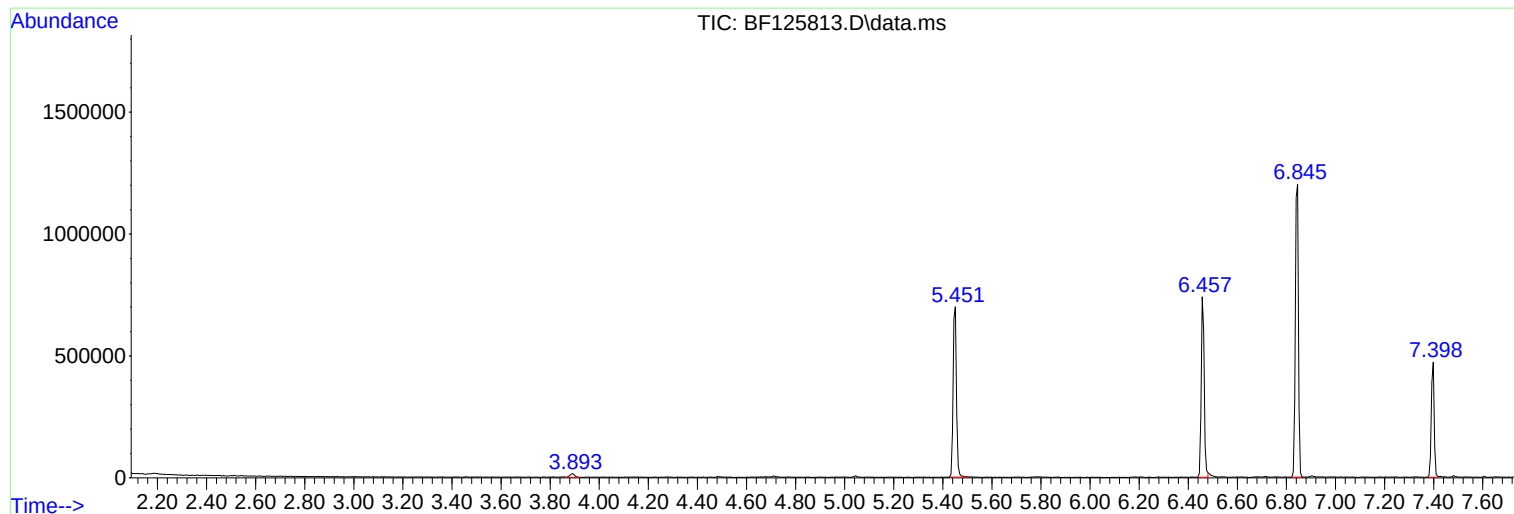

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101221\  
Data File : BF125813.D  
Acq On : 12 Oct 2021 21:11  
Operator : JU/CG  
Sample : M4117-01 5X  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB-1(1.5-2.0)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF100721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101221\  
Data File : BF125813.D  
Acq On : 12 Oct 2021 21:11  
Operator : JU/CG  
Sample : M4117-01 5X  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB-1(1.5-2.0)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF100721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----