

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125814.D
 Acq On : 12 Oct 2021 21:42
 Operator : JU/CG
 Sample : M4164-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-03-100821

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	568	572	583	rVB	362098	350604	24.68%	3.581%
2	6.457	740	743	747	rBV	395976	334517	23.54%	3.416%
3	6.845	805	809	812	rBV	1347906	1120429	78.86%	11.443%
4	7.398	899	903	906	rBV	246503	205056	14.43%	2.094%
5	8.022	1007	1009	1018	rBV	28282	30192	2.12%	0.308%
6	8.122	1023	1026	1030	rVV	1778460	1402675	98.72%	14.326%
7	9.192	1205	1208	1212	rBV	499973	437249	30.77%	4.466%
8	9.875	1320	1324	1328	rBV	1853908	1420820	100.00%	14.511%
9	10.657	1454	1457	1461	rBV	257933	203276	14.31%	2.076%
10	11.357	1573	1576	1579	rBV	1647083	1330919	93.67%	13.593%
11	11.751	1639	1643	1646	rBV	28999	29451	2.07%	0.301%
12	11.880	1663	1665	1670	rBV3	21584	23835	1.68%	0.243%
13	12.439	1757	1760	1762	rBV	73658	66073	4.65%	0.675%
14	12.457	1762	1763	1766	rVB2	59843	48203	3.39%	0.492%
15	12.545	1775	1778	1780	rBV	25718	24614	1.73%	0.251%
16	12.568	1780	1782	1785	rVB	28982	24260	1.71%	0.248%
17	12.798	1818	1821	1823	rBV	39171	38025	2.68%	0.388%
18	12.939	1841	1845	1848	rBV	558217	440181	30.98%	4.496%
19	13.992	2020	2024	2028	rBV	1459064	1284744	90.42%	13.121%
20	15.451	2267	2272	2277	rBV	806591	976141	68.70%	9.970%


Sum of corrected areas: 9791264

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125814.D
Acq On : 12 Oct 2021 21:42
Operator : JU/CG
Sample : M4164-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-03-100821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

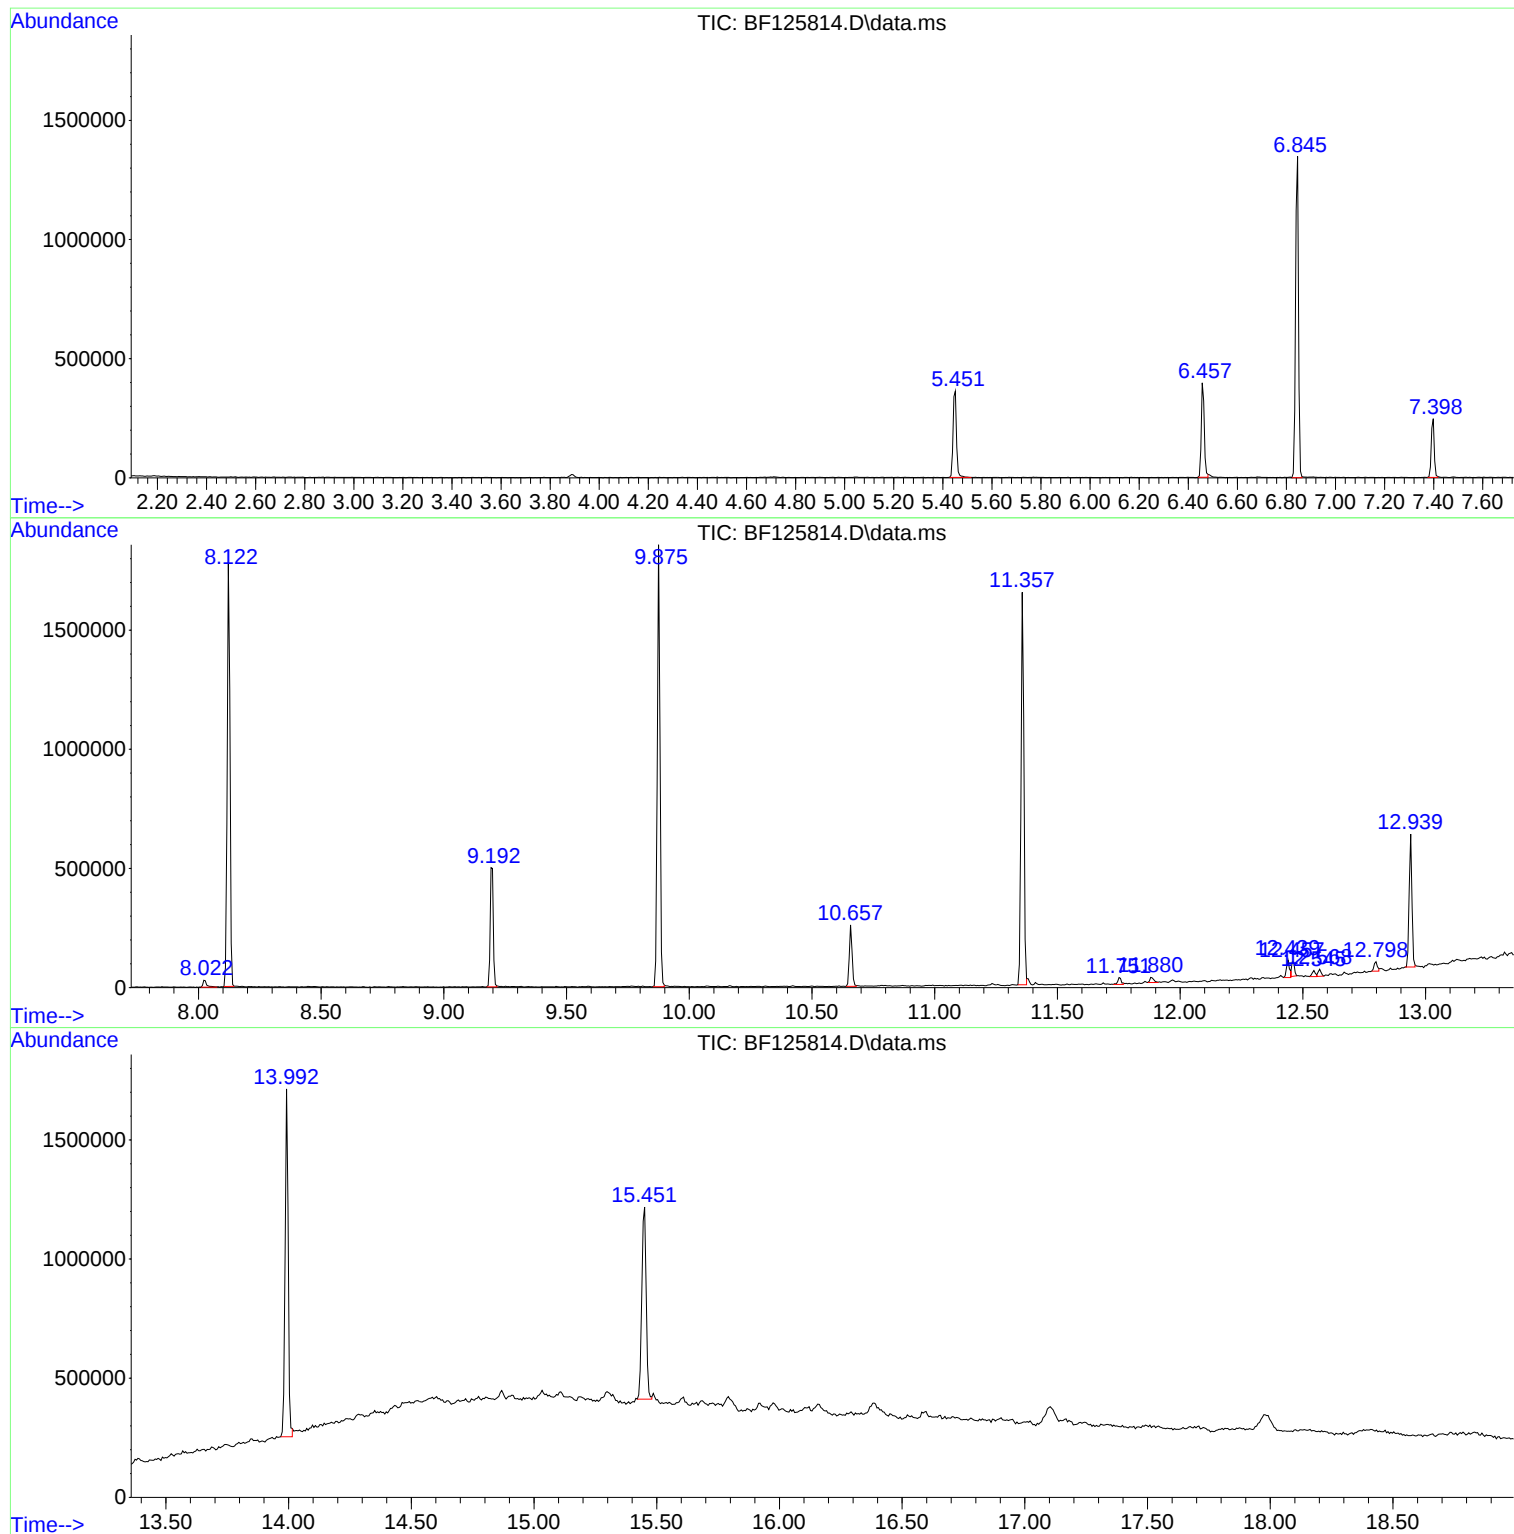

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125814.D
Acq On : 12 Oct 2021 21:42
Operator : JU/CG
Sample : M4164-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-03-100821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125814.D
Acq On : 12 Oct 2021 21:42
Operator : JU/CG
Sample : M4164-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-03-100821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
