
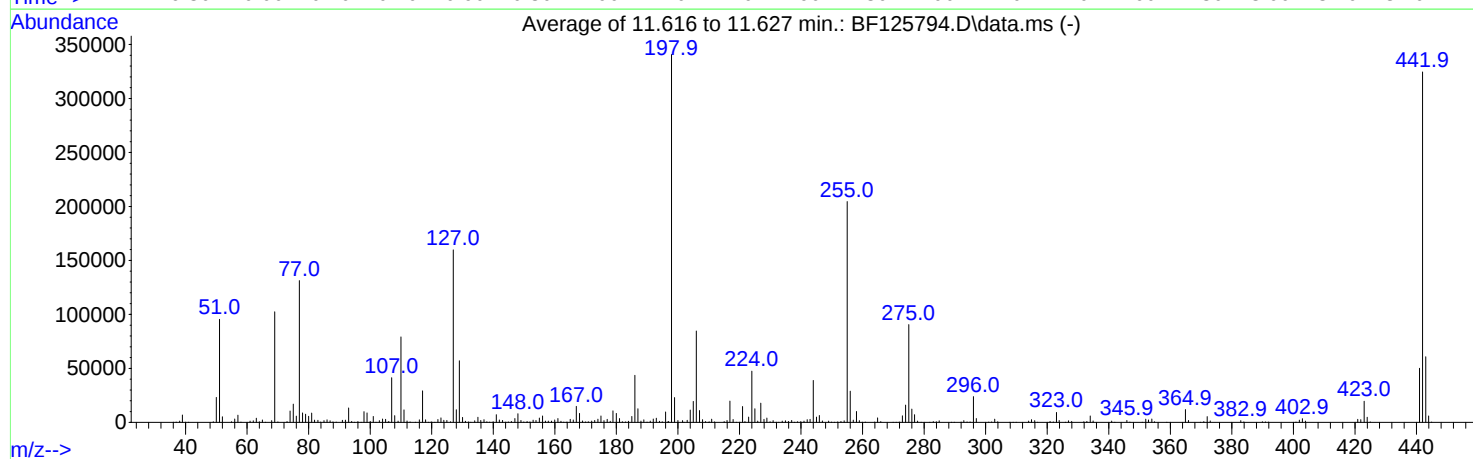


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125794.D
 Acq On : 12 Oct 2021 10:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 13 13:23:32 2021

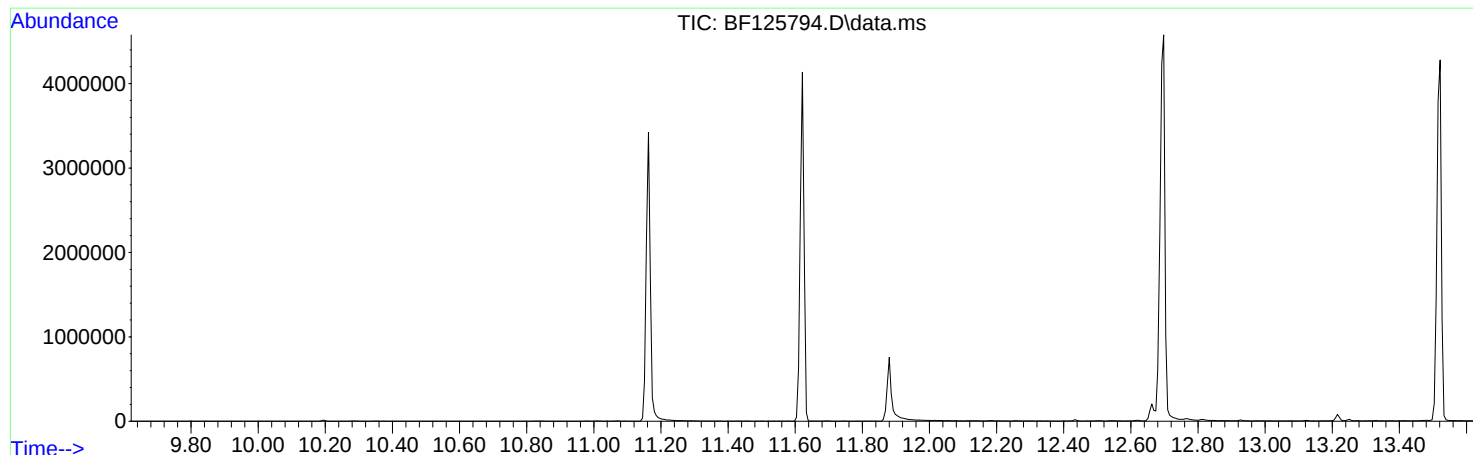




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	95512	PASS
68	69	0.00	2	1.7	1702	PASS
69	198	0.00	100	30.0	102373	PASS
70	69	0.00	2	0.5	491	PASS
127	198	10	80	46.9	159717	PASS
197	198	0.00	2	0.3	954	PASS
198	198	100	100	100.0	340736	PASS
199	198	5	9	6.7	22998	PASS
275	198	10	60	26.6	90560	PASS
365	198	1	100	3.5	11837	PASS
441	198	0.01	100	14.7	50080	PASS
442	442	50	100	100.0	324523	PASS
443	442	15	24	18.7	60835	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
 Data File : BF125794.D
 Acq On : 12 Oct 2021 10:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 12 18:13:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

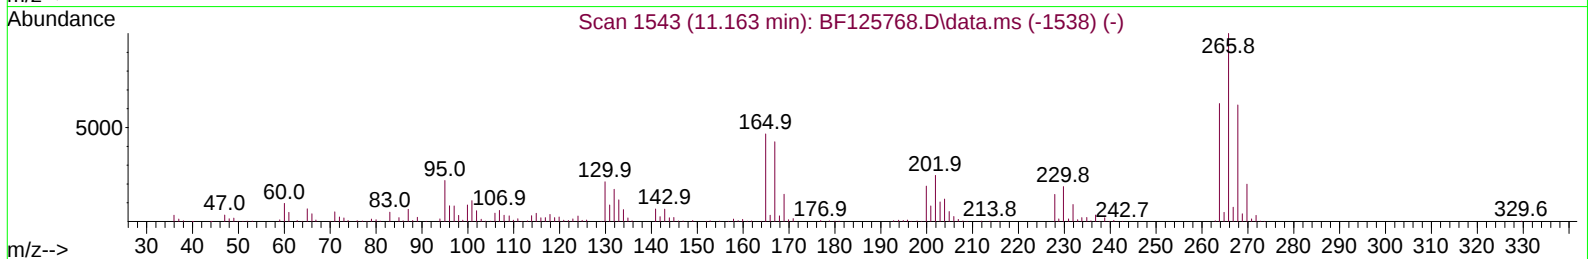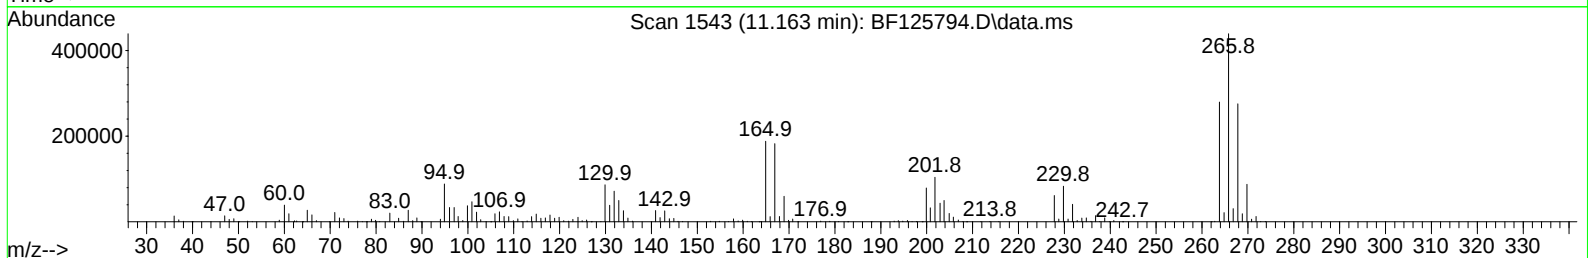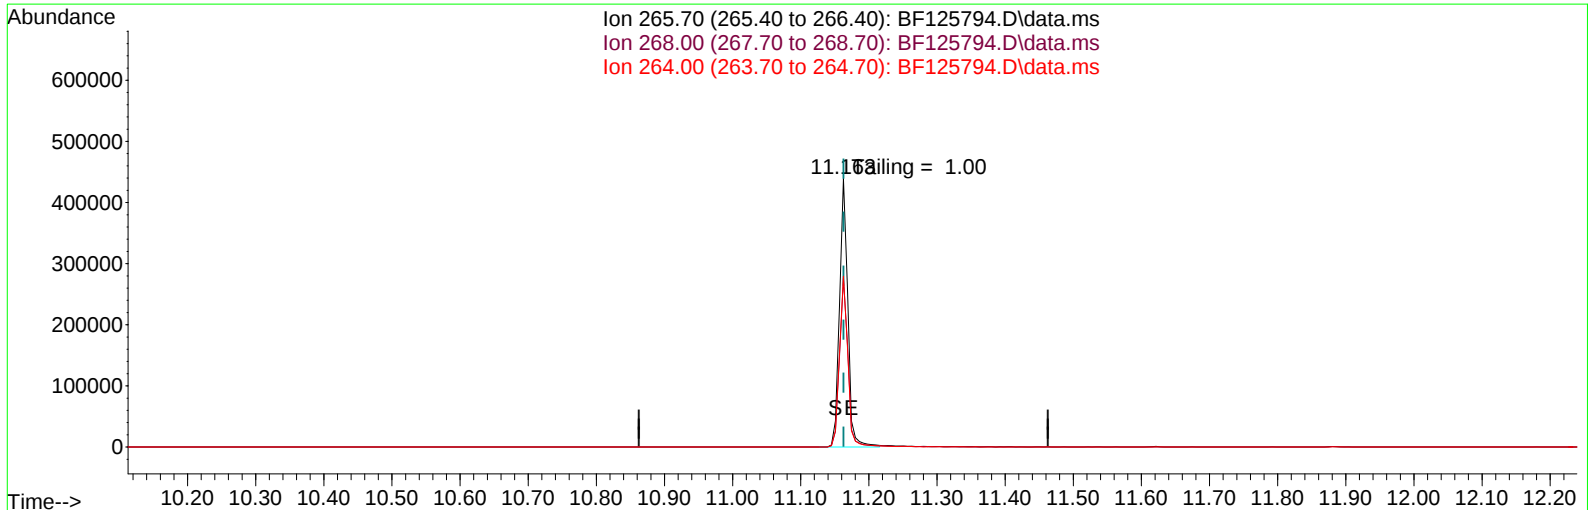

TIC: BF125794.D\data.ms

(70) Pentachlorophenol (C)

11.163min (0.000) 458254.10 ng




response 378157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.79
264.00	69.90	63.65
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\  
Data File : BF125794.D  
Acq On    : 12 Oct 2021  10:29  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 12 18:13:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration

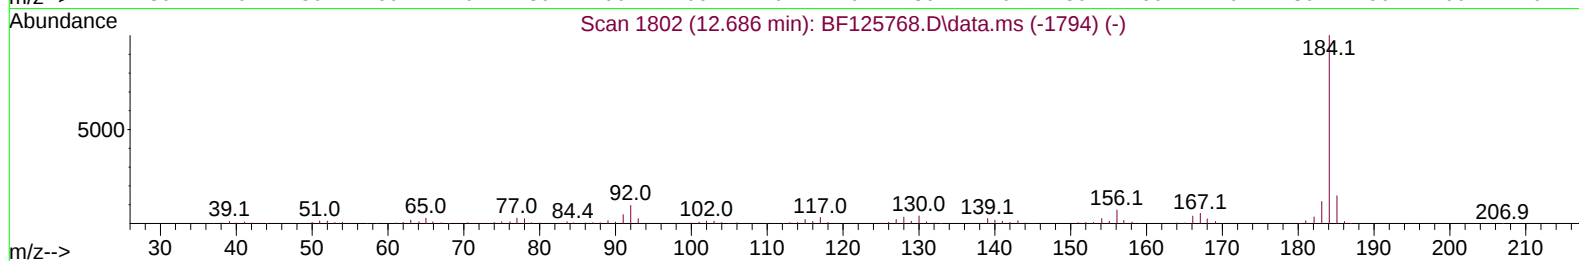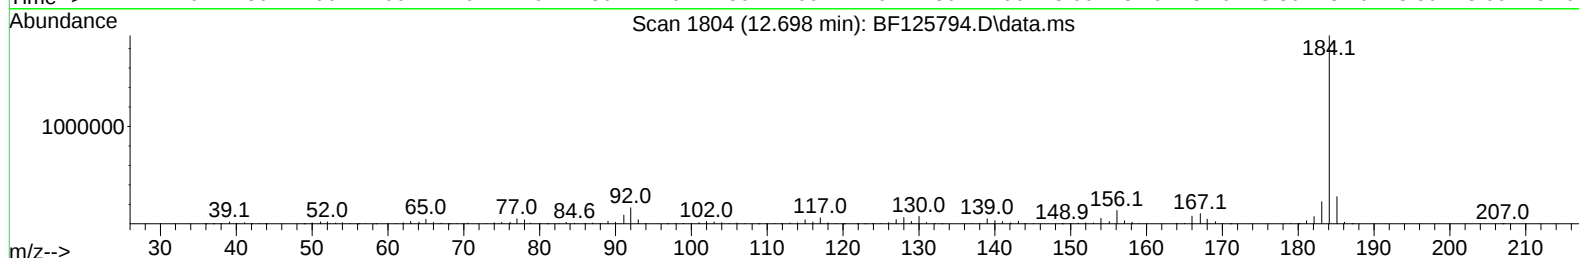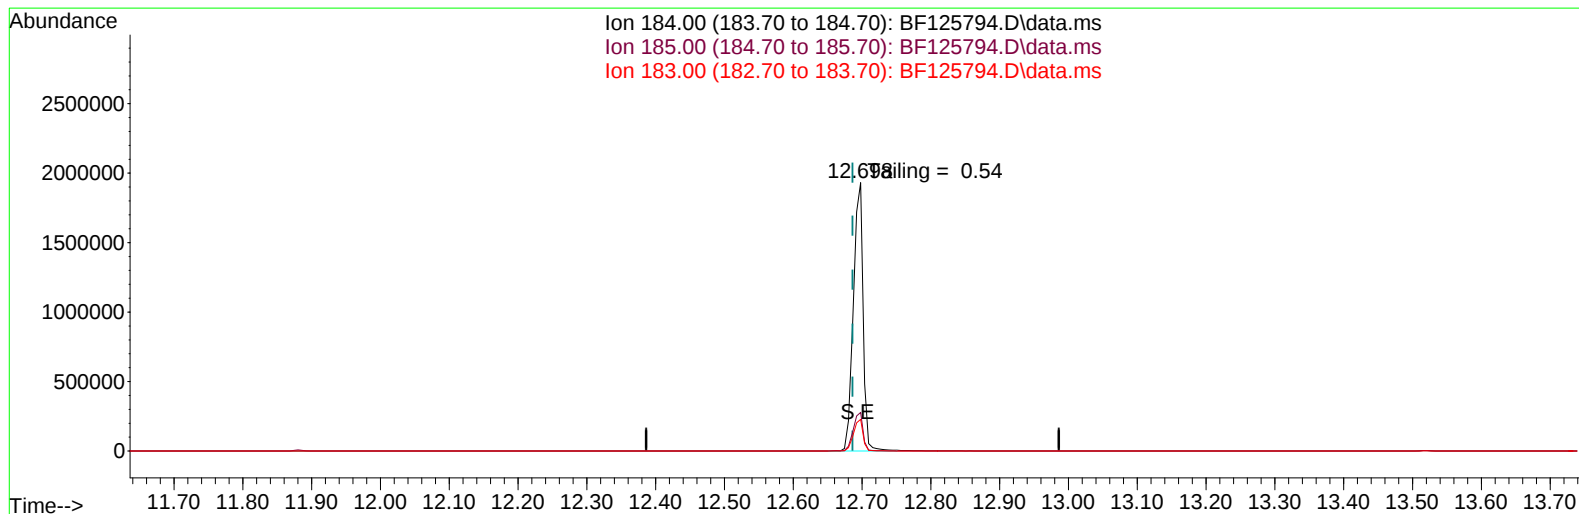

TIC: BF125794.D\data.ms

(77) Benzidine

12.698min (+ 0.012) 4896.67 ng m

response **1900688**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.38
183.00	10.10	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2021	BNA_F	<u>BF125794.D</u>
Compound Name	Response	Retention Time
DDT	784501	13.52
DDD	13292	13.21
DDE	328	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13620	798121	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP