
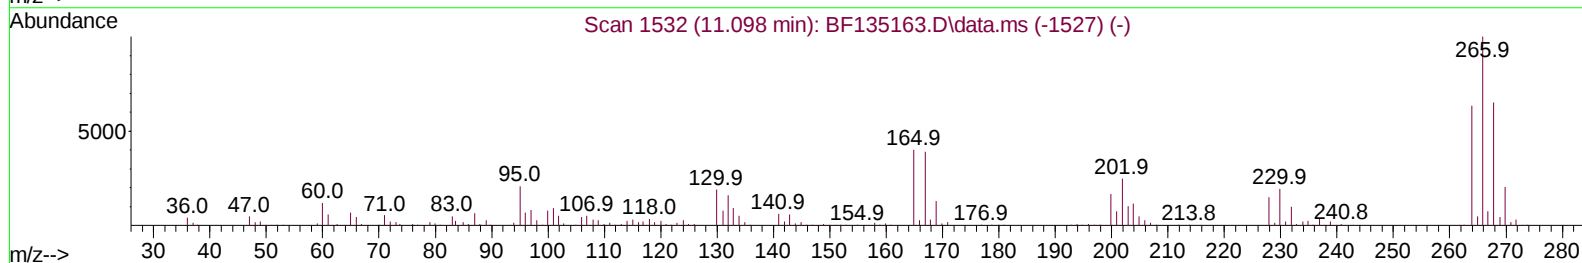
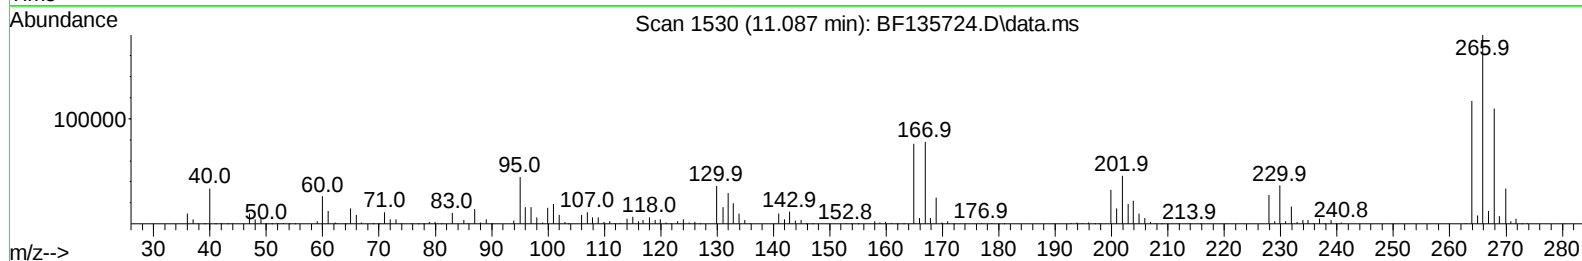


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135724.D
Acq On : 12 Oct 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 12:48:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

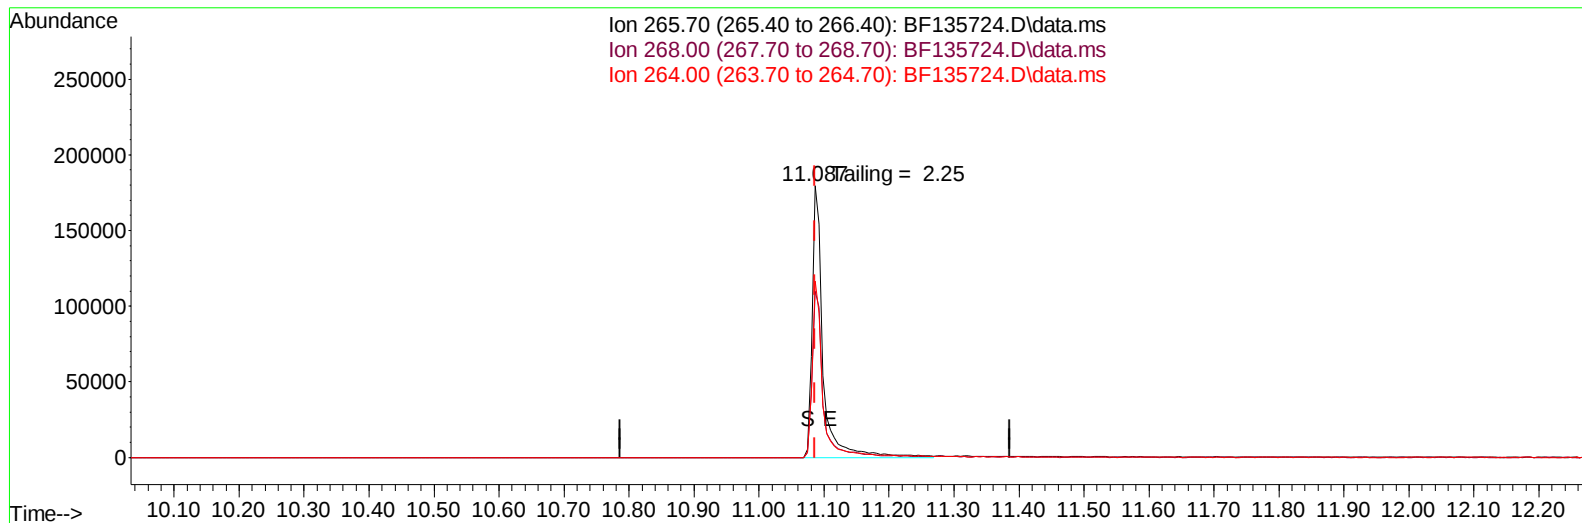

TIC: BF135724.D\data.ms

(70) Pentachlorophenol (C)




11.087min (+ 0.000) 595628.20 ng

response 209428

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.08
264.00	63.50	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135724.D
Acq On : 12 Oct 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 12:48:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

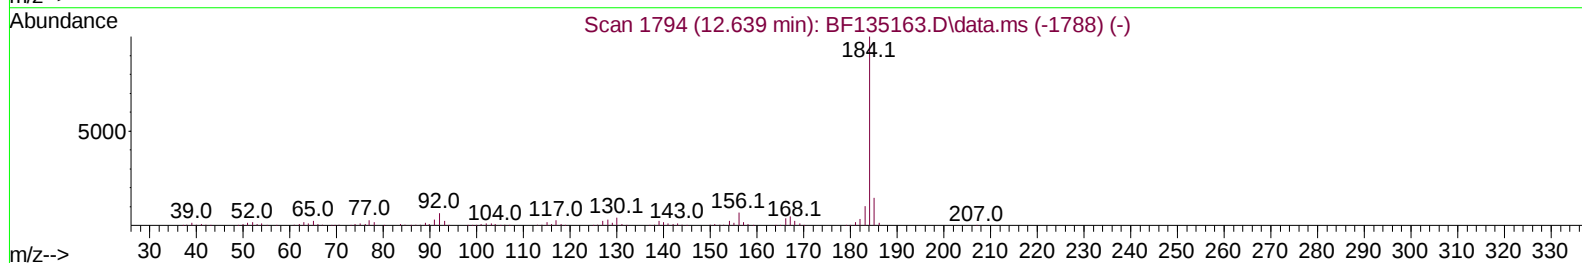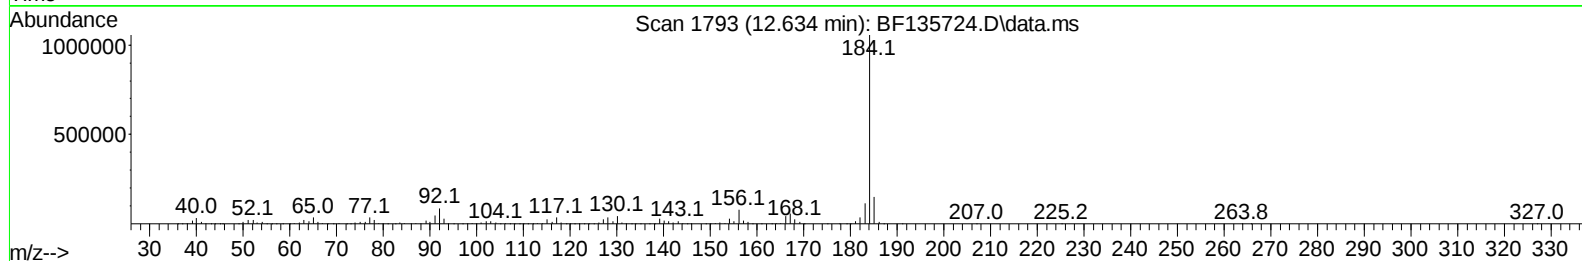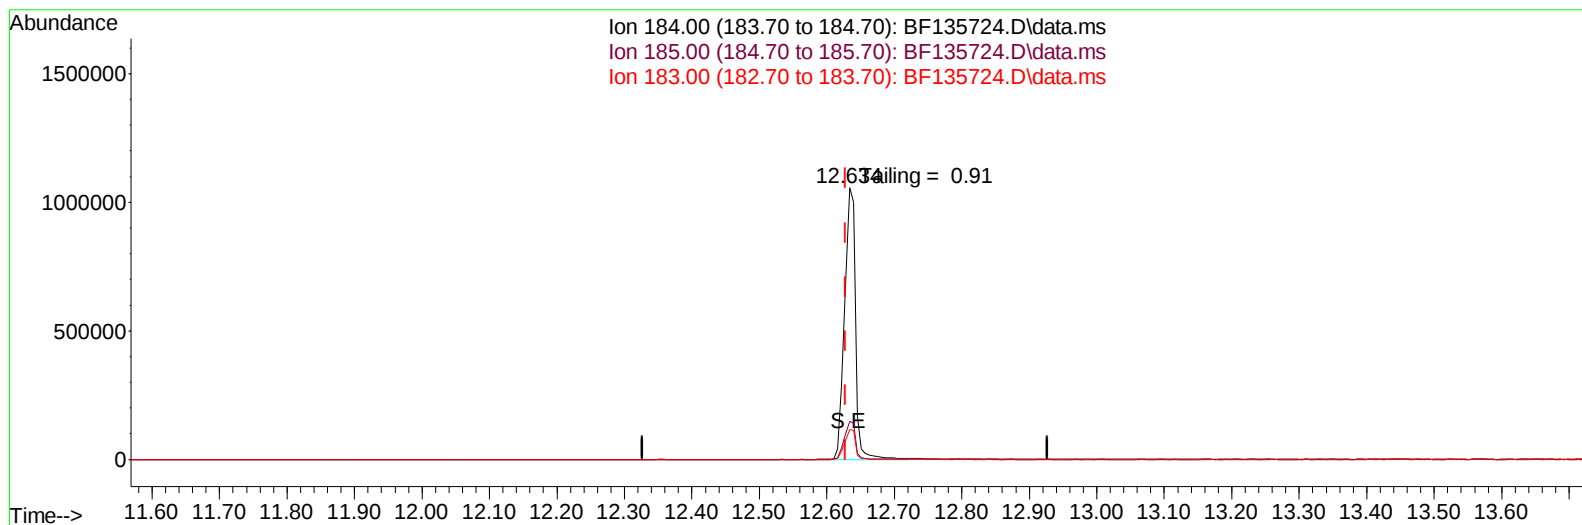

TIC: BF135724.D\data.ms

(77) Benzidine

12.634min (+ 0.006) 221863.09 ng

response 1186316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.14
183.00	10.30	10.92
0.00	0.00	0.00