

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
 Data File : BF135726.D
 Acq On : 12 Oct 2023 10:43
 Operator : CG\JU
 Sample : PB156073BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156073BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	557	561	586	rBV	3152236	3287851	86.68%	14.308%
2	6.392	728	732	750	rBV	2900177	3333322	87.87%	14.505%
3	6.739	787	791	798	rBV	651150	578492	15.25%	2.517%
4	7.310	883	888	904	rBV	2046852	2169840	57.20%	9.442%
5	8.016	1004	1008	1017	rBV	744579	727961	19.19%	3.168%
6	9.098	1186	1192	1195	rBV	3603721	3684982	97.15%	16.036%
7	9.775	1301	1307	1318	rBV	981067	869947	22.93%	3.786%
8	10.575	1439	1443	1454	rBV	2262952	2334095	61.53%	10.157%
9	11.274	1558	1562	1575	rVB	954227	963862	25.41%	4.194%
10	12.874	1829	1834	1837	rBV	3685677	3793261	100.00%	16.507%
11	13.933	2011	2014	2024	rBV	705820	735506	19.39%	3.201%
12	15.409	2261	2265	2277	rBV	332911	500718	13.20%	2.179%




Sum of corrected areas: 22979837

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135726.D
Acq On : 12 Oct 2023 10:43
Operator : CG\JU
Sample : PB156073BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

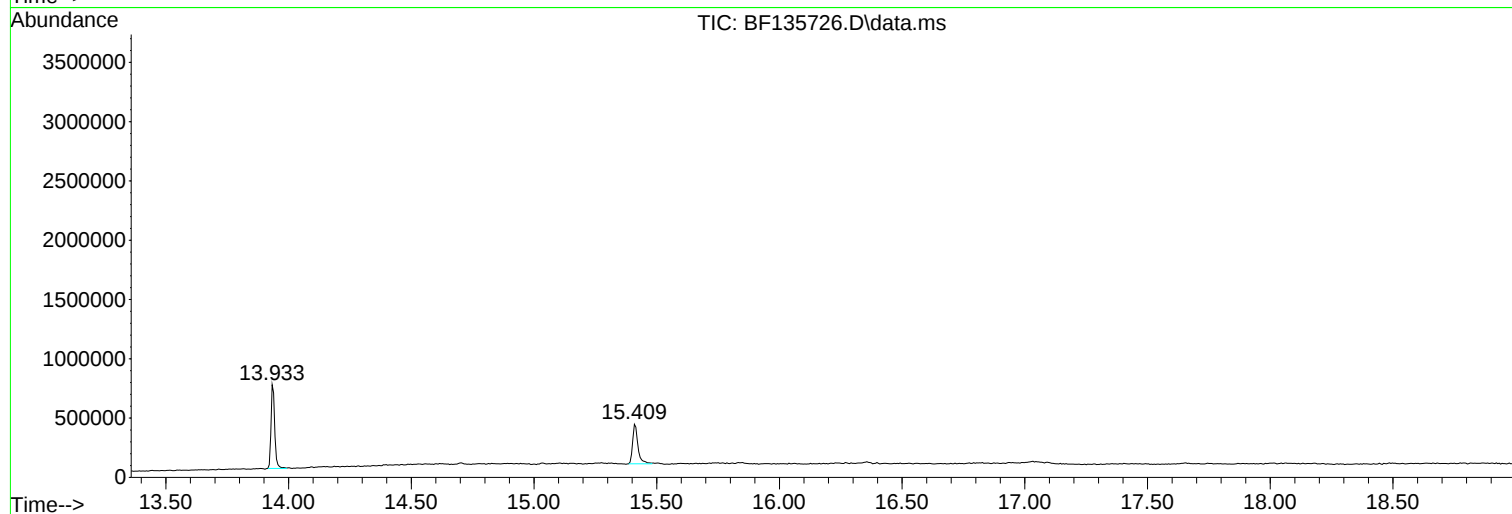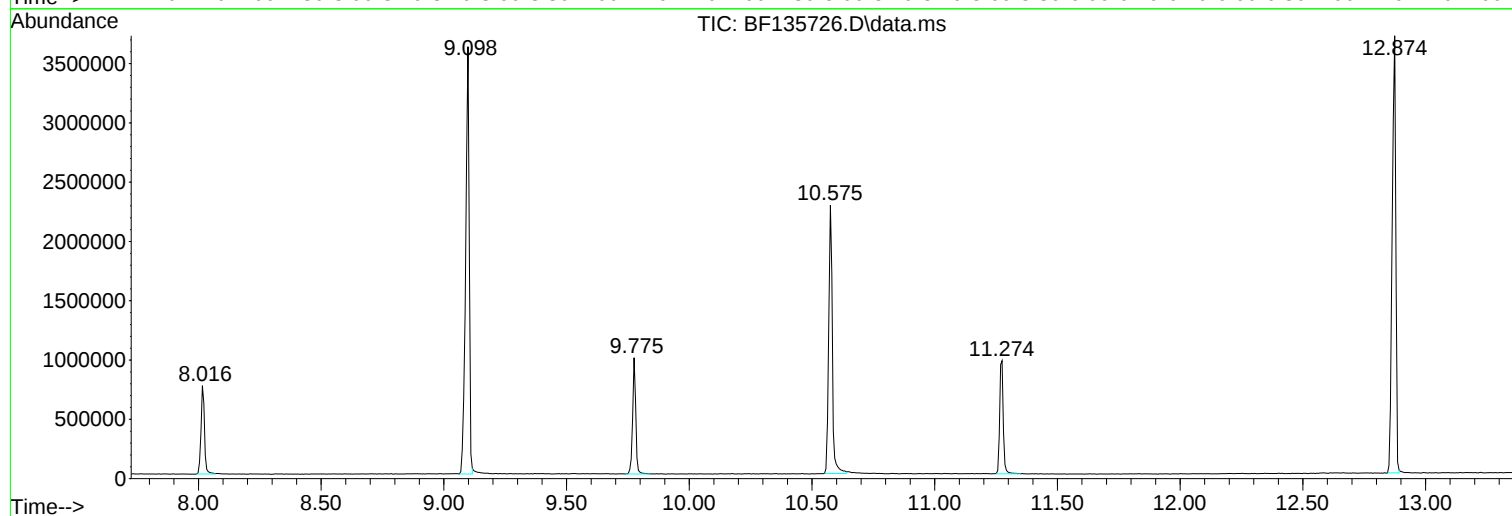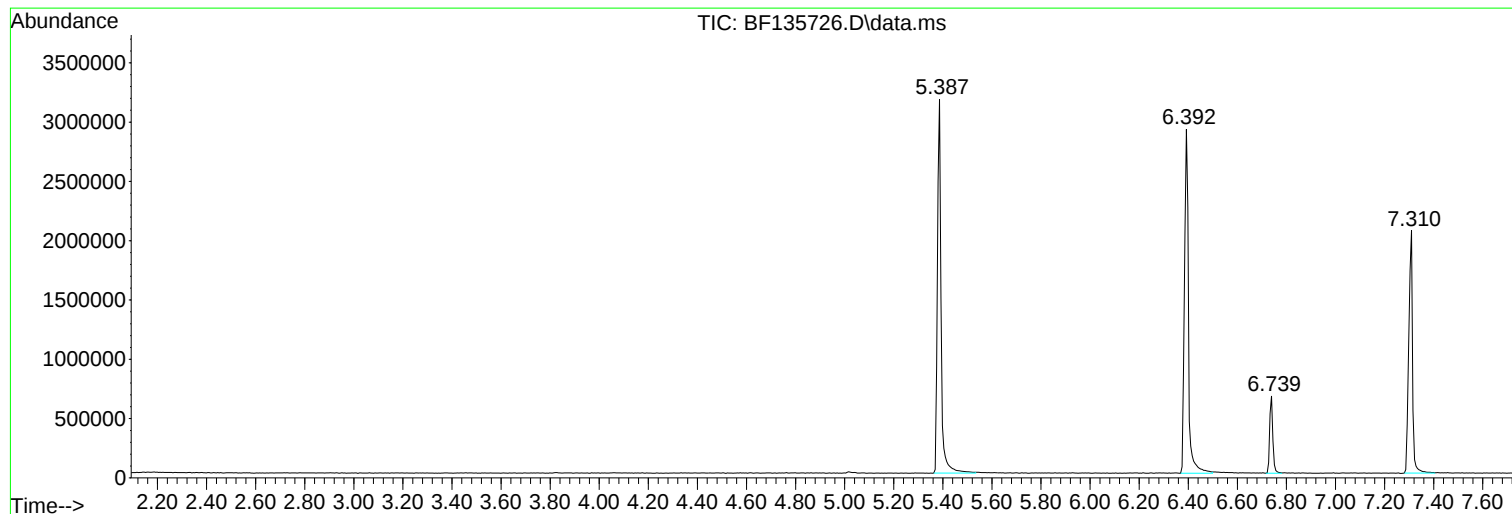

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135726.D
Acq On : 12 Oct 2023 10:43
Operator : CG\JU
Sample : PB156073BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135726.D
Acq On : 12 Oct 2023 10:43
Operator : CG\JU
Sample : PB156073BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------