
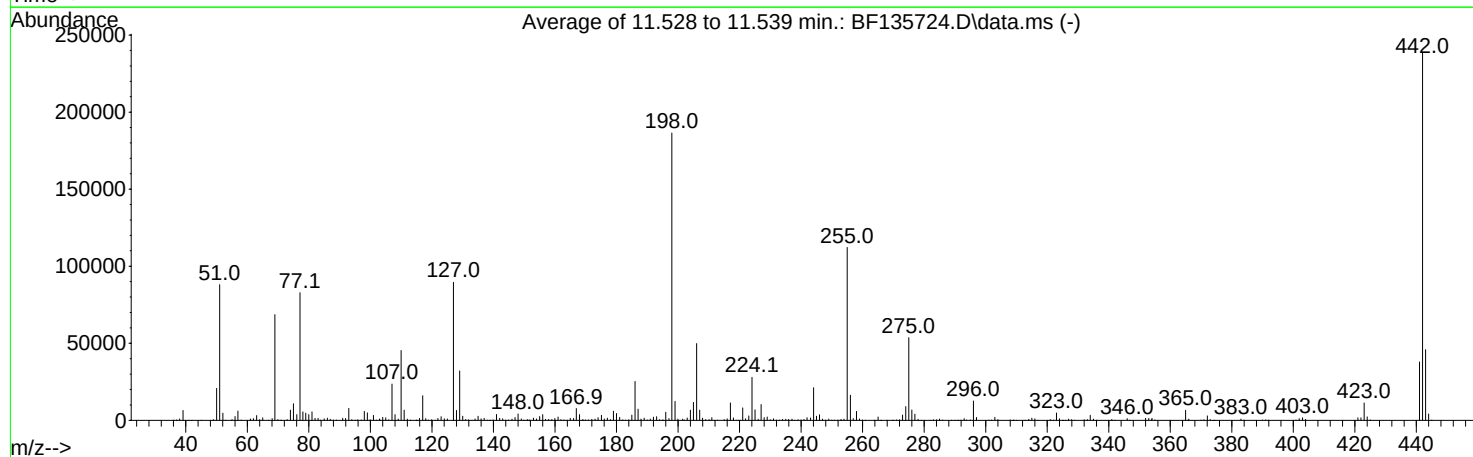


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
 Data File : BF135724.D
 Acq On : 12 Oct 2023 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 02:43:17 2023

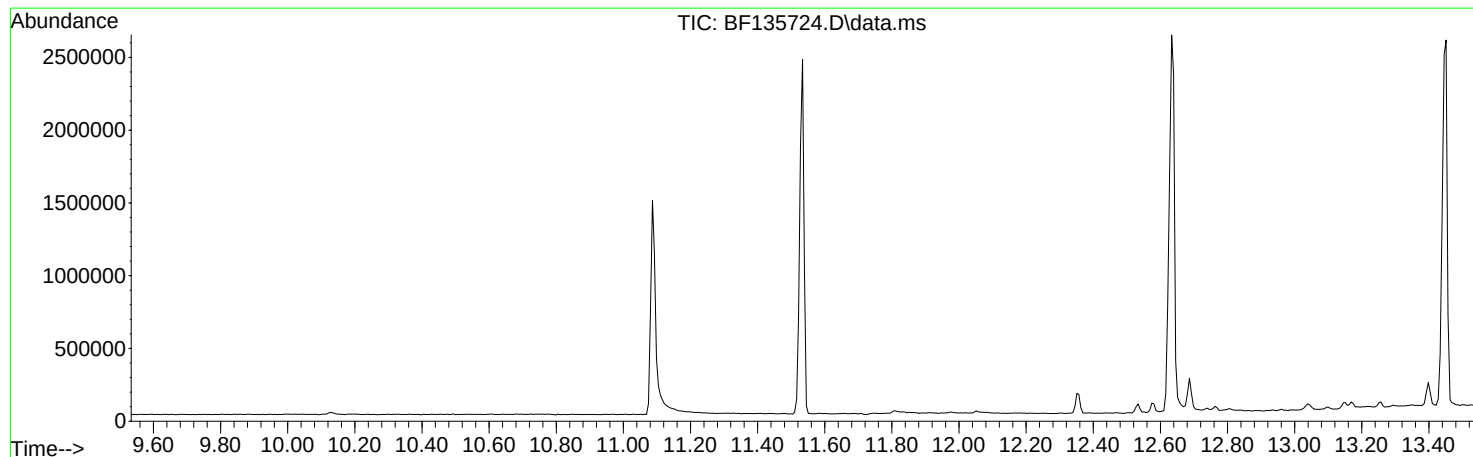




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	88029	PASS
68	69	0.00	2	1.6	1108	PASS
69	198	0.00	100	36.8	68615	PASS
70	69	0.00	2	0.7	483	PASS
127	198	10	80	48.1	89605	PASS
197	198	0.00	2	0.6	1096	PASS
198	198	100	100	100.0	186464	PASS
199	198	5	9	6.6	12338	PASS
275	198	10	60	28.8	53629	PASS
365	198	1	100	3.5	6539	PASS
441	198	0.01	100	20.3	37880	PASS
442	442	50	100	100.0	238677	PASS
443	442	15	24	19.2	45917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
Data File : BF135724.D
Acq On : 12 Oct 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 12 12:48:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 02:43:17 2023
Response via : Initial Calibration

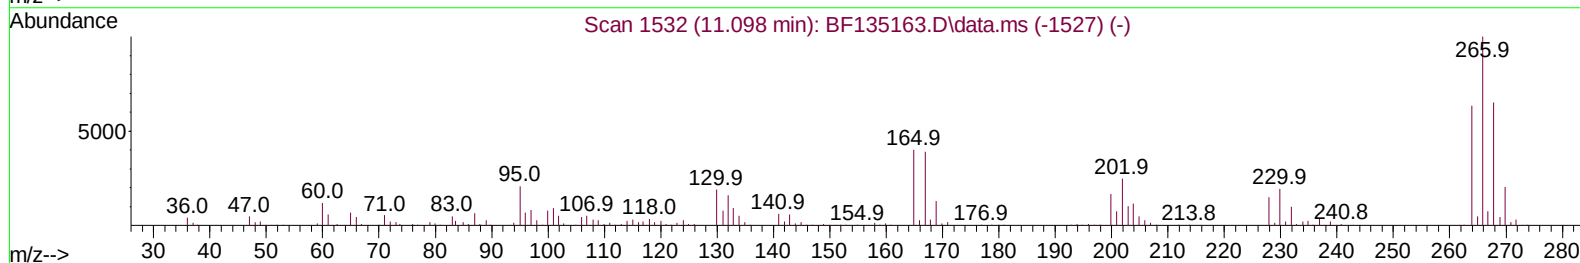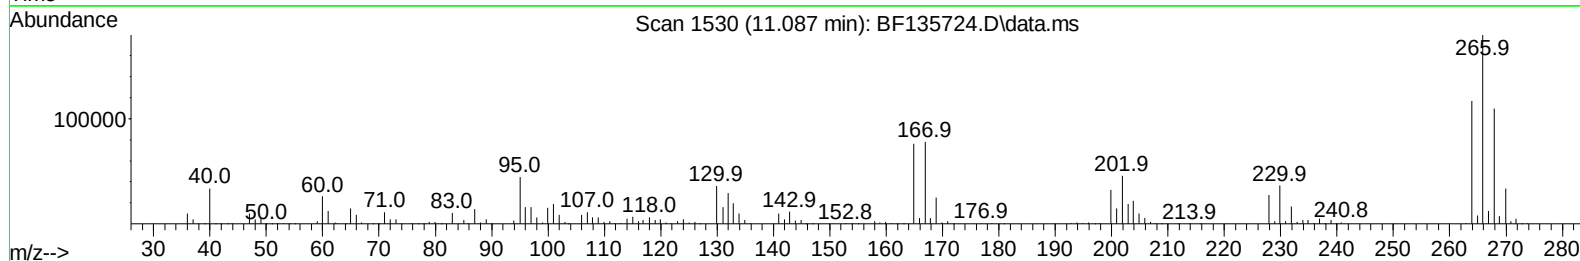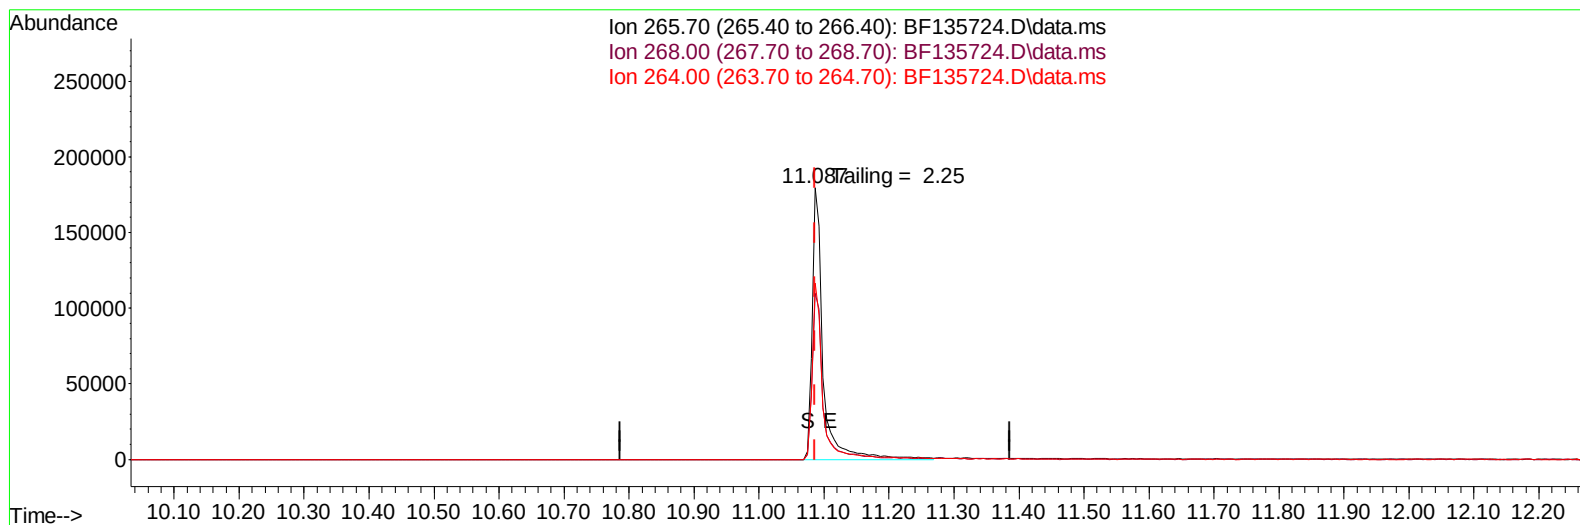

TIC: BF135724.D\data.ms

(70) Pentachlorophenol (C)

11.087min (+ 0.000) 595628.20 ng




response 209428

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.08
264.00	63.50	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101223\
 Data File : BF135724.D
 Acq On : 12 Oct 2023 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 12 12:48:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 02:43:17 2023
 Response via : Initial Calibration

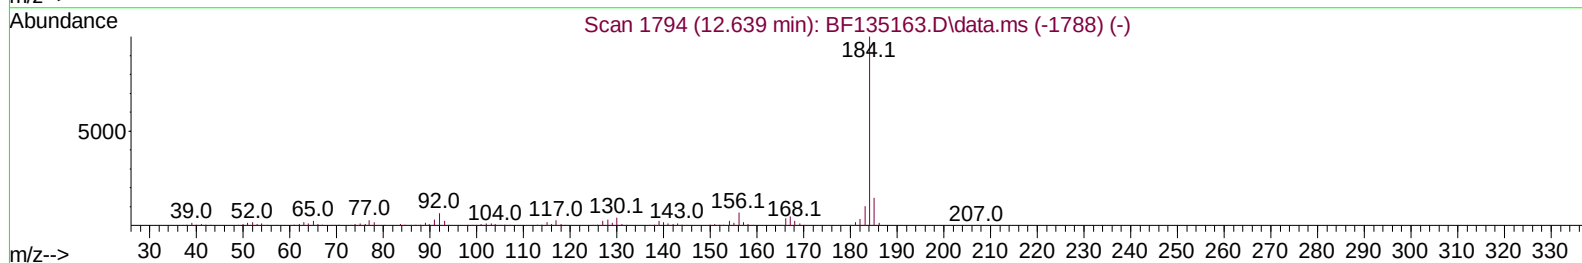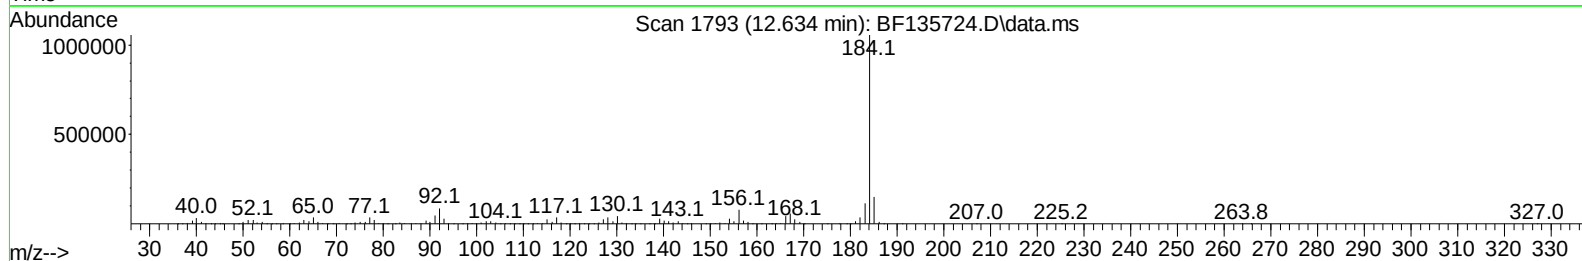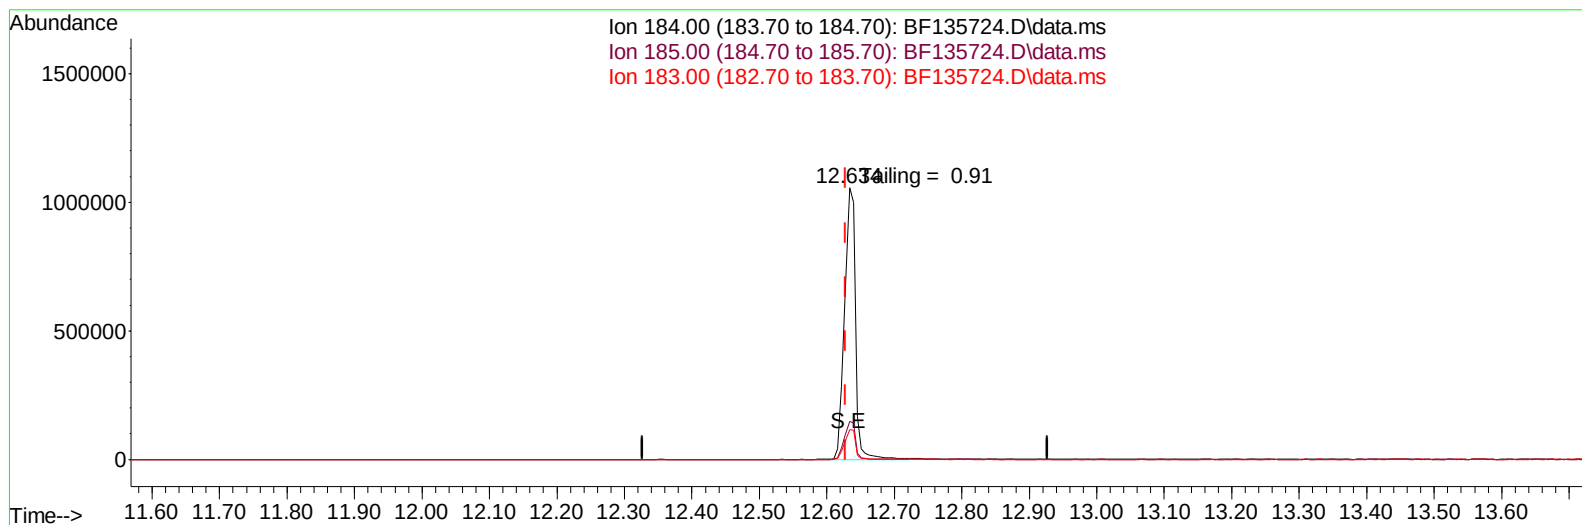

TIC: BF135724.D\data.ms

(77) Benzidine

12.634min (+ 0.006) 221863.09 ng

response 1186316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.14
183.00	10.30	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2023	BNA_F	<u>BF135724.D</u>
Compound Name	Response	Retention Time
DDT	513593	13.451
DDD	16421	13.151
DDE	1195	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17616	531209	3.32

Instrument :
BNA_F
ClientSampleId :
DFTPP