

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
 Data File : BF135756.D
 Acq On : 13 Oct 2023 16:59
 Operator : CG\JU
 Sample : PB156084BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156084BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	557	561	583	rBV	3476057	3808810	88.16%	14.351%
2	6.398	728	733	761	rBV	3430530	3701535	85.68%	13.947%
3	6.740	788	791	805	rBV	779206	683375	15.82%	2.575%
4	7.310	884	888	891	rBV	2402348	2262705	52.37%	8.526%
5	8.022	1005	1009	1028	rBV	884236	894670	20.71%	3.371%
6	9.098	1188	1192	1196	rBV	4021981	3969575	91.88%	14.957%
7	9.775	1304	1307	1322	rVB	1147703	1001673	23.18%	3.774%
8	10.575	1439	1443	1462	rBV	2511908	2609981	60.41%	9.834%
9	11.275	1558	1562	1573	rBV	1150787	1089873	25.23%	4.107%
10	12.875	1829	1834	1837	rBV	4125085	4320359	100.00%	16.279%
11	13.939	2011	2015	2026	rBV	950665	968966	22.43%	3.651%
12	14.704	2140	2145	2149	rBV	64185	67716	1.57%	0.255%
13	15.039	2197	2202	2208	rBV	64500	81947	1.90%	0.309%
14	15.416	2260	2266	2277	rBV	651706	973579	22.53%	3.668%
15	15.851	2334	2340	2345	rBV	36203	59095	1.37%	0.223%
16	17.033	2535	2541	2542	rBV2	26563	45969	1.06%	0.173%




Sum of corrected areas: 26539828

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
Data File : BF135756.D
Acq On : 13 Oct 2023 16:59
Operator : CG\JU
Sample : PB156084BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156084BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

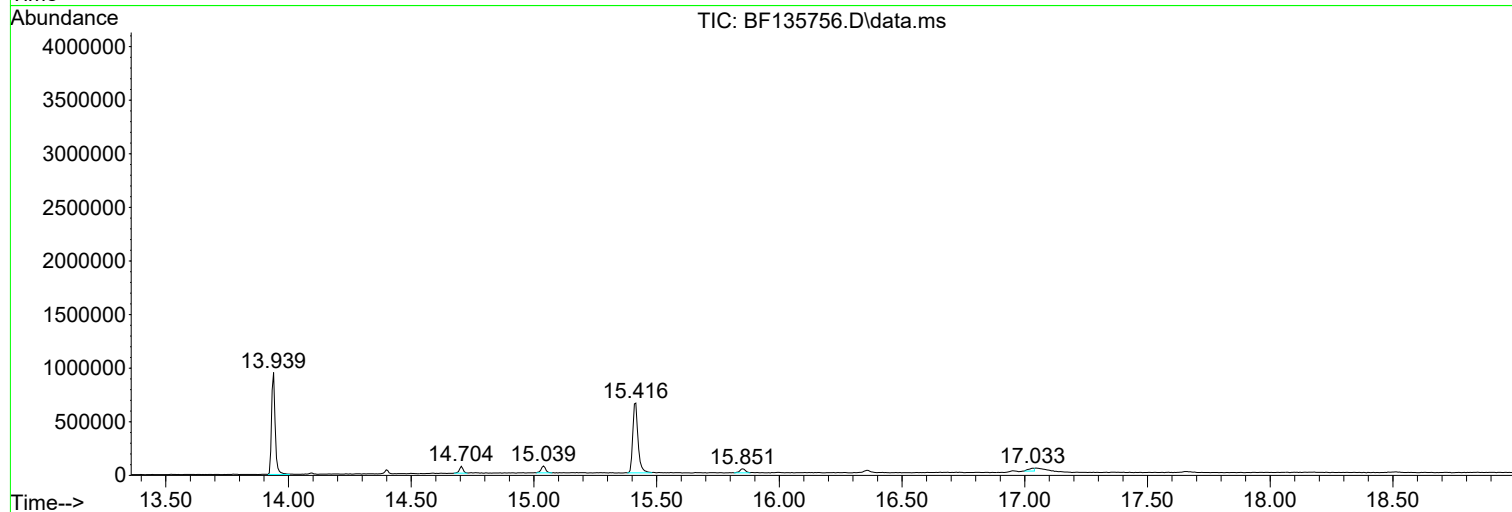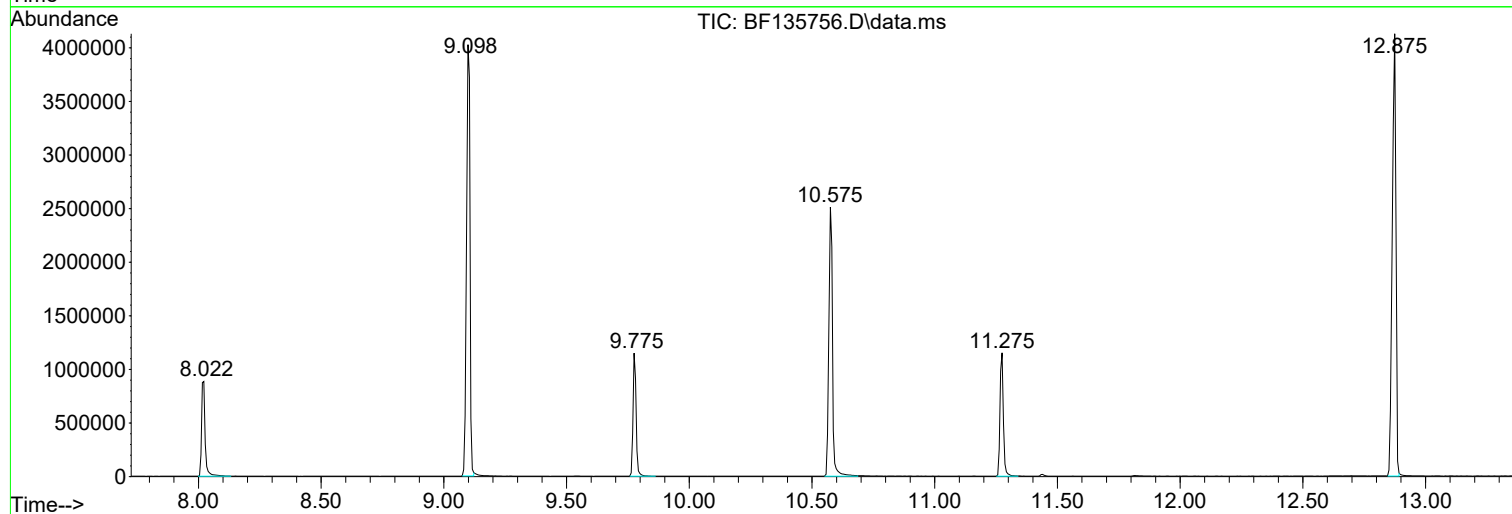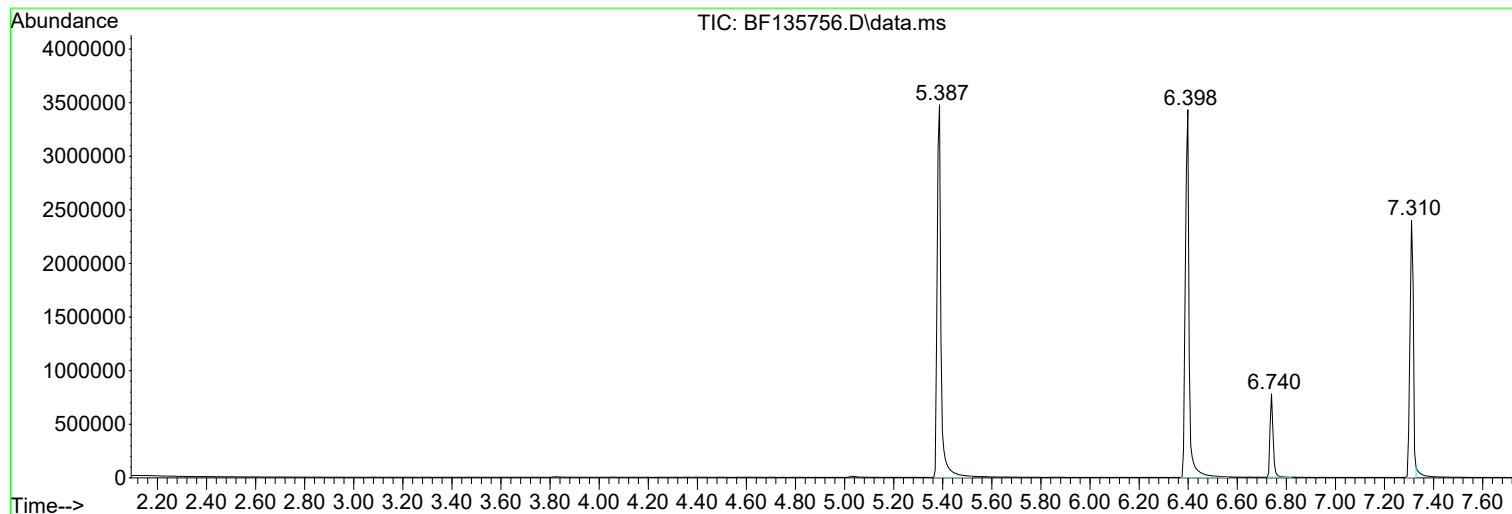

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
Data File : BF135756.D
Acq On : 13 Oct 2023 16:59
Operator : CG\JU
Sample : PB156084BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156084BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
Data File : BF135756.D
Acq On : 13 Oct 2023 16:59
Operator : CG\JU
Sample : PB156084BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156084BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------