
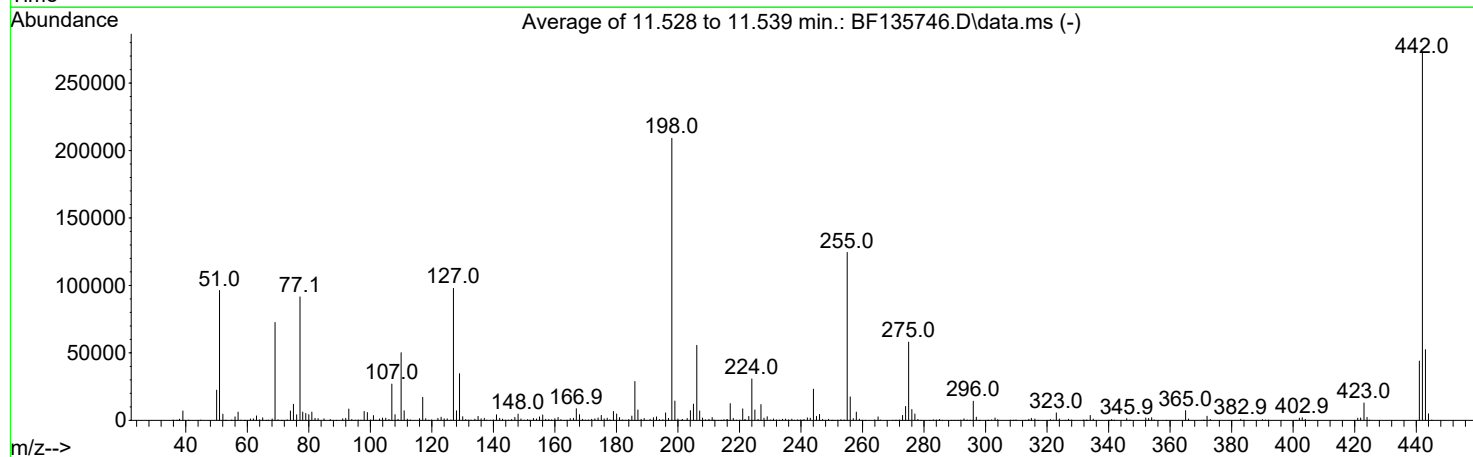


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
Data File : BF135746.D
Acq On : 13 Oct 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 13 17:12:59 2023

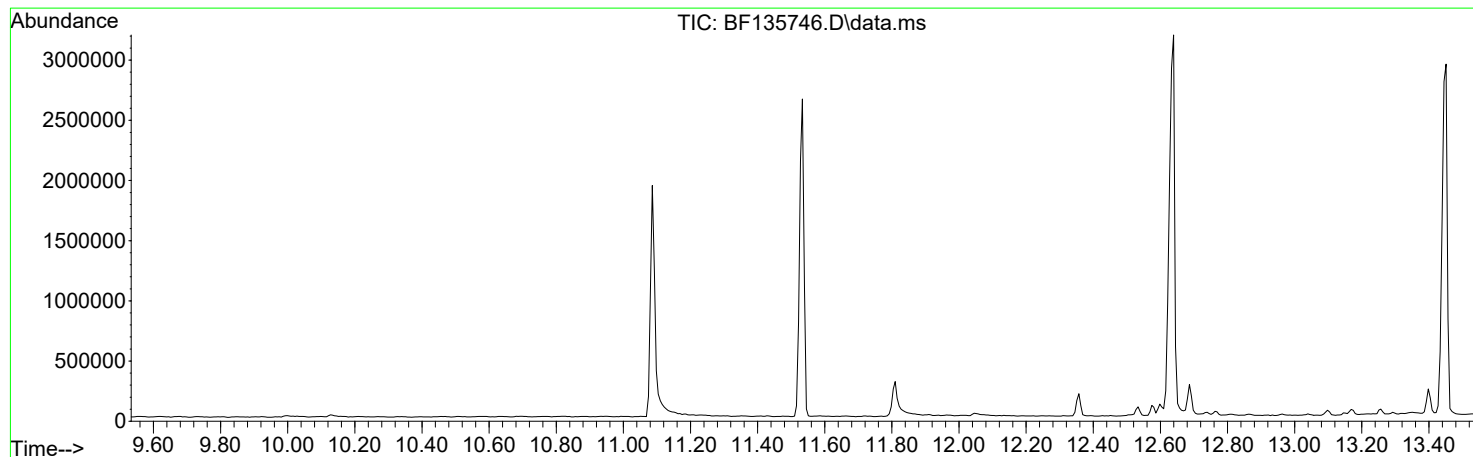

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	96299	PASS
68	69	0.00	2	1.6	1131	PASS
69	198	0.00	100	34.7	72554	PASS
70	69	0.00	2	0.6	434	PASS
127	198	10	80	46.8	97840	PASS
197	198	0.00	2	0.7	1512	PASS
198	198	100	100	100.0	209125	PASS
199	198	5	9	6.9	14337	PASS
275	198	10	60	27.8	58035	PASS
365	198	1	100	3.5	7280	PASS
441	198	0.01	100	21.1	44043	PASS
442	442	50	100	100.0	272640	PASS
443	442	15	24	19.2	52371	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/13/2023	BNA_F	<u>BF135746.D</u>
Compound Name	Response	Retention Time
DDT	598577	13.451
DDD	12748	13.169
DDE	1245	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13993	612570	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101323\
Data File : BF135746.D
Acq On : 13 Oct 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:31:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 13 17:12:59 2023
Response via : Initial Calibration

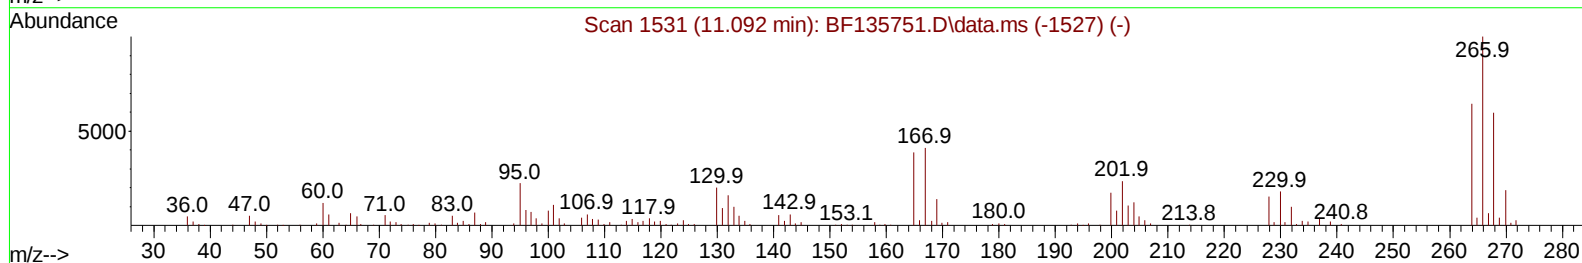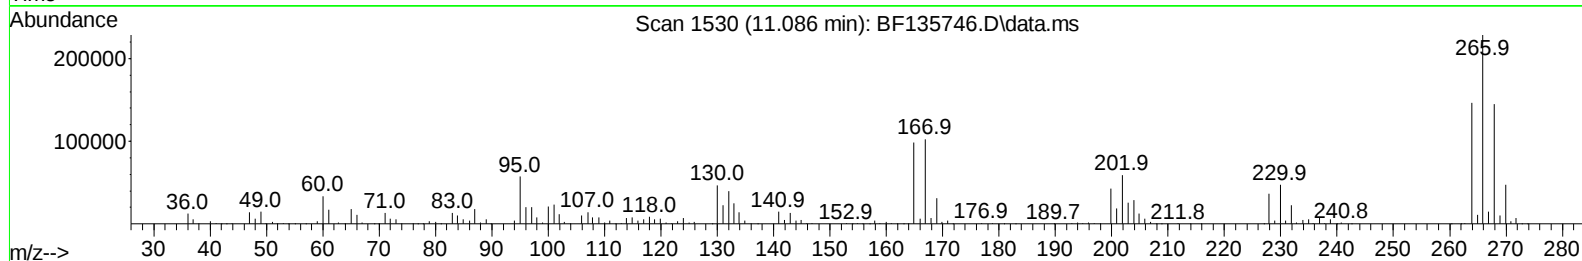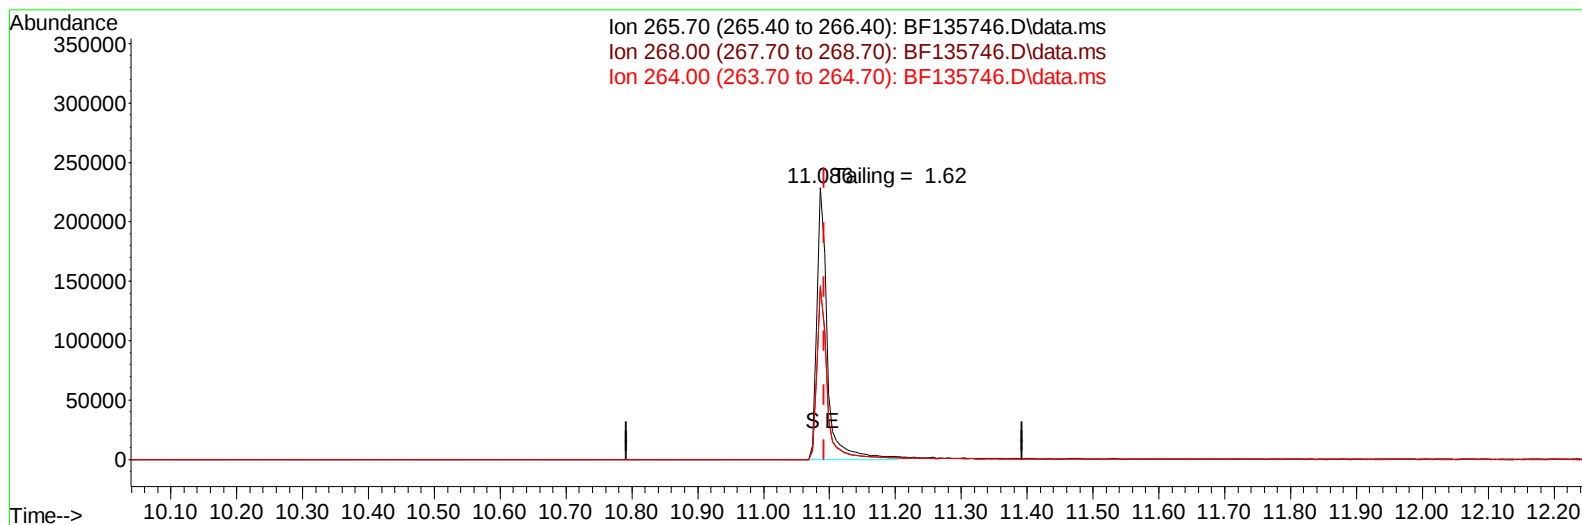

TIC: BF135746.D\data.ms



(70) Pentachlorophenol (C)

11.086min (-0.006) 99577.44 ng

response 250462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.34
264.00	64.30	64.10
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

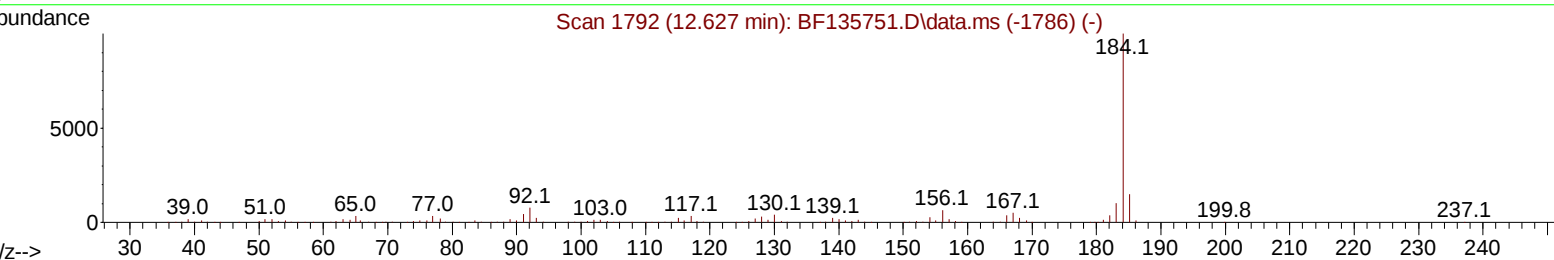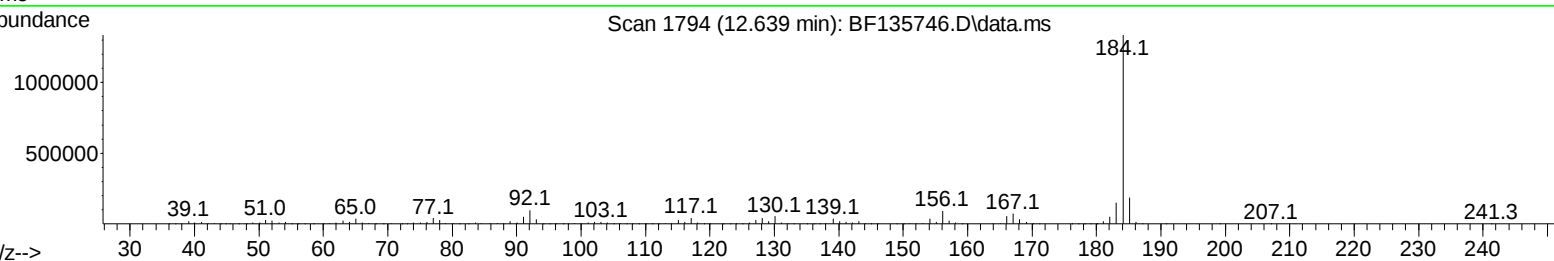

TIC: BF135746.D\data.ms

(77) Benzidine

12.639min (+ 0.012) 47245.97 ng

response **1463950**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.00
183.00	10.20	11.05
0.00	0.00	0.00