

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
 Data File : BF143966.D
 Acq On : 15 Oct 2025 21:51
 Operator : RC/JU
 Sample : Q3337-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LAYDOWN-YARD-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	294	300	306	rBV	7916	13651	1.56%	0.156%
2	5.087	481	492	498	rBV2	12680	23821	2.72%	0.272%
3	5.493	555	561	574	rBV	514096	716384	81.76%	8.165%
4	6.163	670	675	680	rVB	20075	25958	2.96%	0.296%
5	6.498	727	732	743	rBV	553508	735562	83.95%	8.384%
6	6.581	743	746	750	rVB	11069	14620	1.67%	0.167%
7	6.881	792	797	803	rBV	559016	690212	78.77%	7.867%
8	7.439	886	892	903	rBV	329603	442904	50.55%	5.048%
9	8.163	1010	1015	1023	rBV	680636	851638	97.20%	9.707%
10	9.239	1192	1198	1207	rBV	614900	800770	91.39%	9.127%
11	9.922	1306	1314	1319	rBV	684521	876198	100.00%	9.987%
12	10.633	1430	1435	1442	rBV	68425	86958	9.92%	0.991%
13	10.710	1443	1448	1462	rVV	220556	311401	35.54%	3.549%
14	10.833	1464	1469	1475	rVB5	14029	24384	2.78%	0.278%
15	11.269	1539	1543	1546	rBV3	13650	20134	2.30%	0.229%
16	11.304	1546	1549	1552	rVB5	9825	13356	1.52%	0.152%
17	11.410	1562	1567	1575	rBV	548809	765770	87.40%	8.728%
18	11.522	1583	1586	1593	rVB8	5962	9511	1.09%	0.108%
19	11.651	1605	1608	1612	rVB6	6934	9038	1.03%	0.103%
20	11.698	1612	1616	1620	rBV4	9469	12965	1.48%	0.148%
21	11.816	1632	1636	1642	rVB5	12803	20243	2.31%	0.231%
22	11.939	1650	1657	1661	rBV4	31686	60849	6.94%	0.694%
23	12.027	1669	1672	1679	rVB	17298	31985	3.65%	0.365%
24	12.463	1743	1746	1749	rBV2	9215	12632	1.44%	0.144%
25	12.504	1749	1753	1758	rVB5	16917	31742	3.62%	0.362%
26	12.627	1770	1774	1779	rBV	73912	91183	10.41%	1.039%
27	12.857	1808	1813	1819	rBV	71787	109871	12.54%	1.252%
28	12.998	1832	1837	1845	rVB	390507	504477	57.58%	5.750%
29	14.057	2010	2017	2029	rBV	498094	830736	94.81%	9.468%
30	15.545	2265	2270	2280	rVB	379604	634815	72.45%	7.235%


Sum of corrected areas: 8773768

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143966.D
Acq On : 15 Oct 2025 21:51
Operator : RC/JU
Sample : Q3337-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAYDOWN-YARD-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

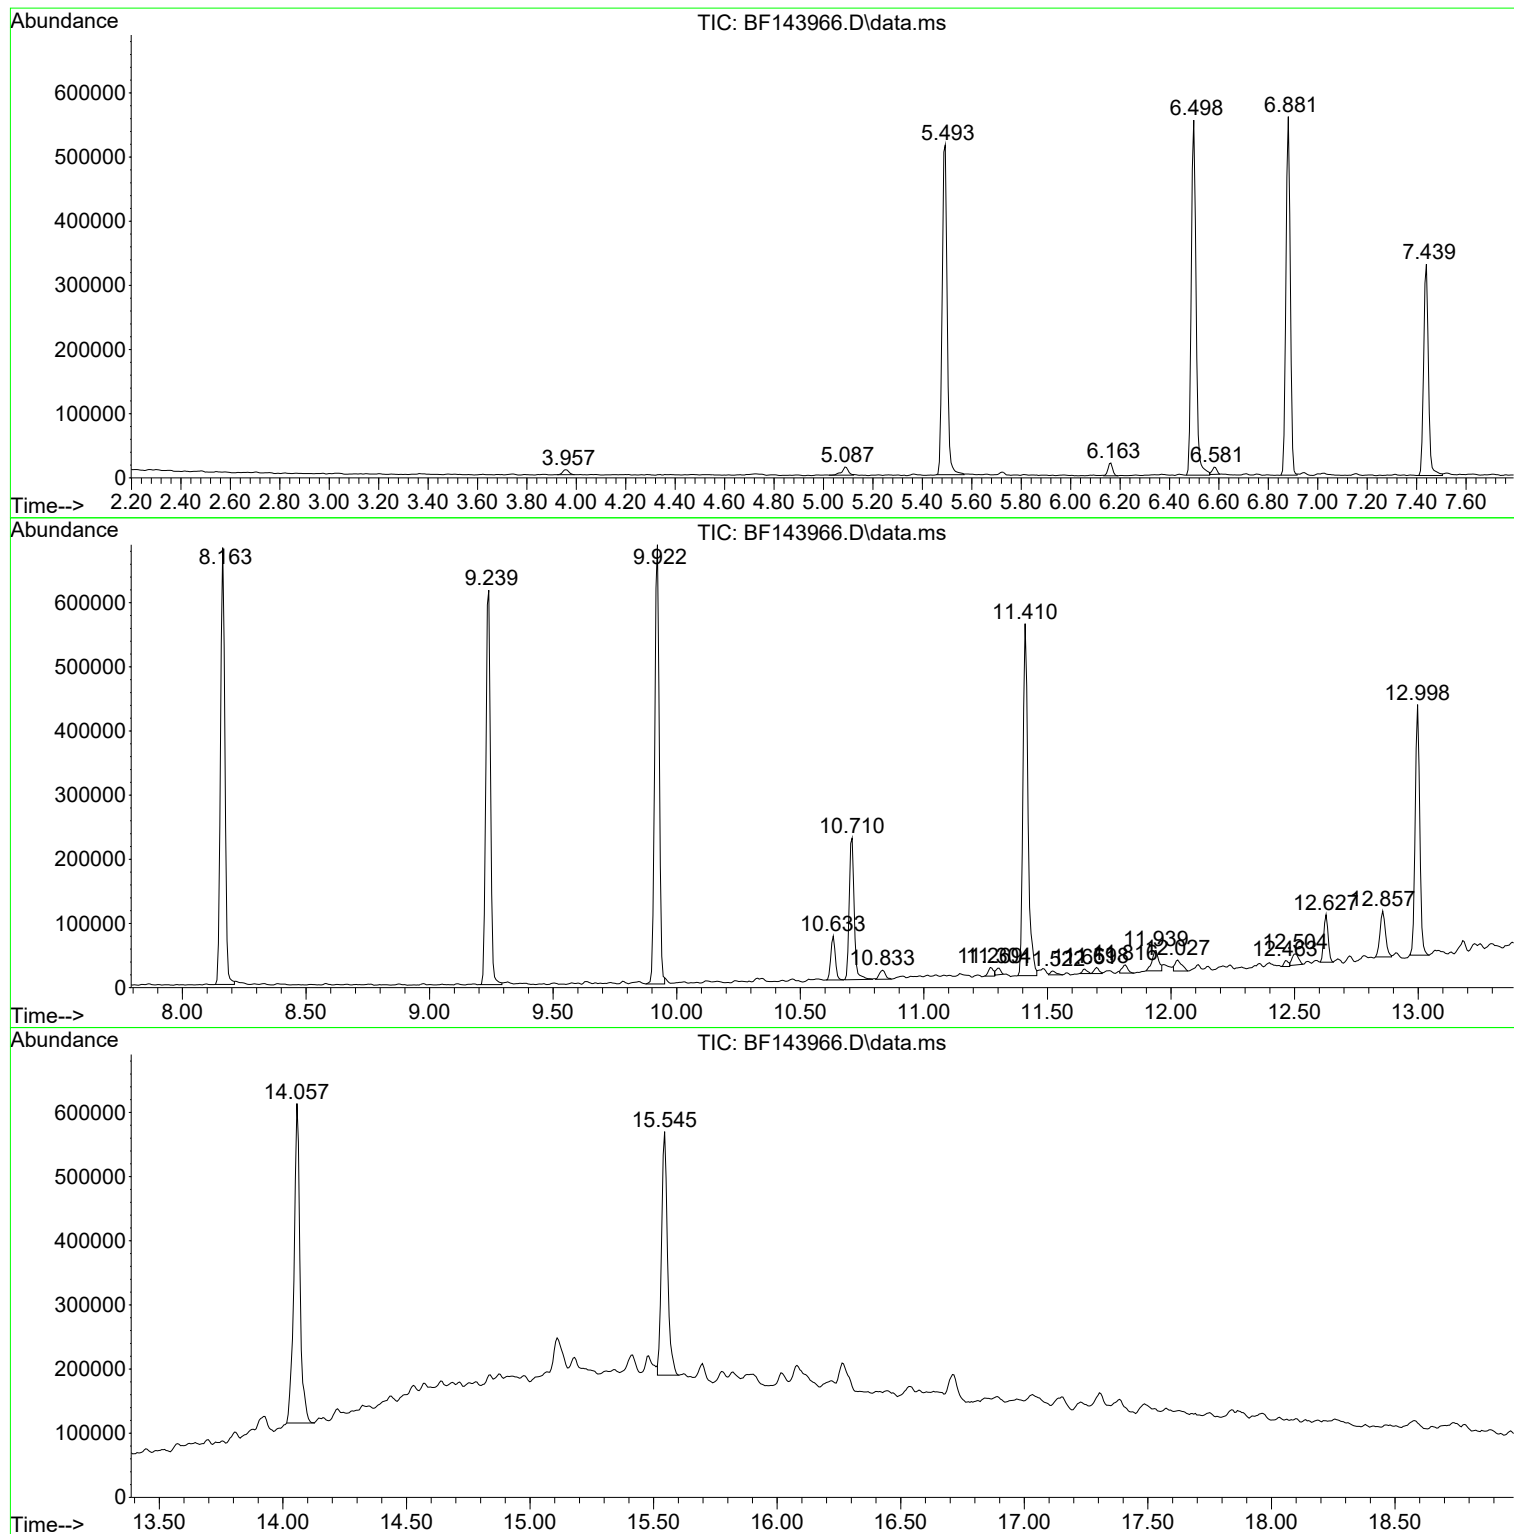

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143966.D
Acq On : 15 Oct 2025 21:51
Operator : RC/JU
Sample : Q3337-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAYDOWN-YARD-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101525\
Data File : BF143966.D
Acq On : 15 Oct 2025 21:51
Operator : RC/JU
Sample : Q3337-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAYDOWN-YARD-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc