


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101618\
 Data File : BF109899.D
 Acq On : 16 Oct 2018 12:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

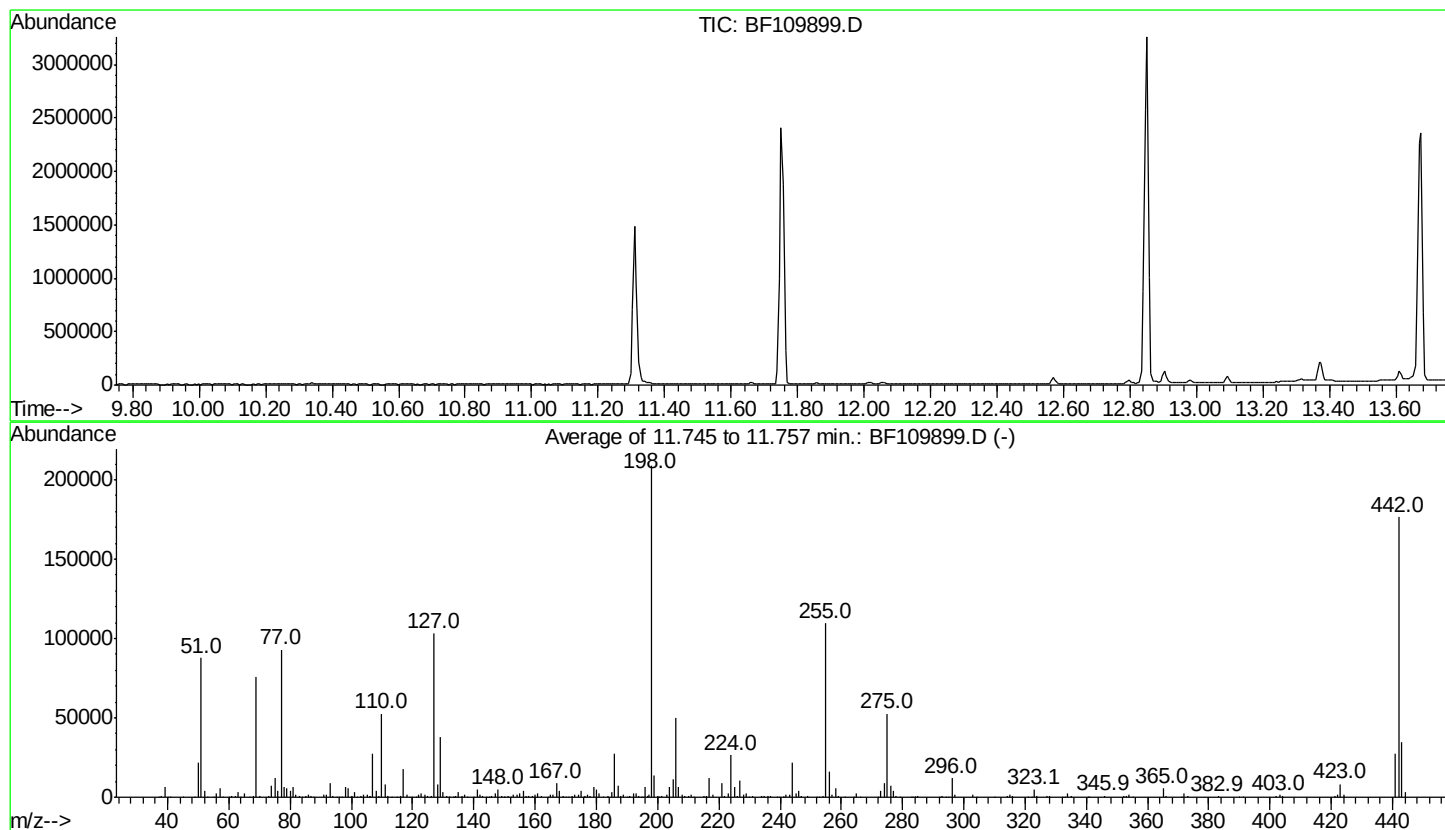

AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	87653	PASS
68	69	0.00	2	1.6	1239	PASS
69	198	0.00	100	36.3	75842	PASS
70	69	0.00	2	0.7	503	PASS
127	198	10	80	49.3	103045	PASS
197	198	0.00	2	0.7	1373	PASS
198	198	100	100	100.0	208898	PASS
199	198	5	9	6.6	13813	PASS
275	198	10	60	25.3	52776	PASS
365	198	1	100	2.7	5604	PASS
441	198	0.01	100	13.3	27744	PASS
442	198	50	100	84.5	176578	PASS
443	442	15	24	19.6	34549	PASS