


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101619\
 Data File : BF117408.D
 Acq On : 16 Oct 2019 12:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 14 19:03:29 2019

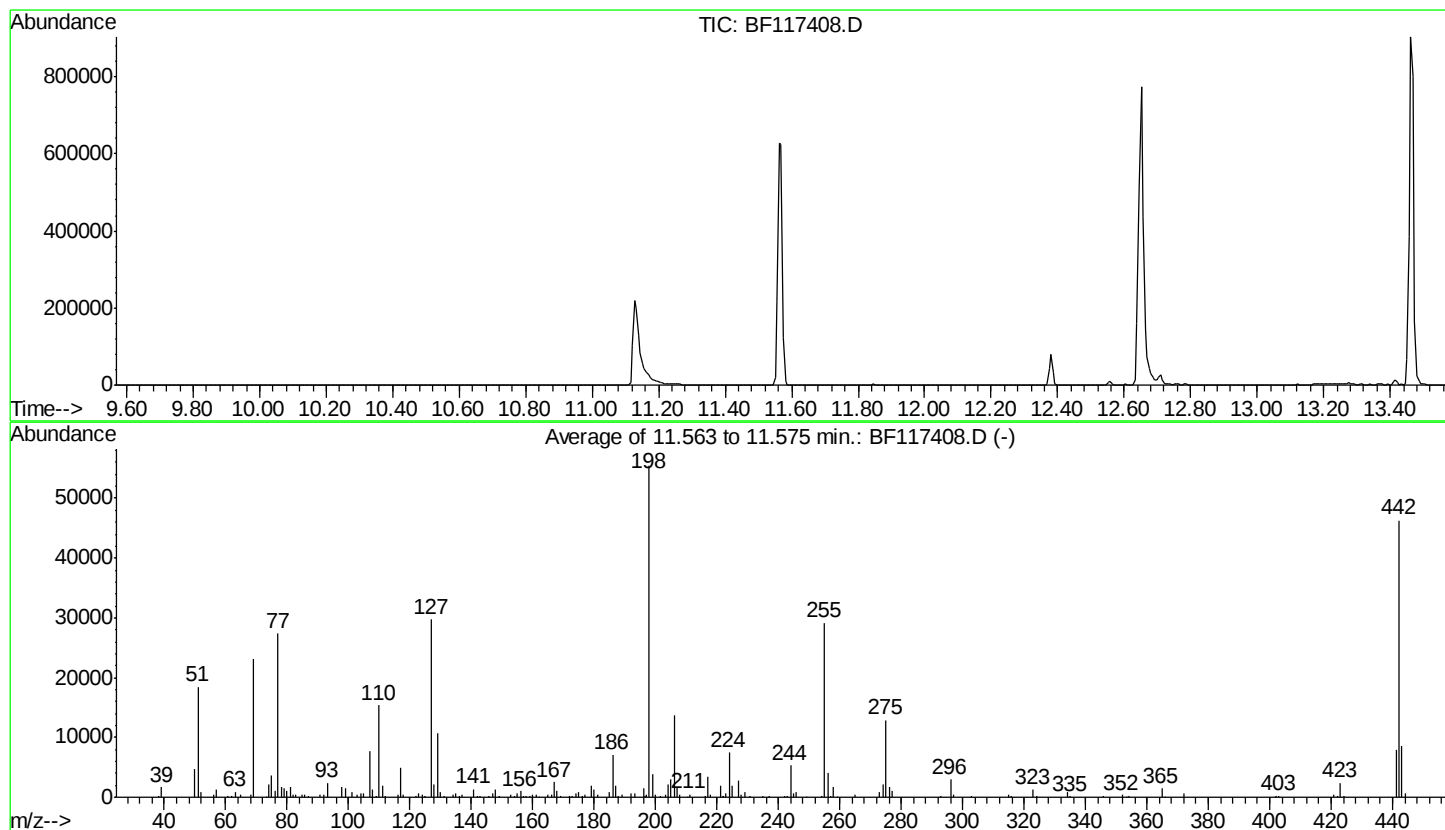

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	18522	PASS
68	69	0.00	2	1.5	355	PASS
69	198	0.00	100	41.9	23212	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	29662	PASS
197	198	0.00	2	0.6	357	PASS
198	198	100	100	100.0	55459	PASS
199	198	5	9	7.0	3863	PASS
275	198	10	60	23.3	12944	PASS
365	198	1	100	2.7	1484	PASS
441	198	0.01	100	14.2	7893	PASS
442	198	50	100	83.4	46261	PASS
443	442	15	24	18.7	8646	PASS