
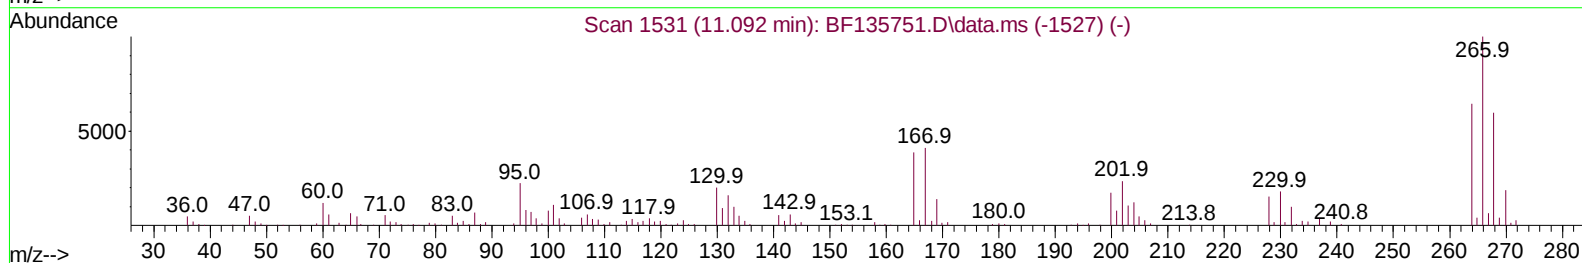
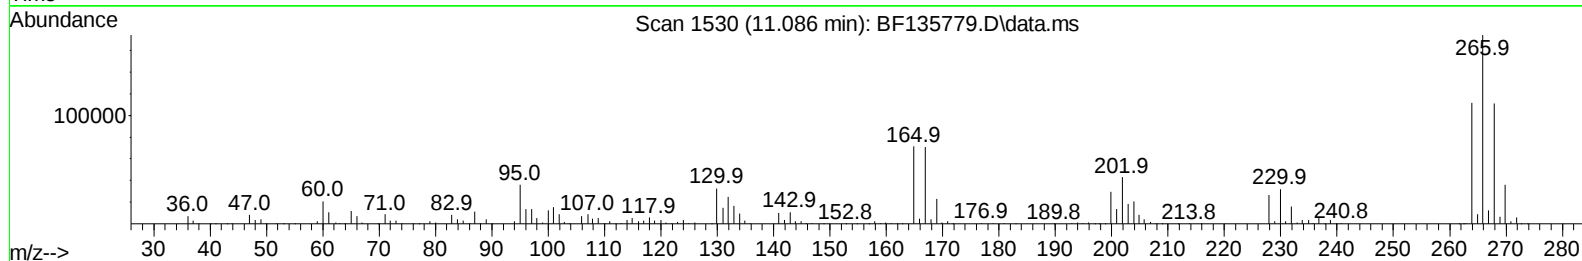


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
 Data File : BF135779.D
 Acq On : 16 Oct 2023 16:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 05:36:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 17 01:22:00 2023
 Response via : Initial Calibration

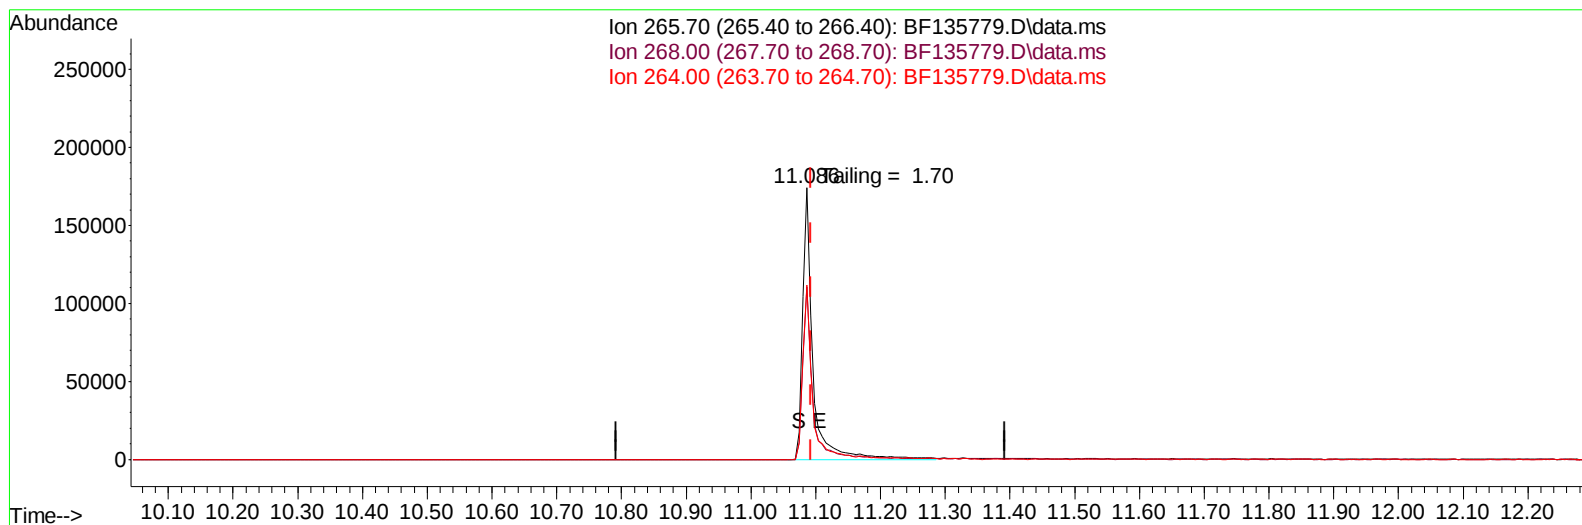




TIC: BF135779.D\data.ms

(70) Pentachlorophenol (C)**11.086min (-0.006) 852554.83 ng****response 192445**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.63
264.00	64.30	64.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135779.D
Acq On : 16 Oct 2023 16:30
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 05:36:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

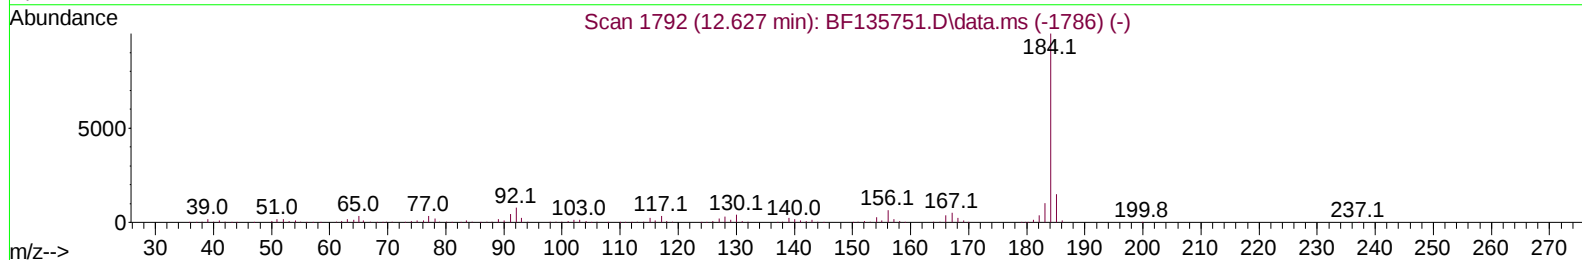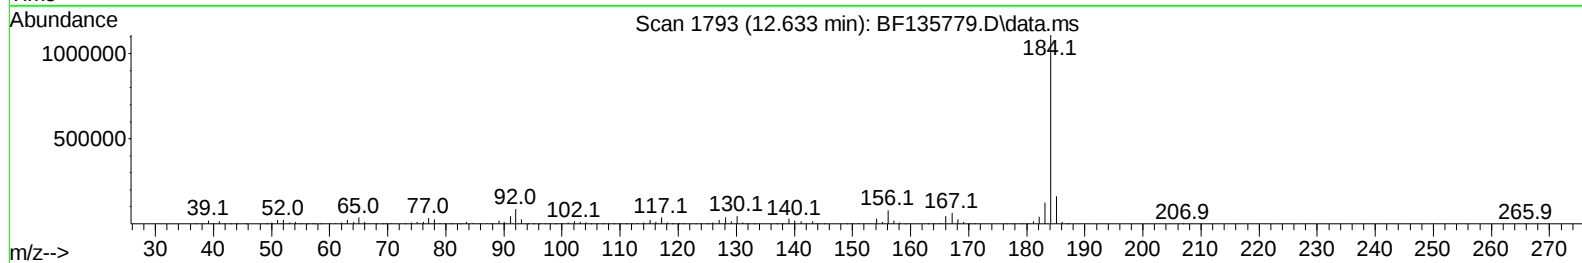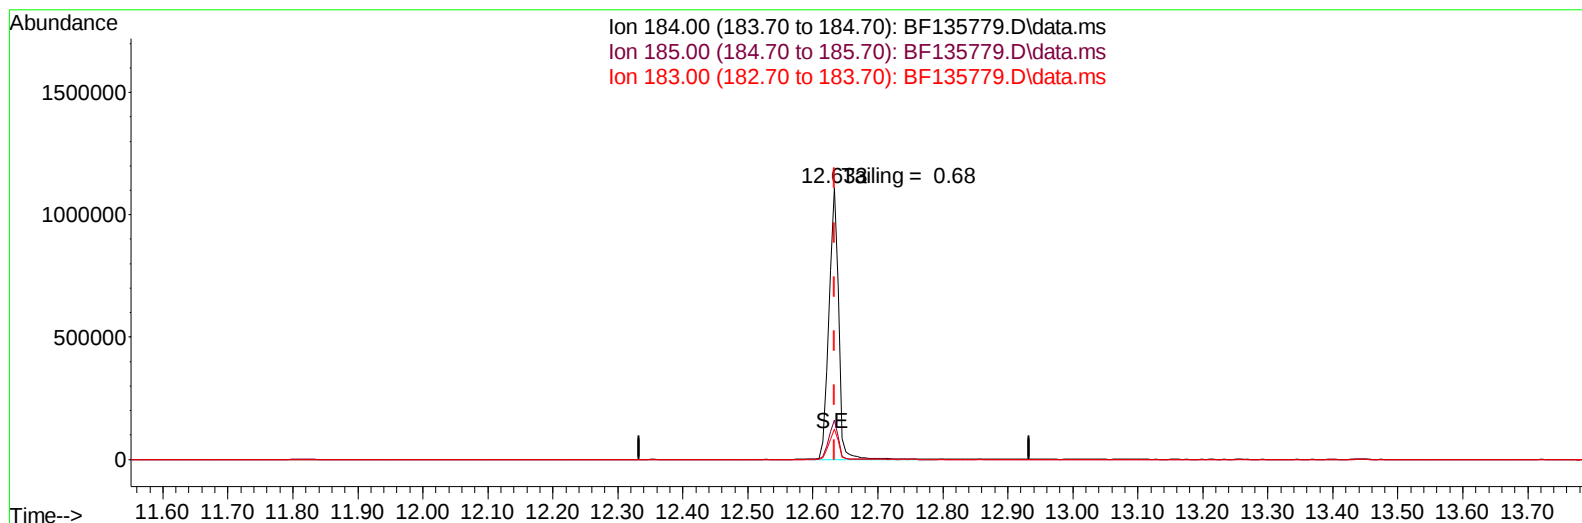

TIC: BF135779.D\data.ms

(77) Benzidine**12.633min (-0.000) 431463.62 ng****response 1148622**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.54
183.00	10.20	11.26
0.00	0.00	0.00