

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
 Data File : BF135786.D
 Acq On : 16 Oct 2023 20:20
 Operator : CG\JU
 Sample : 04656-24
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-10022023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	485	488	500	rBV	148439	205988	6.58%	1.214%
2	5.369	555	558	588	rBV	1304225	1720272	54.98%	10.134%
3	6.387	728	731	759	rBV	903020	1151658	36.81%	6.785%
4	6.734	787	790	800	rBV	659452	603561	19.29%	3.556%
5	7.304	883	887	901	rBV	2083230	1924706	61.52%	11.339%
6	8.016	1005	1008	1026	rBV	867854	783713	25.05%	4.617%
7	9.098	1187	1192	1195	rBV	3309934	3128752	100.00%	18.432%
8	9.775	1303	1307	1321	rBV	930013	817487	26.13%	4.816%
9	10.569	1439	1442	1465	rBV	1789433	1787456	57.13%	10.530%
10	11.269	1558	1561	1571	rBV	945339	849652	27.16%	5.005%
11	12.869	1828	1833	1836	rBV	3116719	2868024	91.67%	16.896%
12	13.933	2011	2014	2024	rBV	525781	553557	17.69%	3.261%
13	15.410	2261	2265	2279	rBV	394667	579821	18.53%	3.416%




Sum of corrected areas: 16974647

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135786.D
Acq On : 16 Oct 2023 20:20
Operator : CG\JU
Sample : 04656-24
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-10022023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

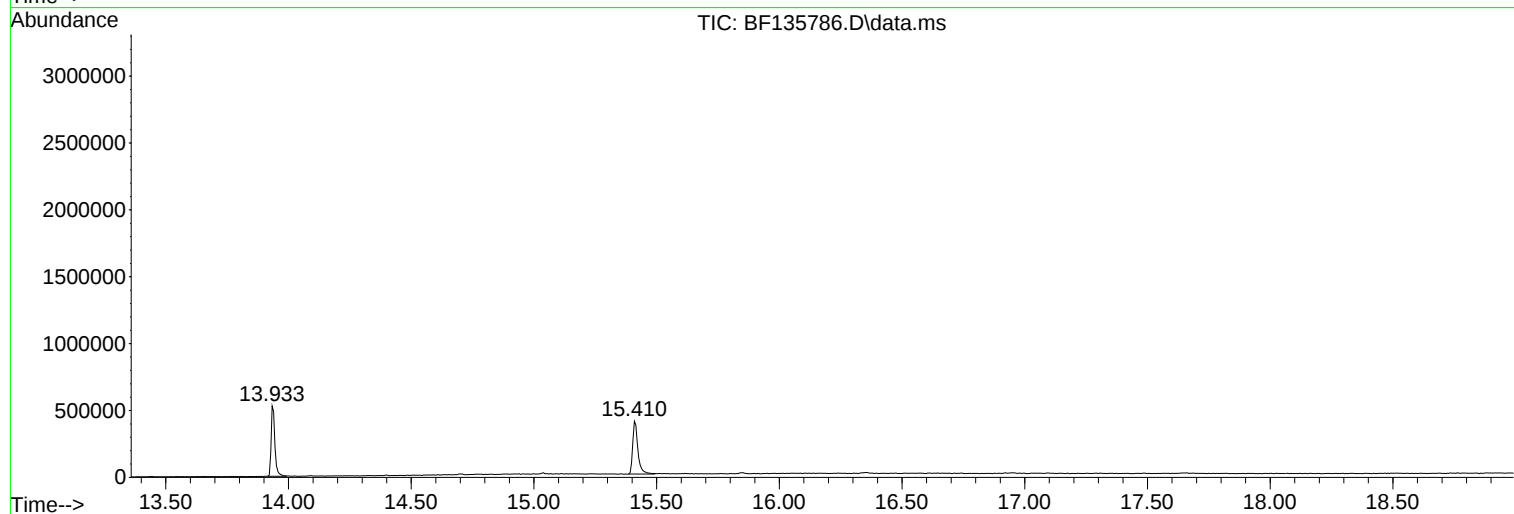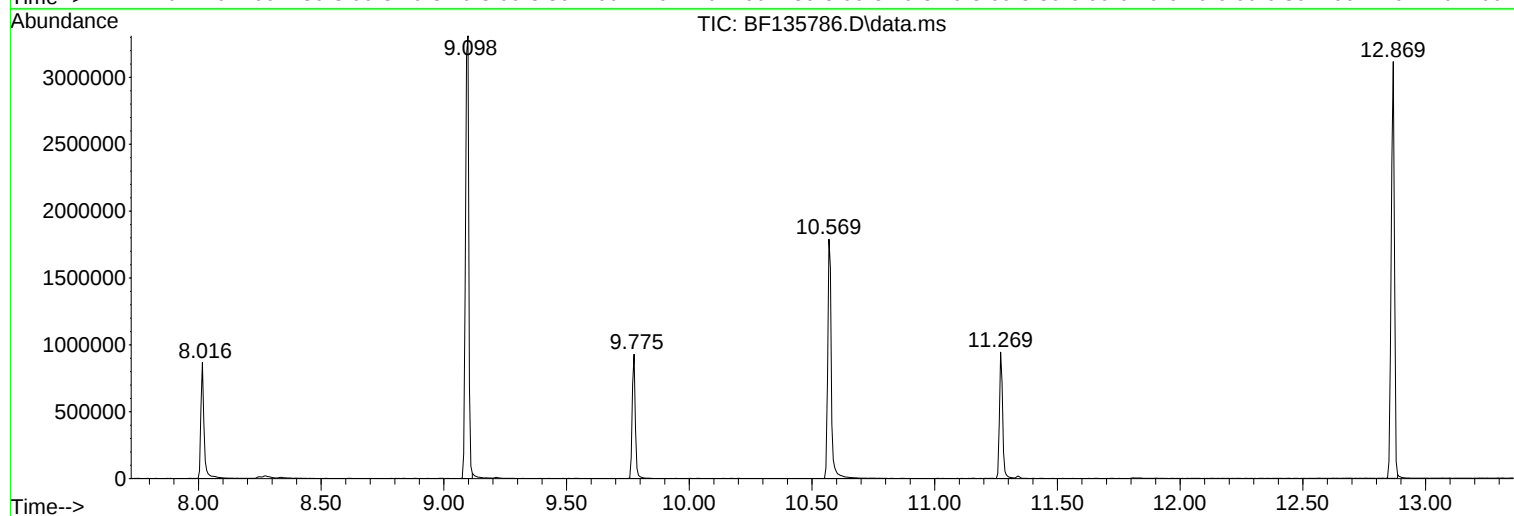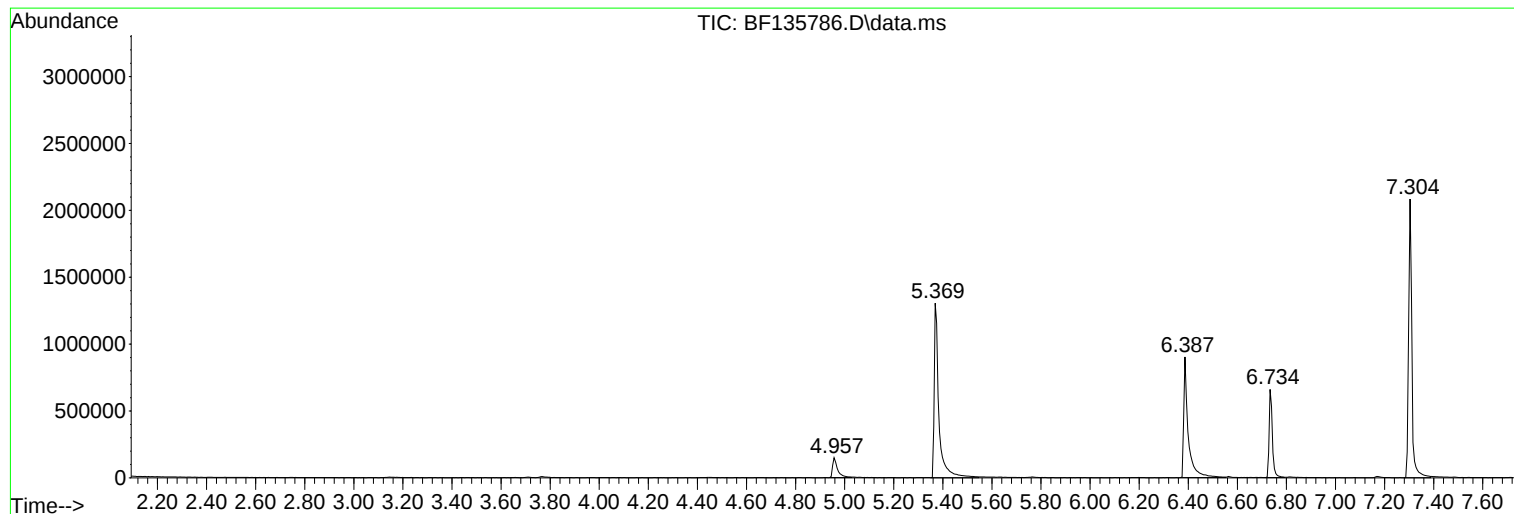

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135786.D
Acq On : 16 Oct 2023 20:20
Operator : CG\JU
Sample : 04656-24
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-10022023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135786.D
Acq On : 16 Oct 2023 20:20
Operator : CG\JU
Sample : 04656-24
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-10022023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc