

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
 Data File : BF135787.D
 Acq On : 16 Oct 2023 20:52
 Operator : CG\JU
 Sample : 04656-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-101I

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.751	279	283	292	rBV2	35960	63782	2.04%	0.392%
2	5.369	555	558	587	rBV	965441	1341485	42.92%	8.248%
3	6.387	728	731	758	rBV	513957	822546	26.32%	5.057%
4	6.734	787	790	802	rBV	563836	553869	17.72%	3.405%
5	7.304	883	887	903	rBV	2045671	1934714	61.90%	11.895%
6	7.428	905	908	915	rBV2	28530	47725	1.53%	0.293%
7	8.016	1005	1008	1032	rBV	819309	741083	23.71%	4.556%
8	9.098	1188	1192	1195	rBV	3394076	3125365	100.00%	19.215%
9	9.775	1303	1307	1320	rBV	974570	814187	26.05%	5.006%
10	10.574	1439	1443	1460	rBV	1830311	1960108	62.72%	12.051%
11	11.269	1558	1561	1571	rBV	948523	840692	26.90%	5.169%
12	11.804	1649	1652	1656	rBV2	48655	60704	1.94%	0.373%
13	12.868	1828	1833	1836	rBV	3104971	2919866	93.42%	17.951%
14	13.939	2011	2015	2022	rVB	463793	479391	15.34%	2.947%
15	15.409	2261	2265	2278	rBV	376579	559795	17.91%	3.442%




Sum of corrected areas: 16265312

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135787.D
Acq On : 16 Oct 2023 20:52
Operator : CG\JU
Sample : 04656-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

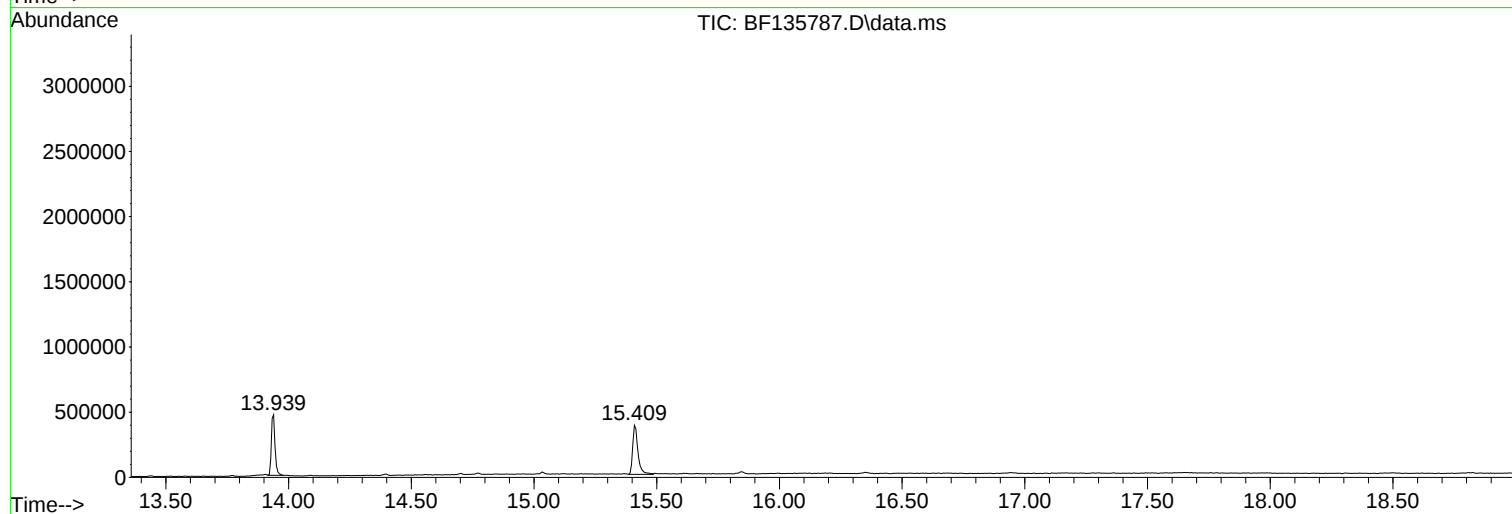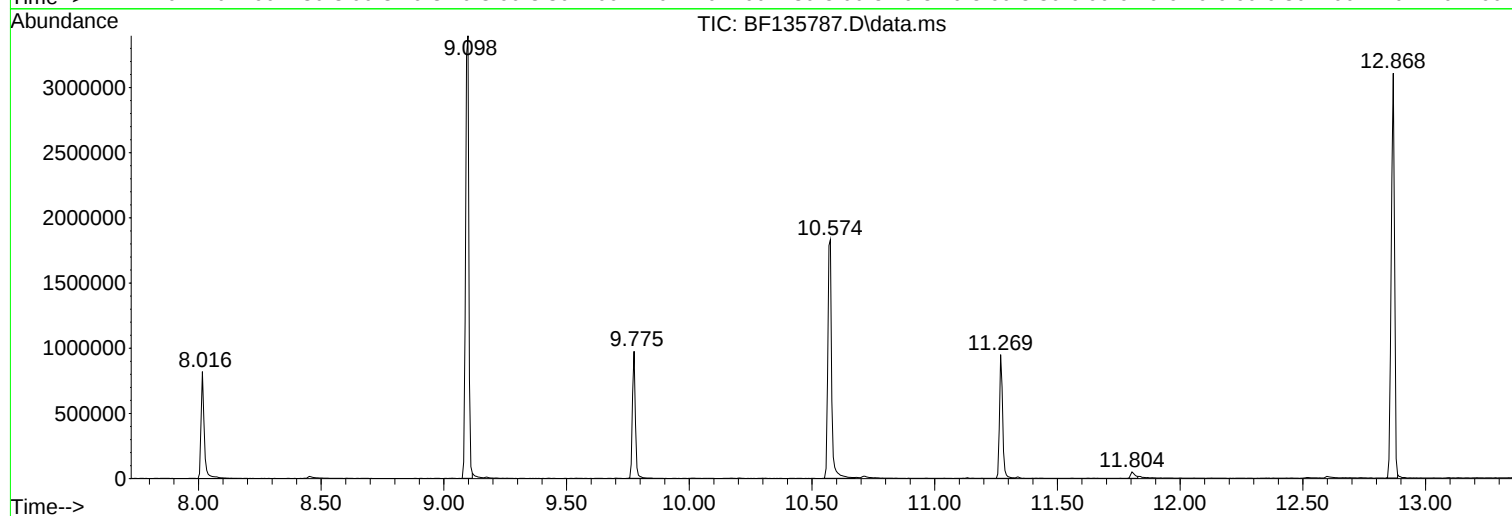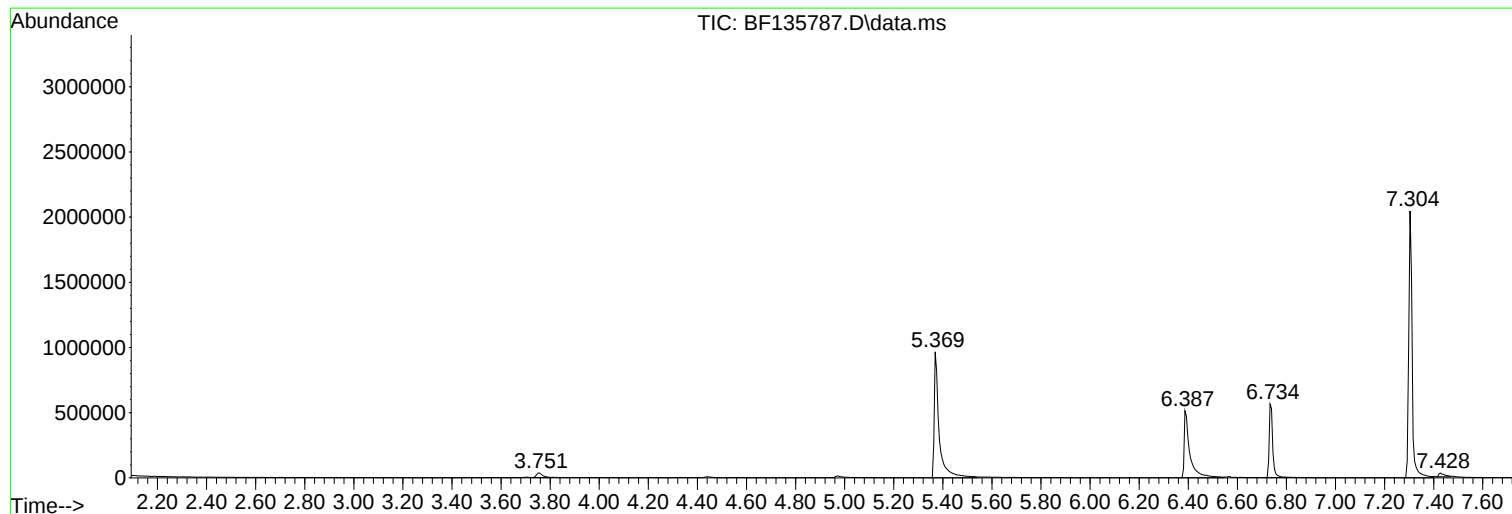

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135787.D
Acq On : 16 Oct 2023 20:52
Operator : CG\JU
Sample : 04656-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135787.D
Acq On : 16 Oct 2023 20:52
Operator : CG\JU
Sample : 04656-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------