
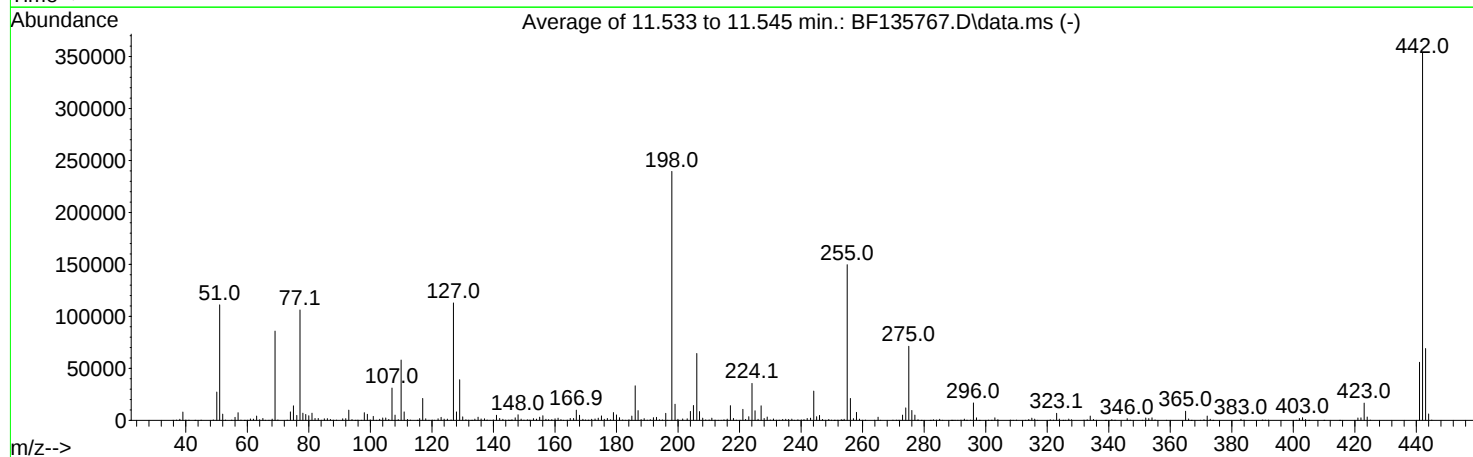


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135767.D
Acq On : 16 Oct 2023 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

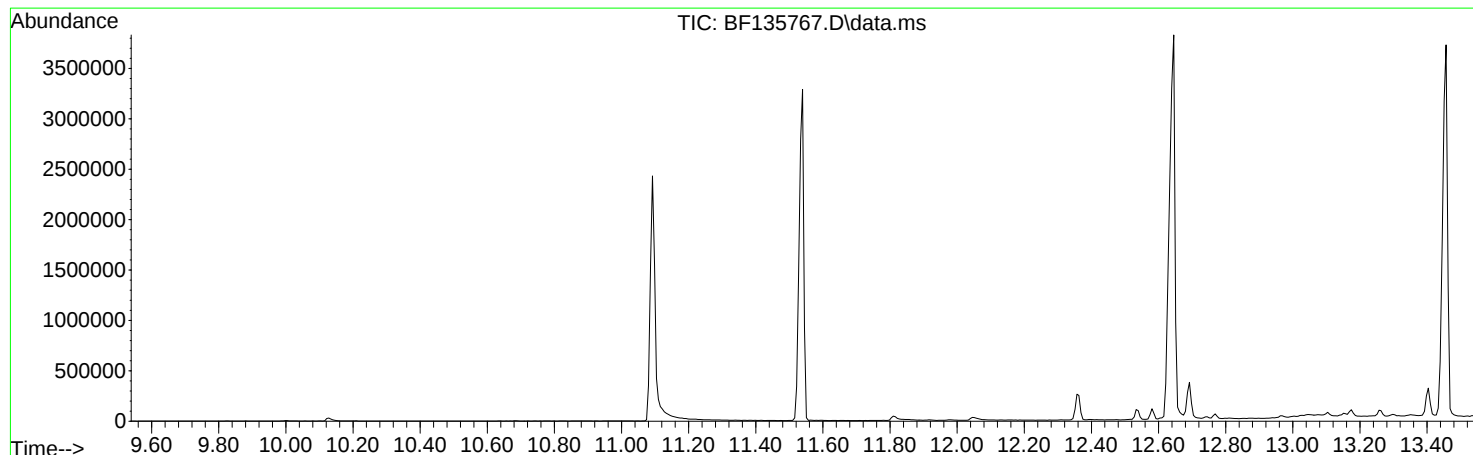




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	111131	PASS
68	69	0.00	2	1.4	1233	PASS
69	198	0.00	100	35.8	85833	PASS
70	69	0.00	2	0.6	483	PASS
127	198	10	80	47.2	113003	PASS
197	198	0.00	2	0.1	159	PASS
198	198	100	100	100.0	239445	PASS
199	198	5	9	6.5	15503	PASS
275	198	10	60	29.8	71272	PASS
365	198	1	100	3.7	8836	PASS
441	198	0.01	100	23.4	55928	PASS
442	442	50	100	100.0	353835	PASS
443	442	15	24	19.5	69091	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135767.D
Acq On : 16 Oct 2023 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:34:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

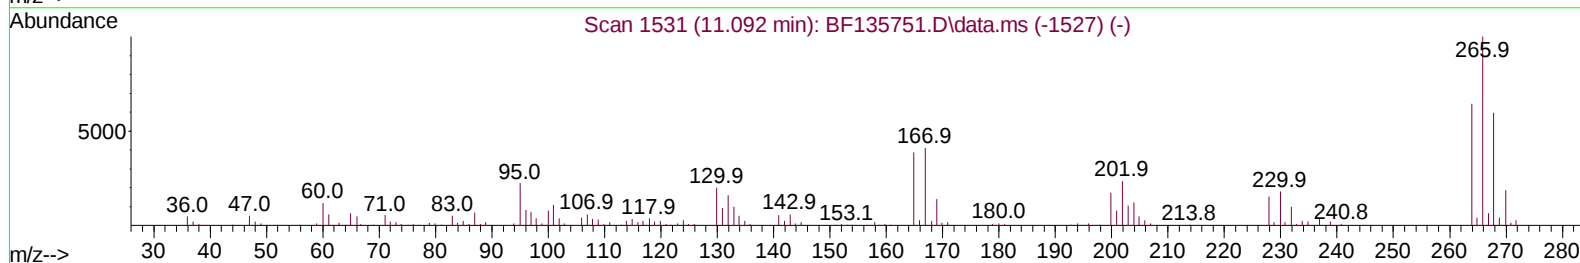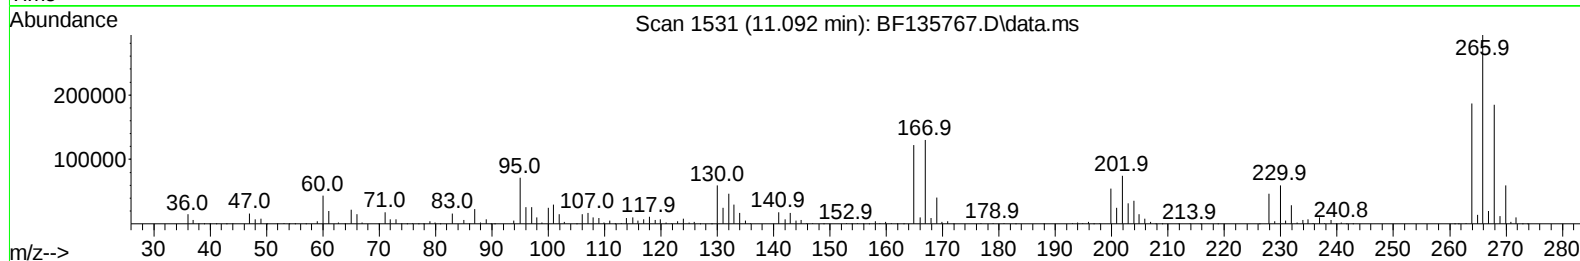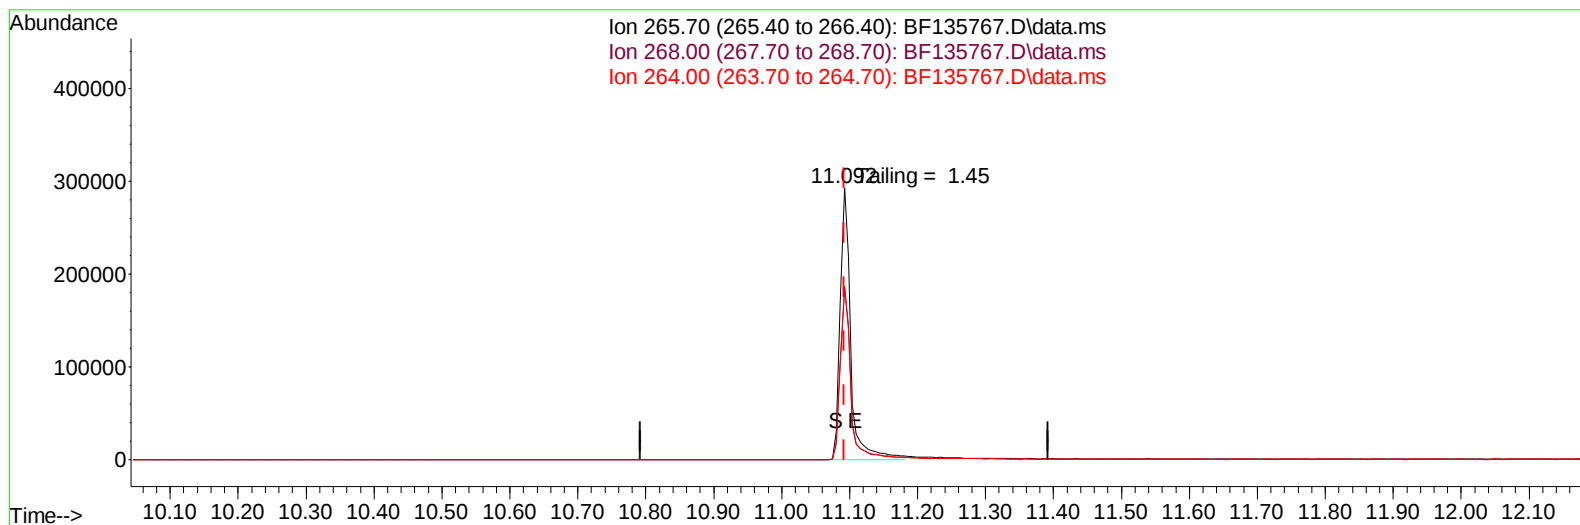

TIC: BF135767.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.000) 896796.83 ng




response 314492

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	62.93
264.00	64.30	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135767.D
Acq On : 16 Oct 2023 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:34:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

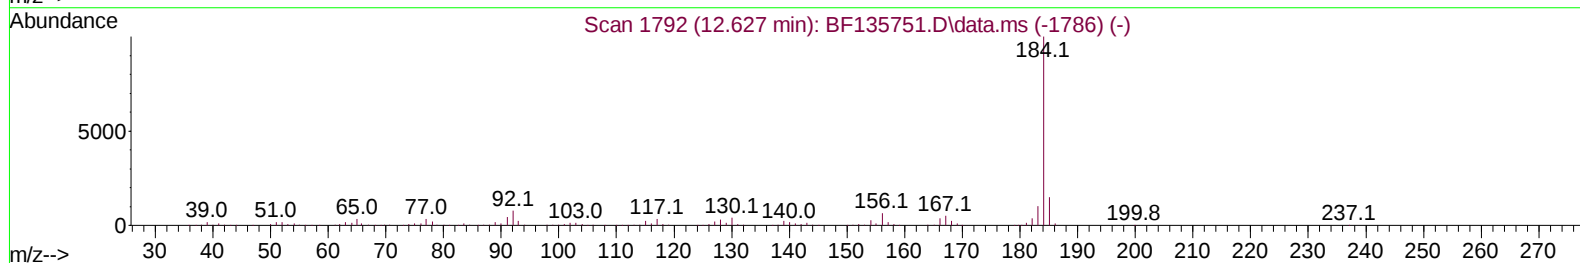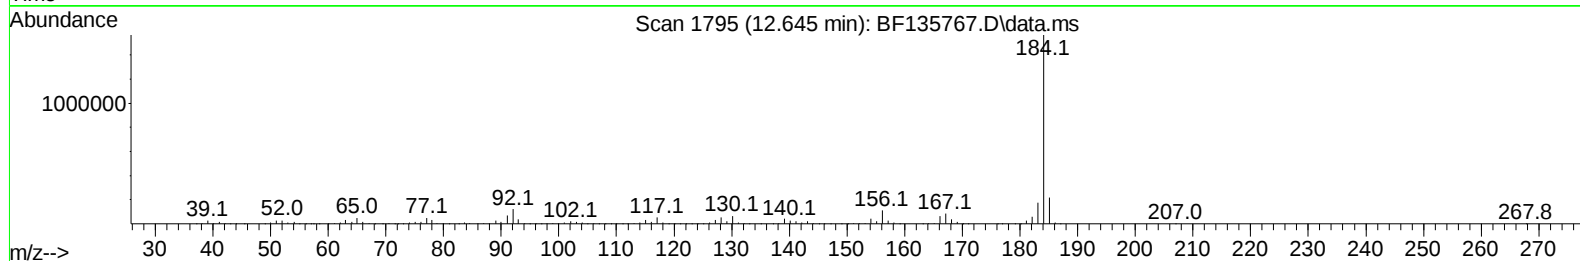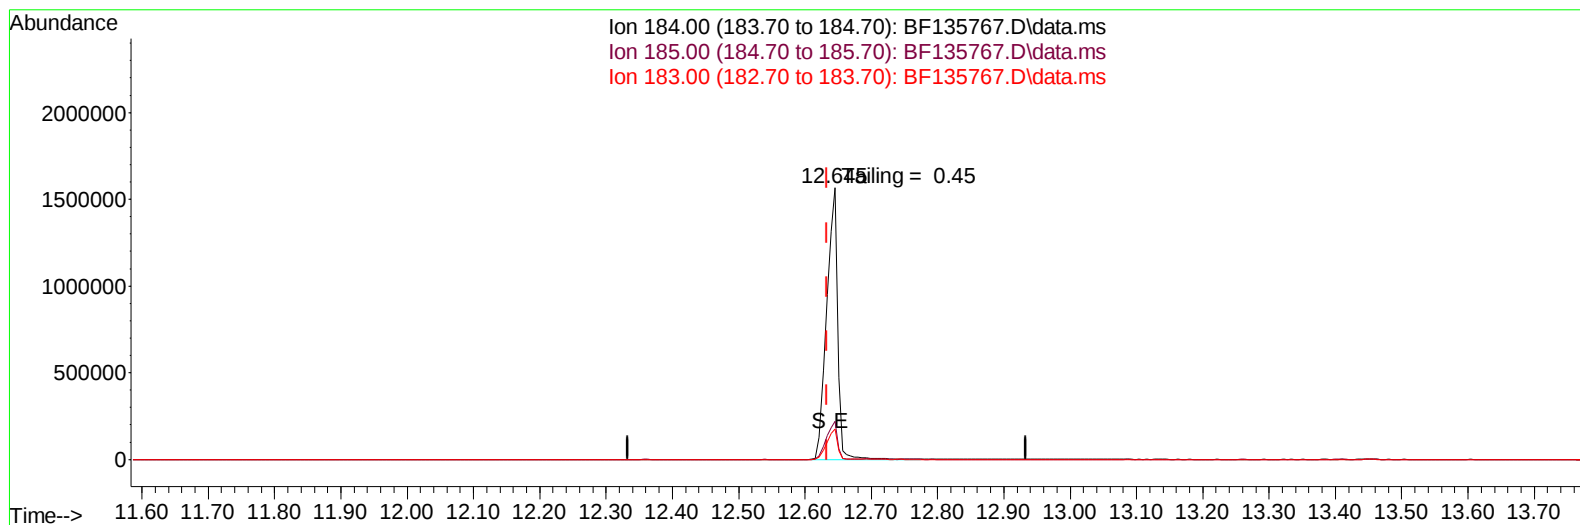

TIC: BF135767.D\data.ms

(77) Benzidine

12.645min (+ 0.012) 7716.52 ng m

response 1820711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.05
183.00	10.20	11.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2023	BNA_F	<u>BF135767.D</u>
Compound Name	Response	Retention Time
DDT	743675	13.457
DDD	17182	13.174
DDE	1133	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18315	761990	2.40

Instrument :
BNA_F
ClientSampleId :
DFTPP