
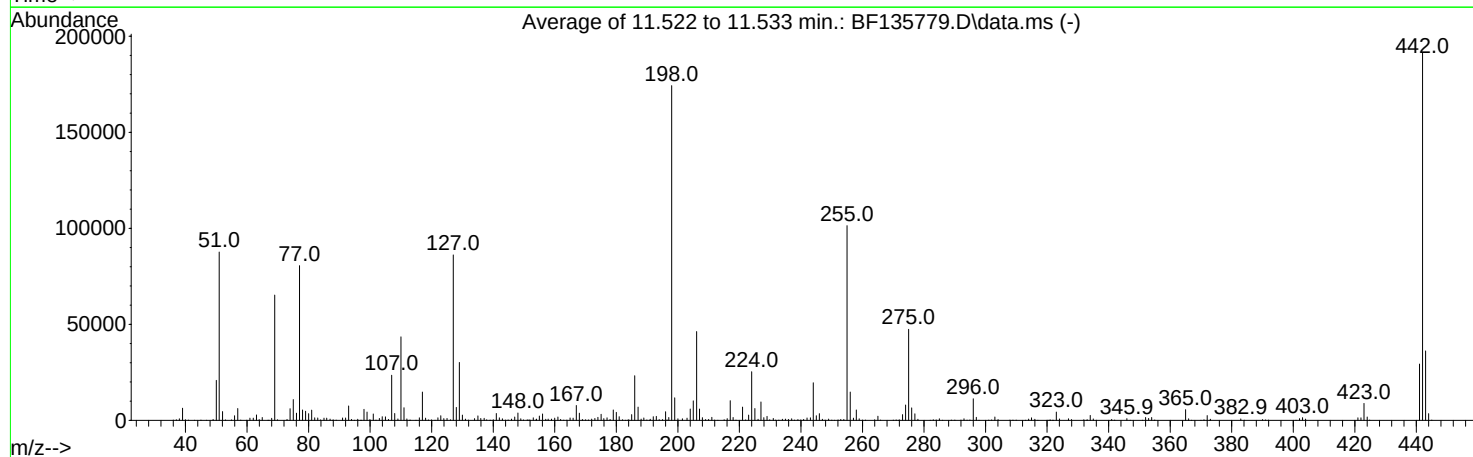


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135779.D
Acq On : 16 Oct 2023 16:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

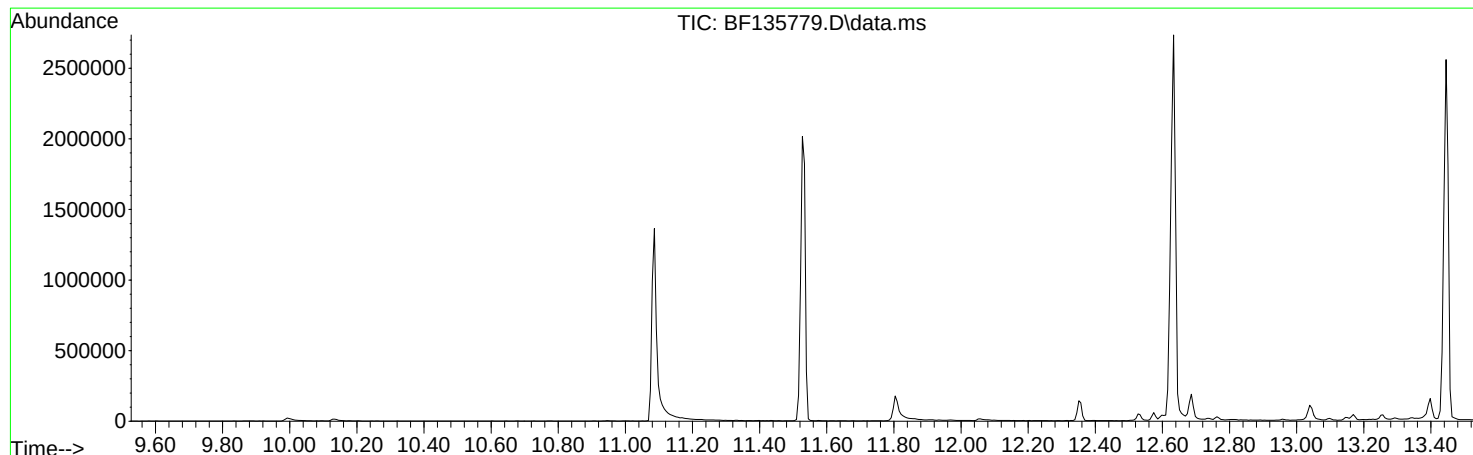




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	87618	PASS
68	69	0.00	2	1.7	1084	PASS
69	198	0.00	100	37.5	65256	PASS
70	69	0.00	2	0.5	357	PASS
127	198	10	80	49.5	86179	PASS
197	198	0.00	2	0.8	1465	PASS
198	198	100	100	100.0	174248	PASS
199	198	5	9	6.7	11714	PASS
275	198	10	60	27.2	47421	PASS
365	198	1	100	3.2	5624	PASS
441	198	0.01	100	16.9	29362	PASS
442	442	50	100	100.0	191541	PASS
443	442	15	24	18.9	36139	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135779.D
Acq On : 16 Oct 2023 16:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:36:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

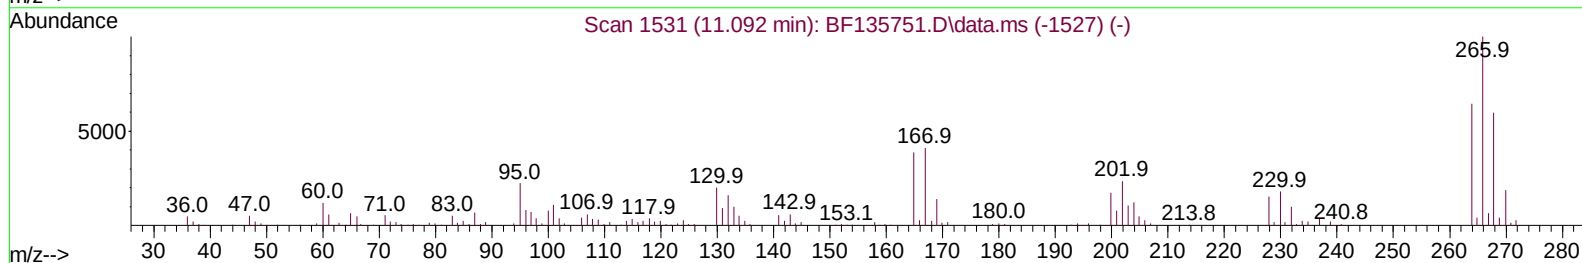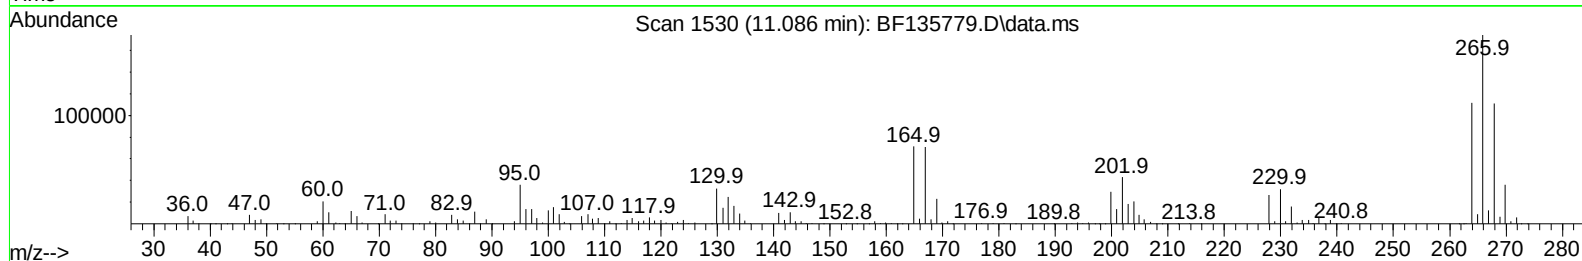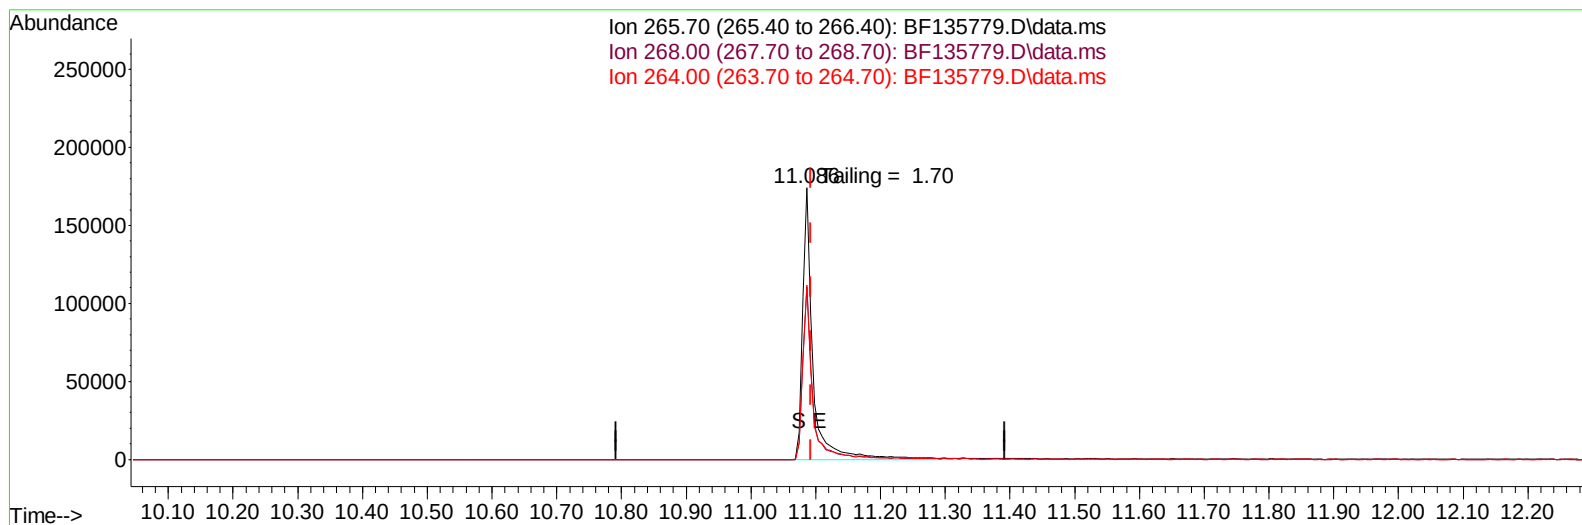

TIC: BF135779.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 852554.83 ng




response 192445

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.63
264.00	64.30	64.27
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101623\
Data File : BF135779.D
Acq On    : 16 Oct 2023 16:30
Operator  : CG\JU
Sample    : DFTPP
Misc      :
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:36:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

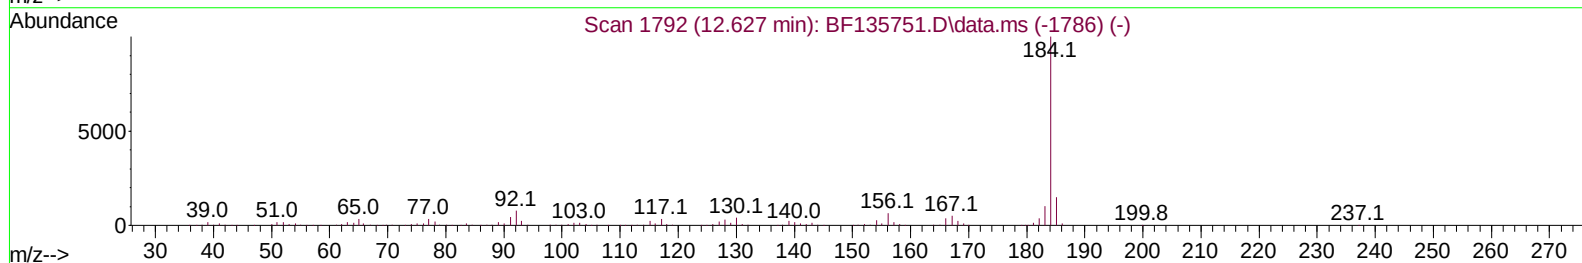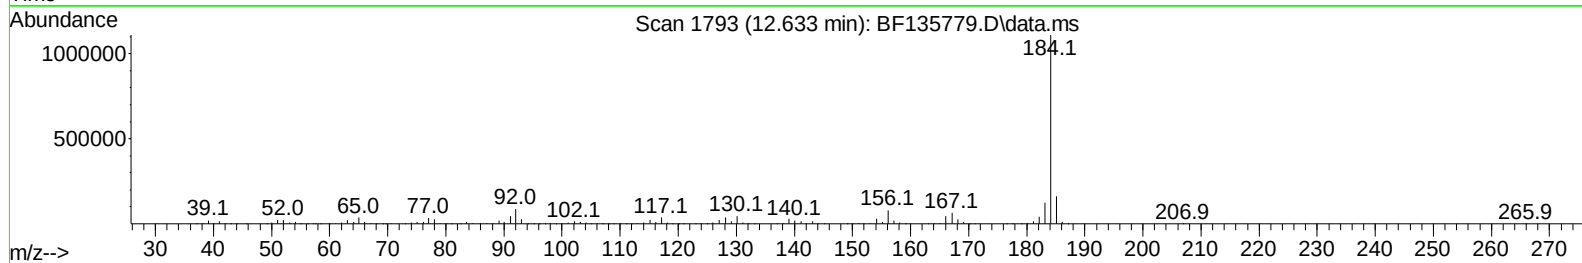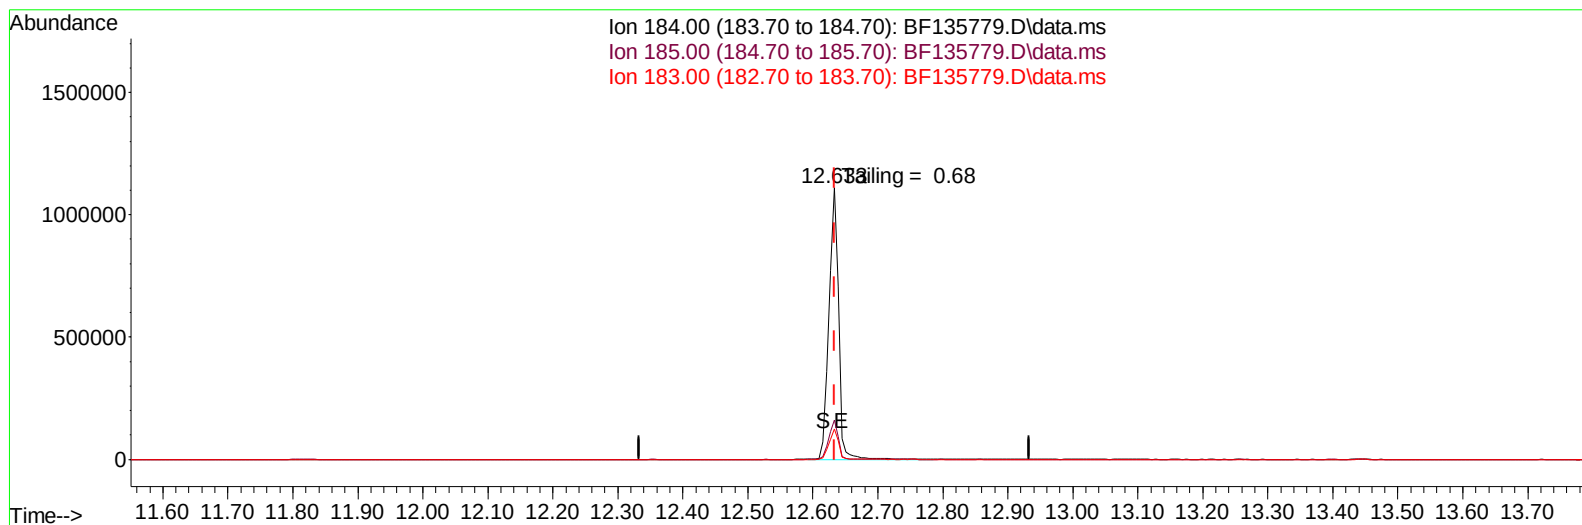

TIC: BF135779.D\data.ms

(77) Benzidine

12.633min (-0.000) 431463.62 ng

response **1148622**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.54
183.00	10.20	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2023	BNA_F	<u>BF135779.D</u>
Compound Name	Response	Retention Time
DDT	476543	13.445
DDD	9996	13.168
DDE	1177	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11173	487716	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP