
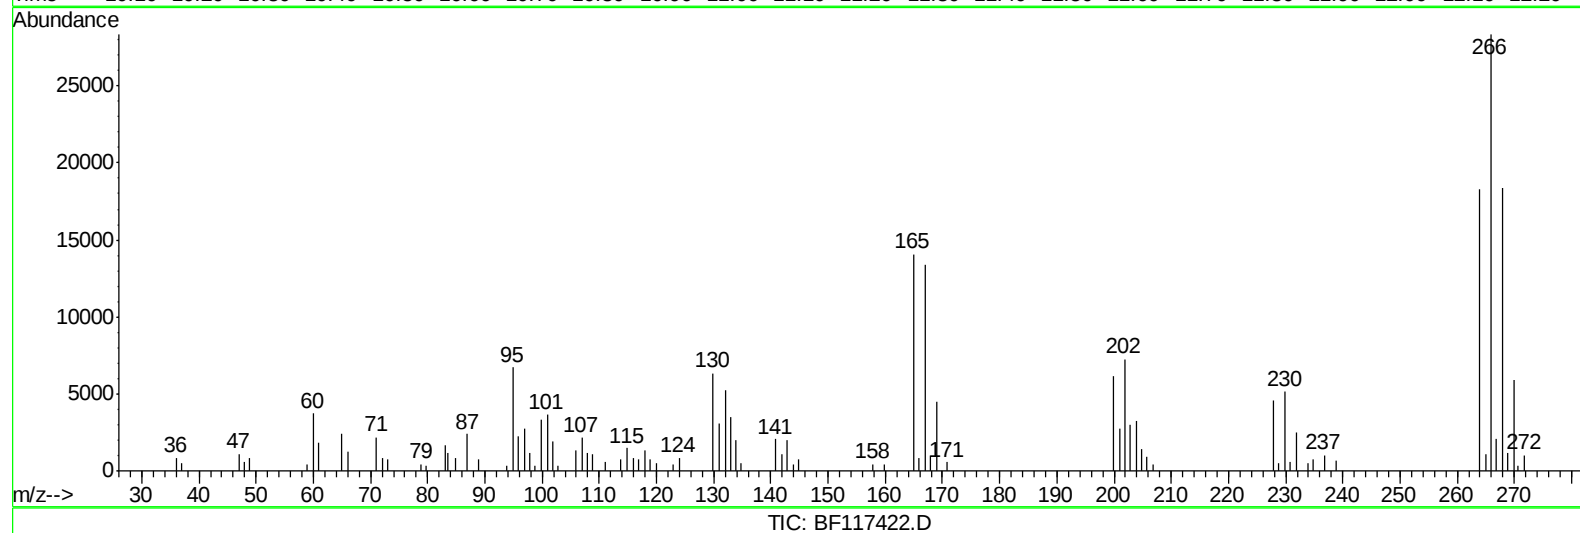


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101719\
Data File : BF117422.D
Acq On : 17 Oct 2019 15:16
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 09:22:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 19:03:29 2019
Response via : Initial Calibration

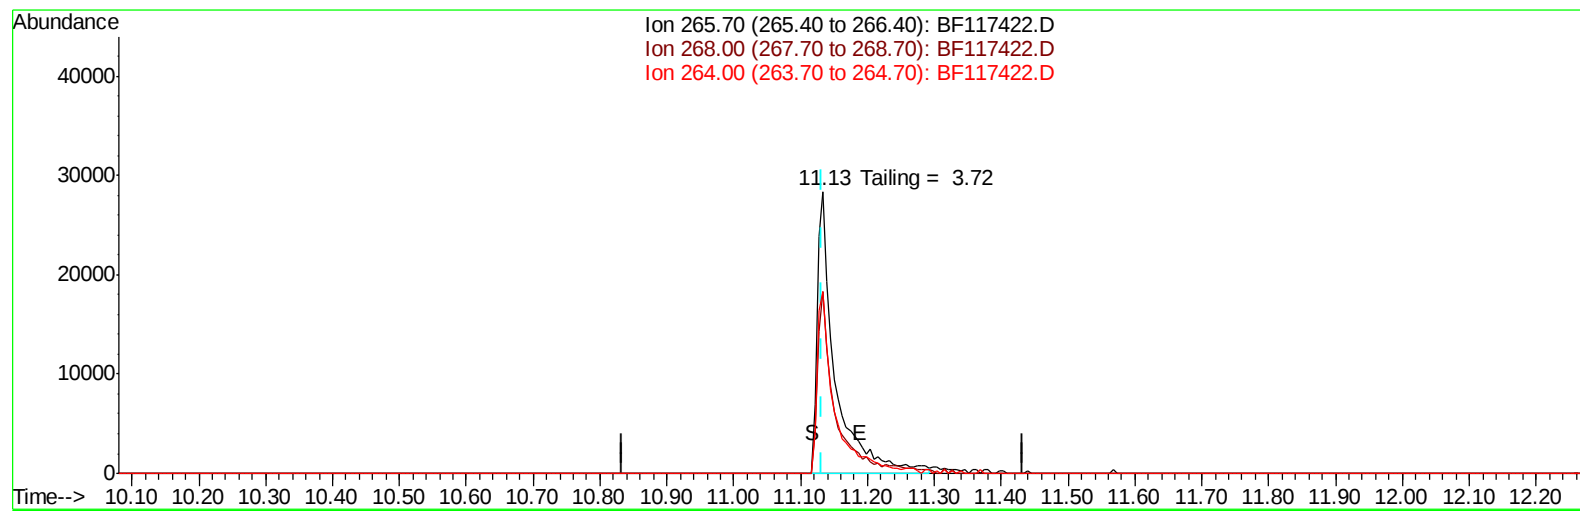

(70) Pentachlorophenol (C)



11.133min (+0.000) 62129.02ng

response 52546

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	64.69
264.00	53.60	64.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101719\
Data File : BF117422.D
Acq On : 17 Oct 2019 15:16
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 09:22:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 19:03:29 2019
Response via : Initial Calibration

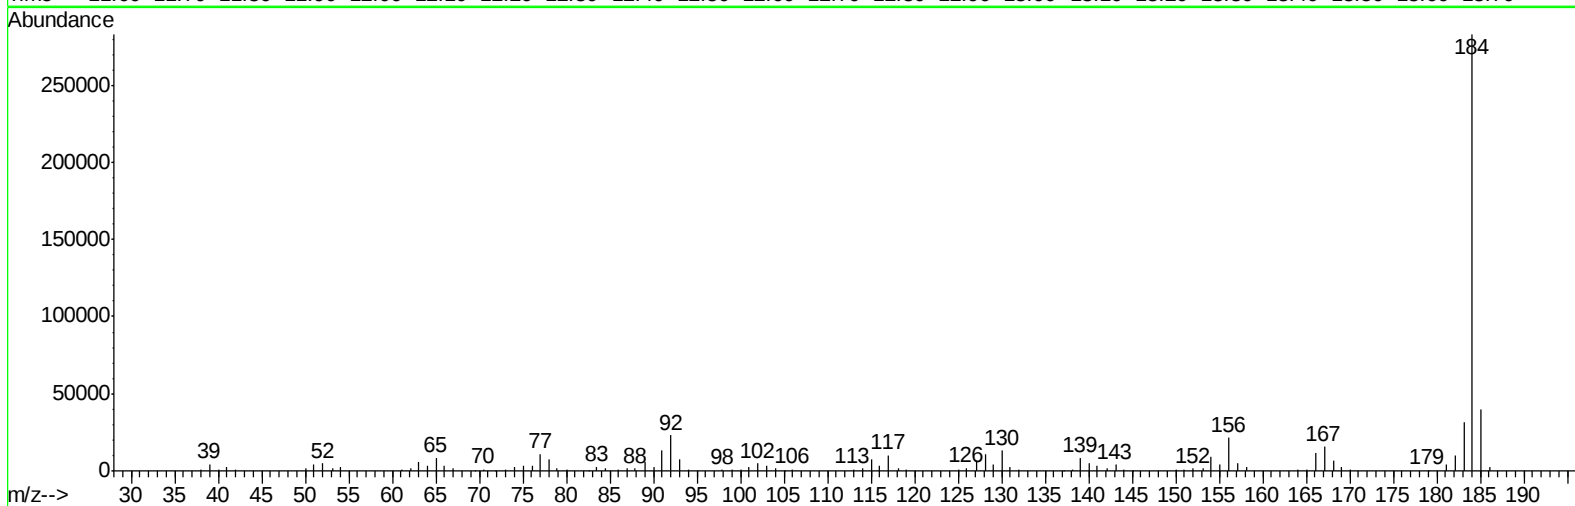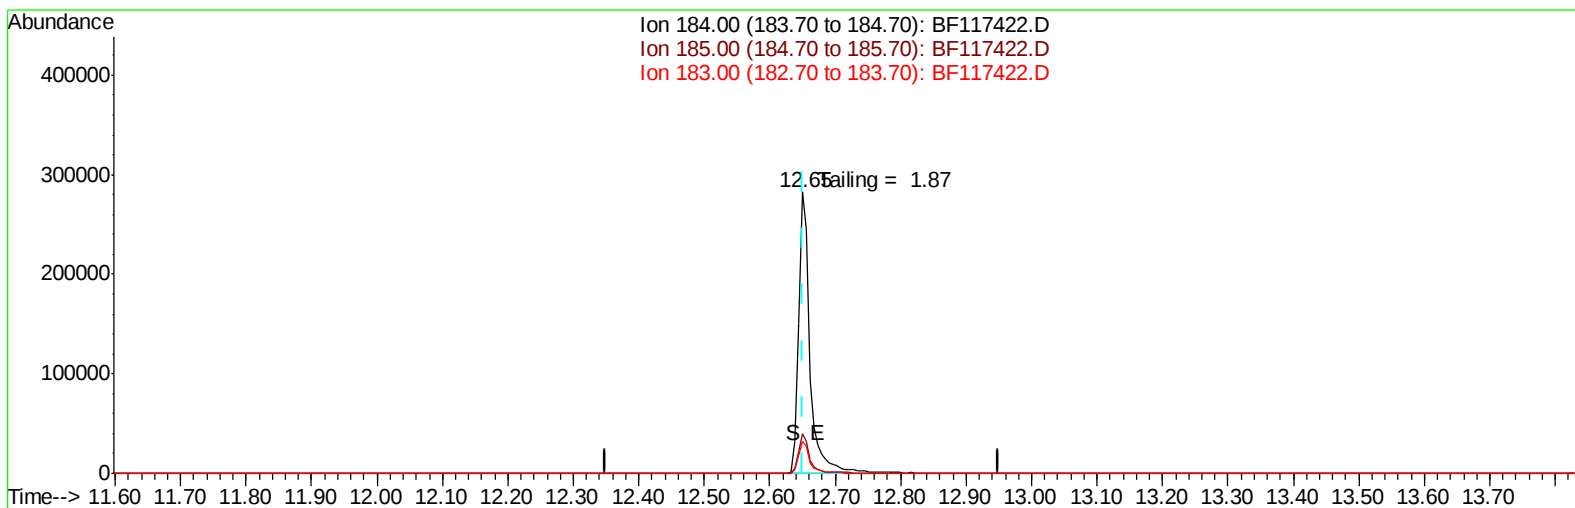

TIC: BF117422.D

(77) Benzidine

12.651min (+0.000) 0.00ng

response 345422

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.14
183.00	11.10	11.20
0.00	0.00	0.00