

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
 Data File : BF135822.D
 Acq On : 17 Oct 2023 20:30
 Operator : CG\JU
 Sample : 04740-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BW1D

Quant Time: Oct 18 02:01:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 17 01:22:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.740	152	77843	20.000	ng	0.00
21) Naphthalene-d8	8.016	136	294458	20.000	ng	0.00
39) Acenaphthene-d10	9.775	164	147965	20.000	ng	-0.01
64) Phenanthrene-d10	11.269	188	281313	20.000	ng	-0.01
76) Chrysene-d12	13.933	240	153722	20.000	ng	#-0.02
86) Perylene-d12	15.410	264	173538	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	320152	66.123	ng	0.00
7) Phenol-d6	6.392	99	222897	36.896	ng	0.00
23) Nitrobenzene-d5	7.304	82	543428	101.502	ng	-0.01
42) 2,4,6-Tribromophenol	10.575	330	221856	156.254	ng	-0.01
45) 2-Fluorobiphenyl	9.092	172	974415	102.964	ng	-0.01
79) Terphenyl-d14	12.869	244	930005	112.039	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135822.D
Acq On : 17 Oct 2023 20:30
Operator : CG\JU
Sample : 04740-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BW1D

Quant Time: Oct 18 02:01:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration




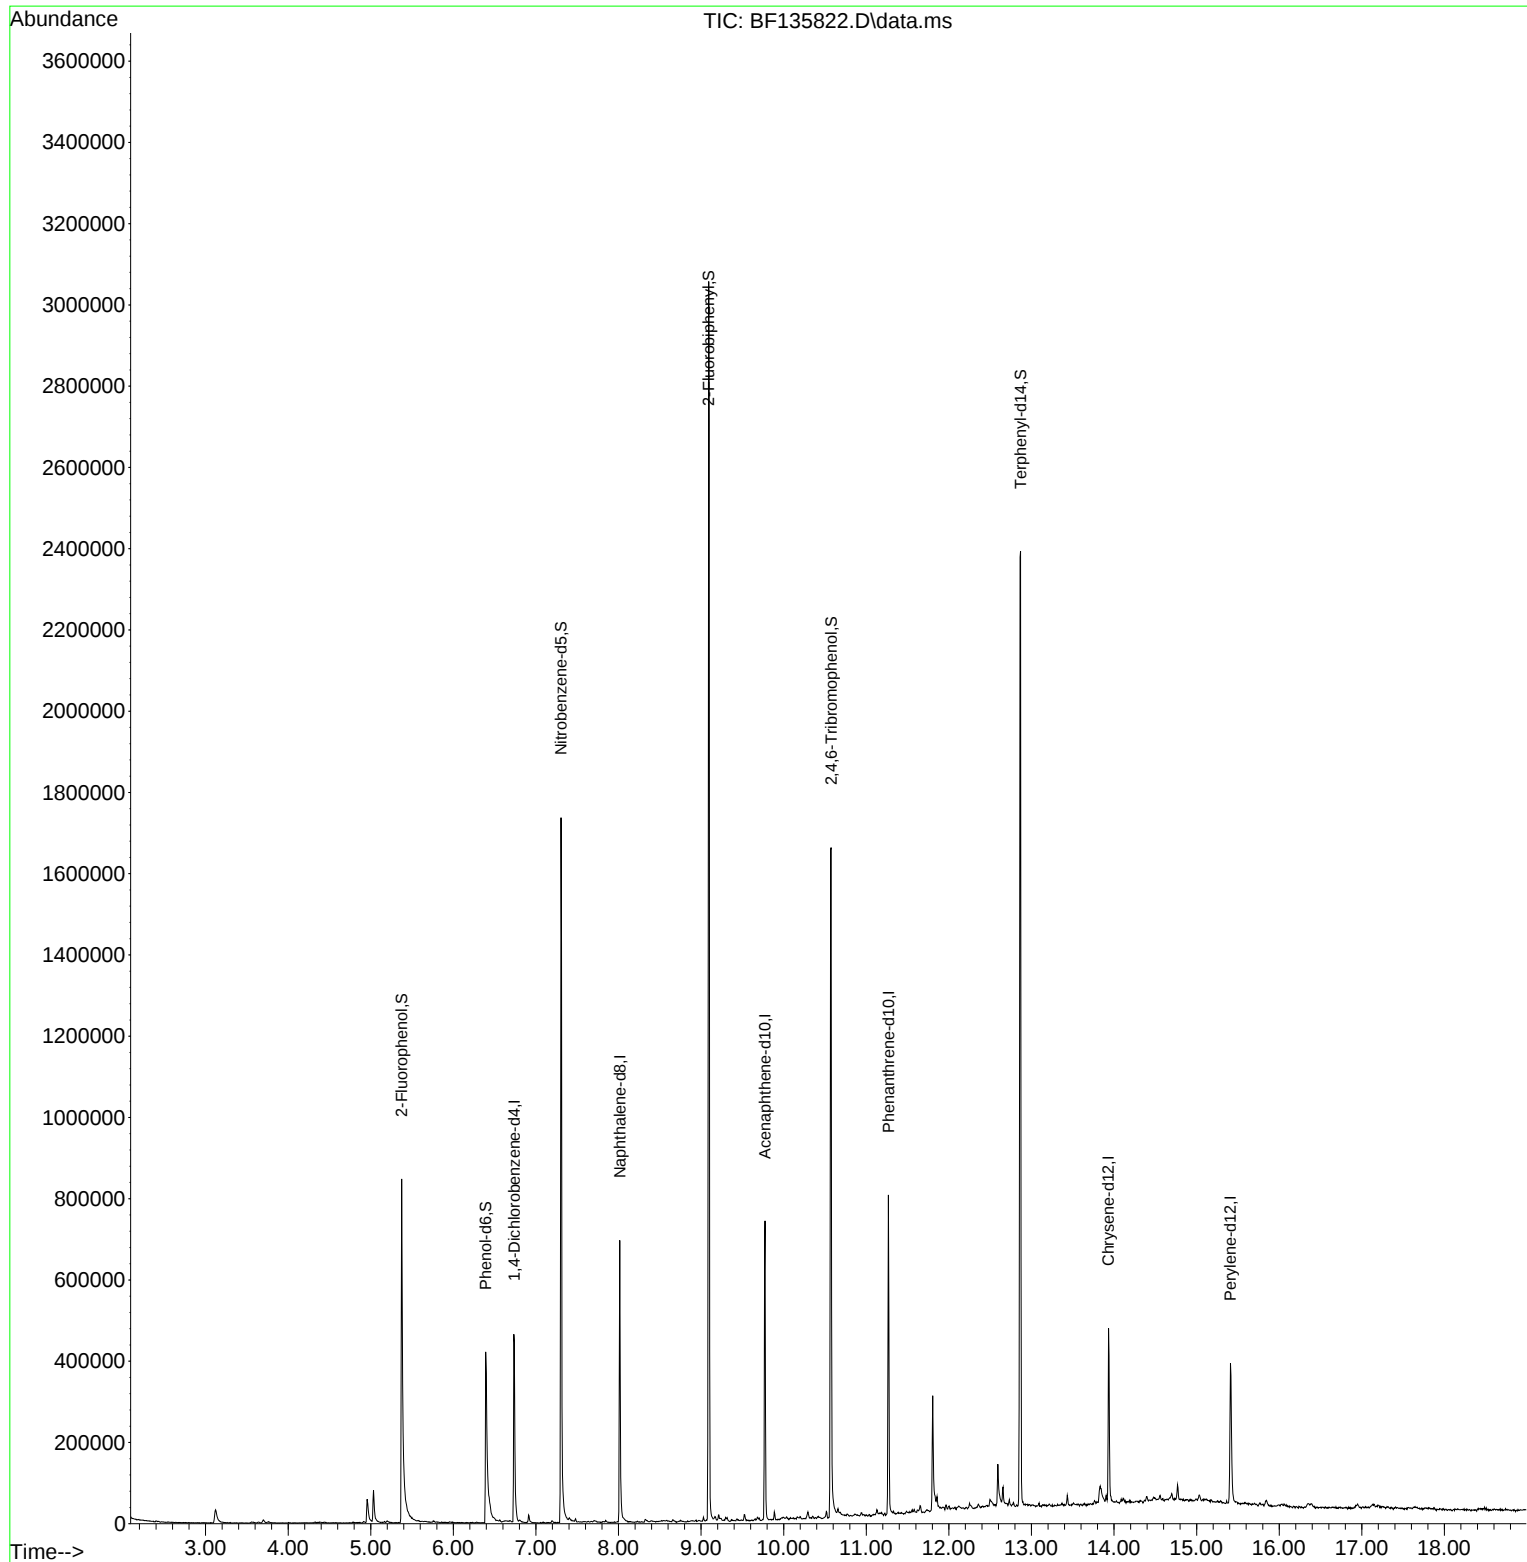




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.740 min Scan# 791
Delta R.T. -0.006 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30




Instrument :
BNA_F
ClientSampleId :
BW1D


Tgt Ion:152 Resp: 77843
Ion Ratio Lower Upper
152 100
150 148.3 124.5 186.7
115 56.7 49.0 73.4

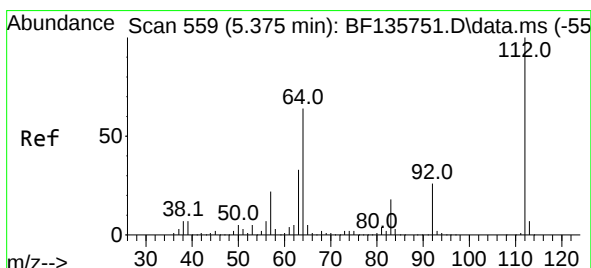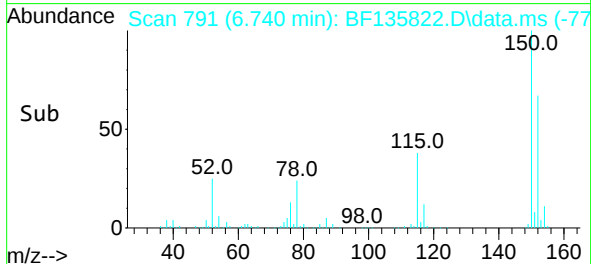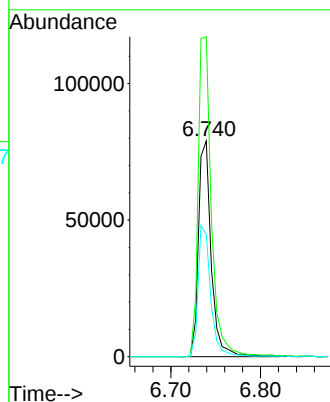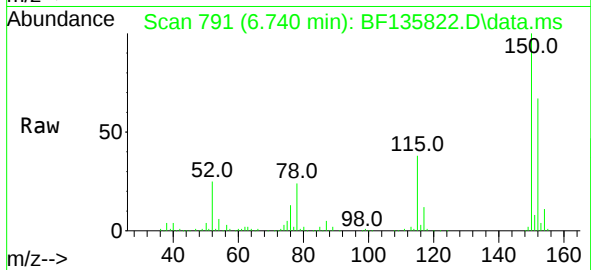

#5
2-Fluorophenol
Concen: 66.123 ng
RT: 5.375 min Scan# 559
Delta R.T. -0.000 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30

Tgt Ion:112 Resp: 320152
Ion Ratio Lower Upper
112 100
64 64.5 51.2 76.8
63 34.8 26.1 39.1


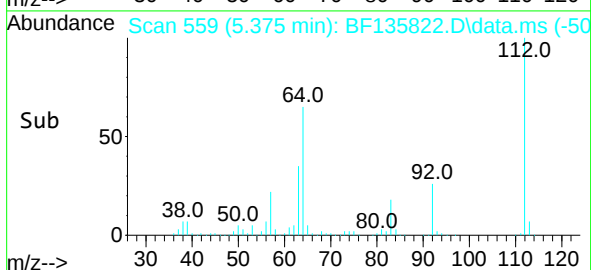
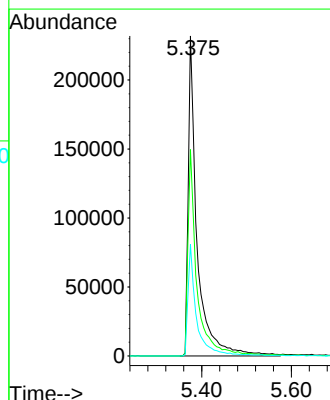
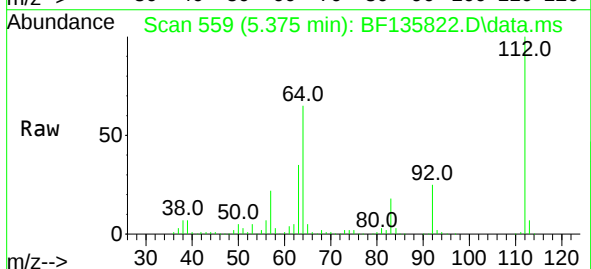


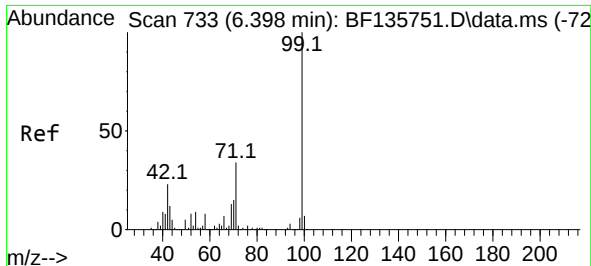

#7
Phenol-d6
Concen: 36.896 ng
RT: 6.392 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30




Instrument :
BNA_F
ClientSampleId :
BW1D


Tgt Ion: 99 Resp: 222897
Ion Ratio Lower Upper
99 100
42 22.9 18.4 27.6
71 33.9 27.2 40.8

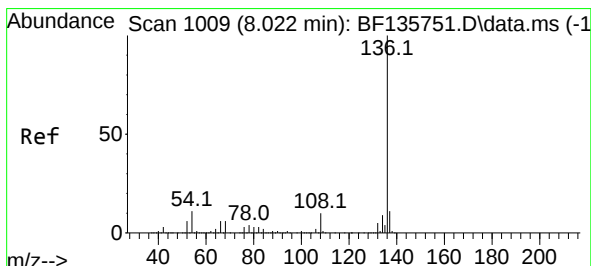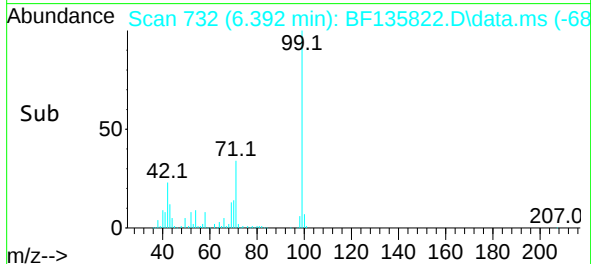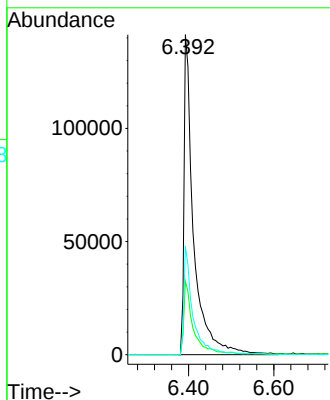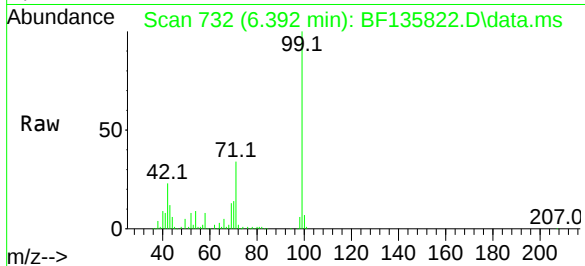

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30

Tgt Ion: 136 Resp: 294458
Ion Ratio Lower Upper
136 100
137 11.1 8.6 12.8
54 9.2 8.5 12.7
68 5.3 4.8 7.2


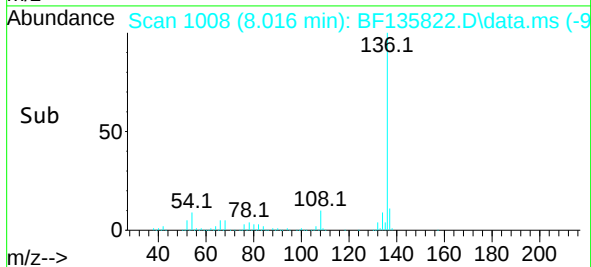
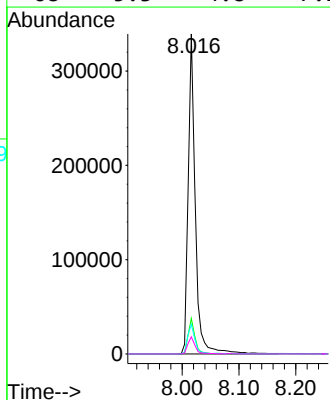
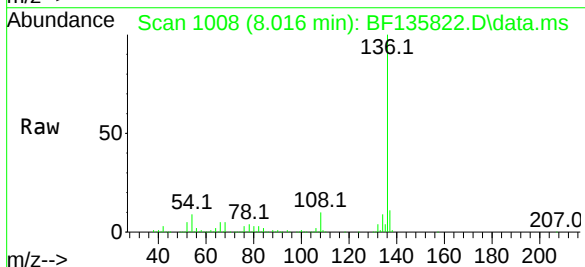


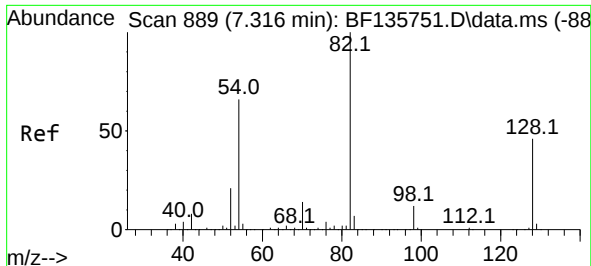

#23
Nitrobenzene-d5
Concen: 101.502 ng
RT: 7.304 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30




Instrument :
BNA_F
ClientSampleId :
BW1D

Tgt Ion: 82 Resp: 543428
Ion Ratio Lower Upper
82 100
128 42.6 37.0 55.6
54 64.5 52.8 79.2

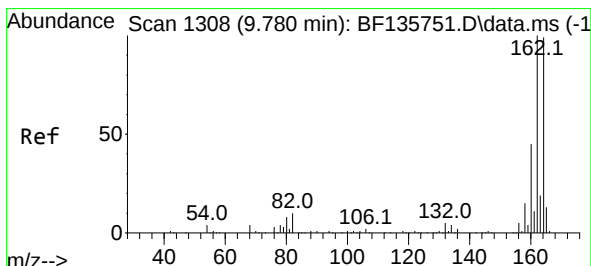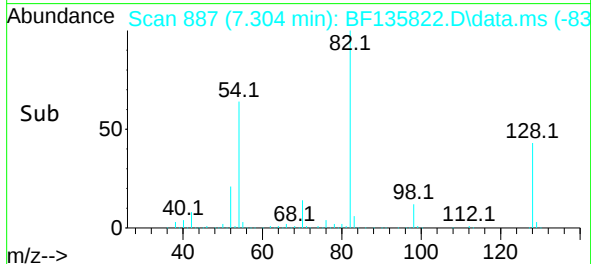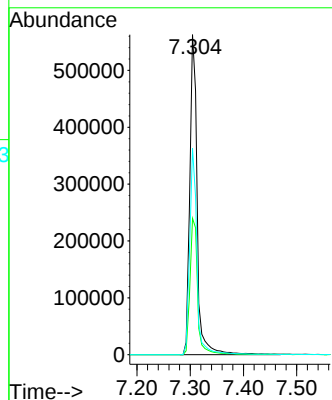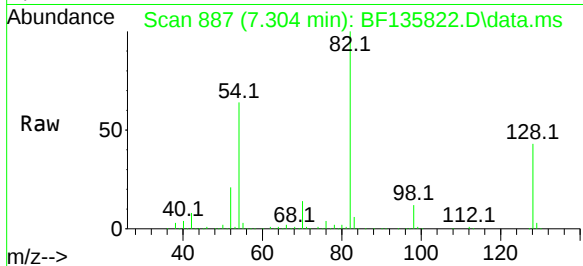

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.775 min Scan# 1307
Delta R.T. -0.012 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30

Tgt Ion:164 Resp: 147965
Ion Ratio Lower Upper
164 100
162 101.6 80.8 121.2
160 45.4 36.6 54.8


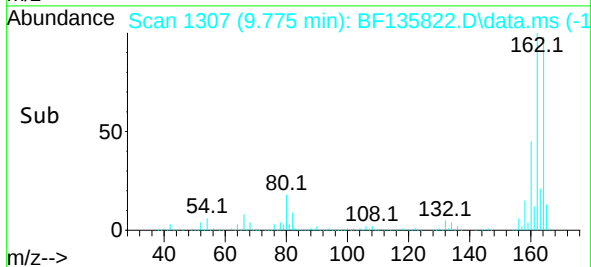
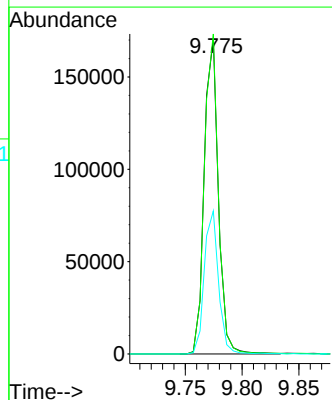
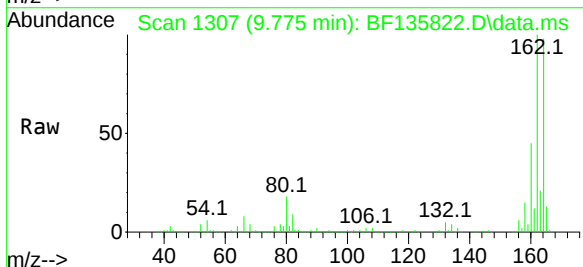




#42
2,4,6-Tribromophenol
Concen: 156.254 ng
RT: 10.575 min Scan# 1444
Delta R.T. -0.012 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30




Instrument :
BNA_F
ClientSampleId :
BW1D


Tgt Ion:330 Resp: 221856
Ion Ratio Lower Upper
330 100
332 95.7 75.0 112.4
141 31.5 25.8 38.6

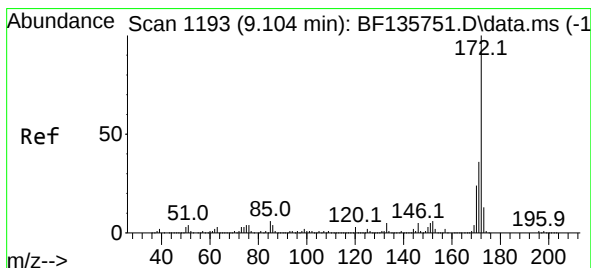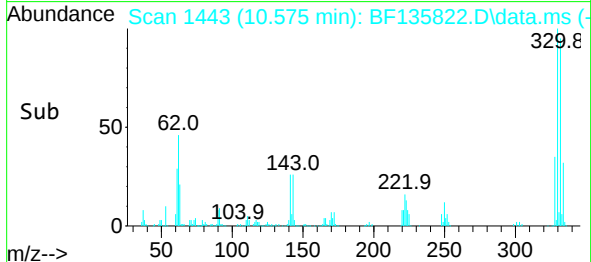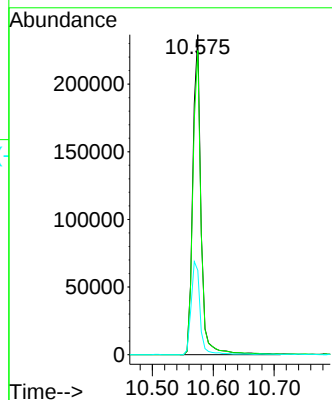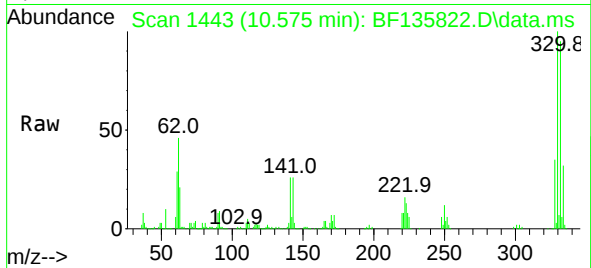

#45
2-Fluorobiphenyl
Concen: 102.964 ng
RT: 9.092 min Scan# 1191
Delta R.T. -0.012 min
Lab File: BF135822.D
Acq: 17 Oct 2023 20:30

Tgt Ion:172 Resp: 974415
Ion Ratio Lower Upper
172 100
171 36.0 28.4 42.6
170 23.7 18.8 28.2

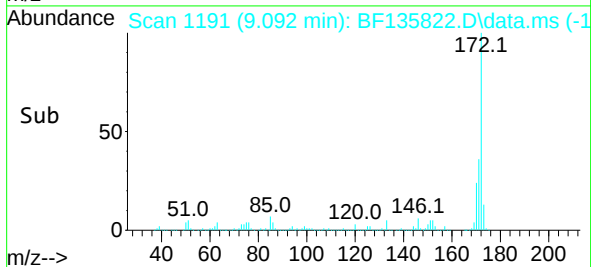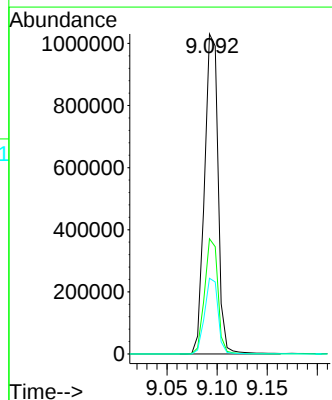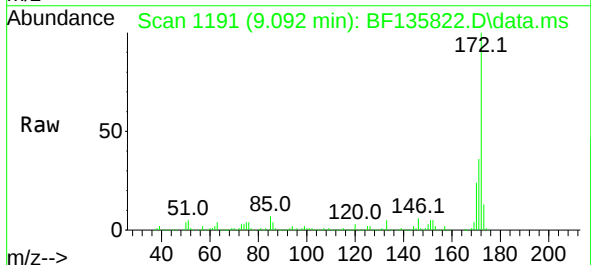

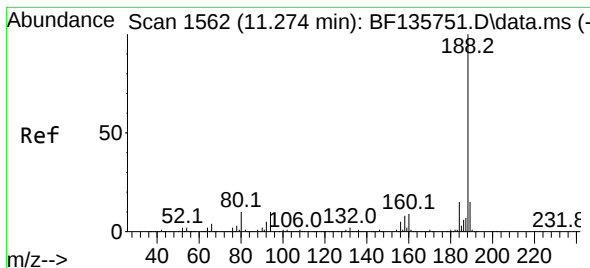

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.269 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF135822.D

Acq: 17 Oct 2023 20:30

Instrument :

BNA_F

ClientSampleId :

BW1D





Tgt Ion:188 Resp: 281313

Ion Ratio Lower Upper

188 100

94 9.4 8.0 12.0

80 9.4 8.3 12.5

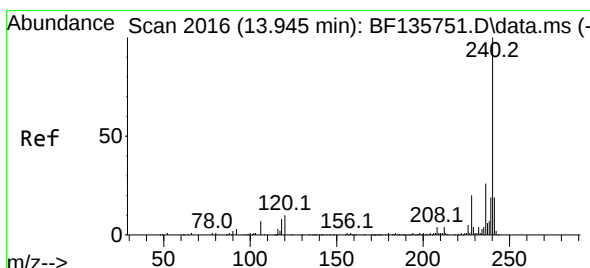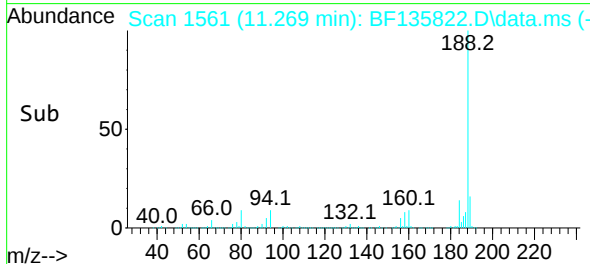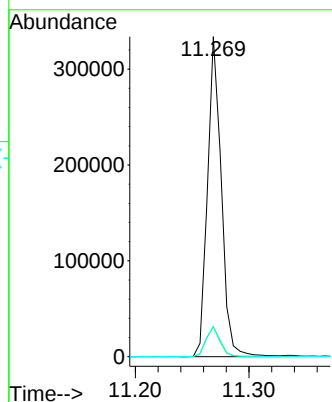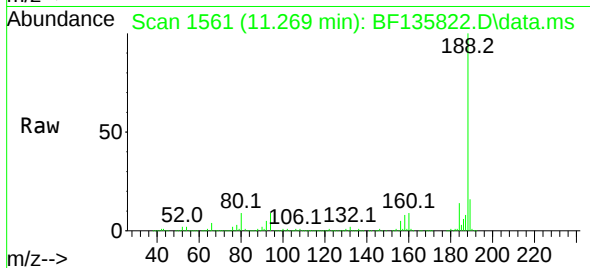

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.933 min Scan# 2014

Delta R.T. -0.018 min

Lab File: BF135822.D

Acq: 17 Oct 2023 20:30




Tgt Ion:240 Resp: 153722


Ion Ratio Lower Upper

240 100

120 12.4 8.2 12.2#

236 25.2 21.2 31.8

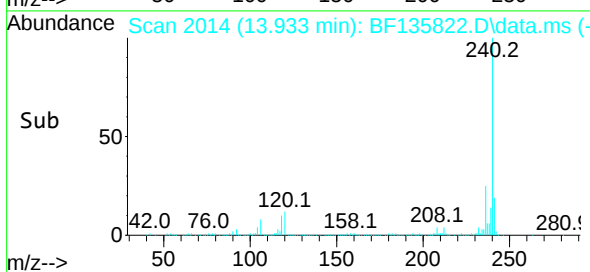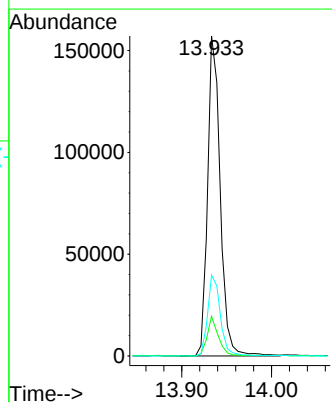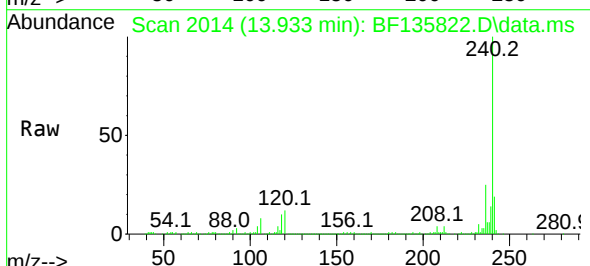

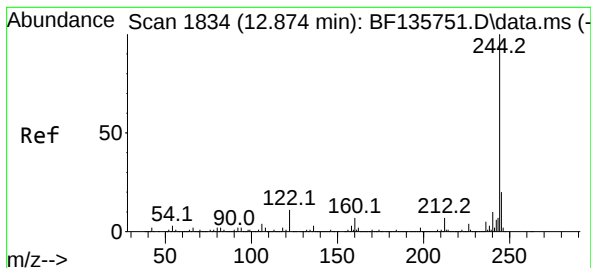

#79

Terphenyl-d14

Concen: 112.039 ng

RT: 12.869 min Scan# 1833

Delta R.T. -0.012 min

Lab File: BF135822.D

Acq: 17 Oct 2023 20:30

Instrument :

BNA_F

ClientSampleId :

BW1D





Tgt Ion:244 Resp: 930005

Ion Ratio Lower Upper

244 100

212 6.3 5.6 8.4

122 9.6 9.0 13.6

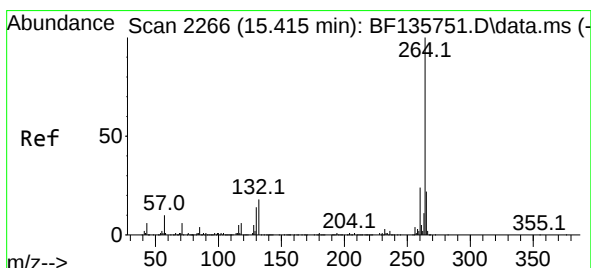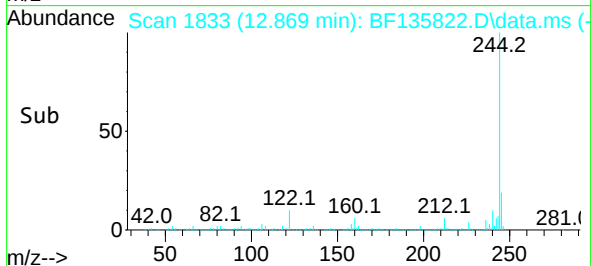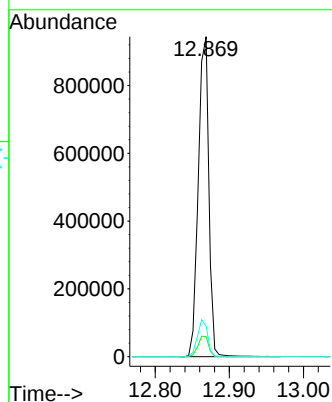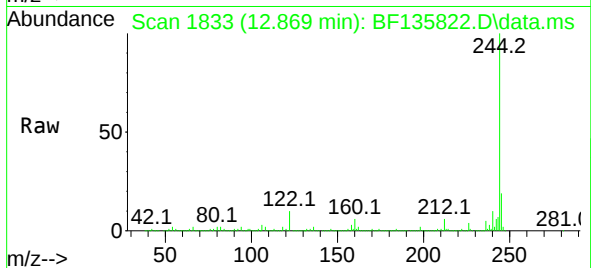

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.410 min Scan# 2265

Delta R.T. -0.012 min

Lab File: BF135822.D

Acq: 17 Oct 2023 20:30

Tgt Ion:264 Resp: 173538

Ion Ratio Lower Upper

264 100

260 24.2 19.2 28.8

265 20.1 17.4 26.2

