

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
 Data File : BF135804.D
 Acq On : 17 Oct 2023 10:56
 Operator : CG\JU
 Sample : PB156118BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156118BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	557	561	580	rBV	3375042	3531221	88.12%	13.924%
2	6.398	728	733	757	rBV	3155753	3548139	88.55%	13.991%
3	6.734	787	790	802	rBV	758932	704515	17.58%	2.778%
4	7.310	883	888	891	rBV	2426615	2227412	55.59%	8.783%
5	8.016	1005	1008	1026	rVB	1063327	921195	22.99%	3.632%
6	9.098	1186	1192	1195	rBV	4155426	3873299	96.66%	15.273%
7	9.775	1303	1307	1321	rVB	1313929	1073214	26.78%	4.232%
8	10.575	1439	1443	1456	rBV	2521421	2603350	64.97%	10.266%
9	11.269	1558	1561	1570	rBV	1237017	1164179	29.05%	4.591%
10	12.874	1828	1834	1837	rBV	3784167	4007136	100.00%	15.801%
11	13.939	2011	2015	2027	rVB	894910	923649	23.05%	3.642%
12	15.415	2261	2266	2275	rVB	568093	782697	19.53%	3.086%




Sum of corrected areas: 25360006

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135804.D
Acq On : 17 Oct 2023 10:56
Operator : CG\JU
Sample : PB156118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

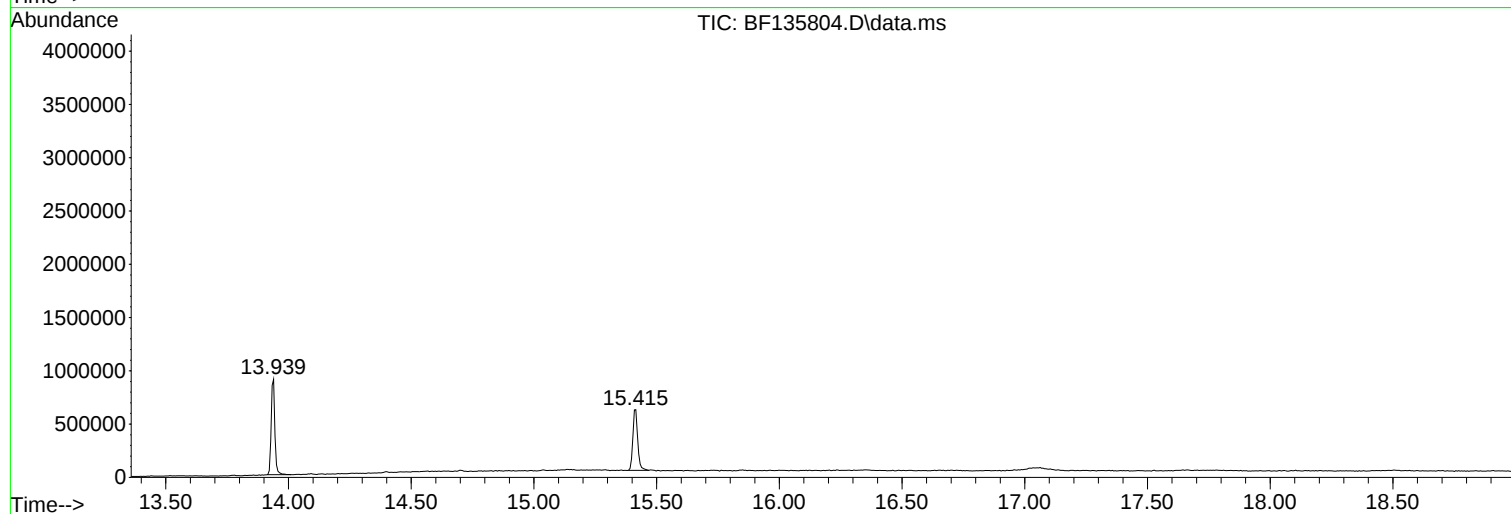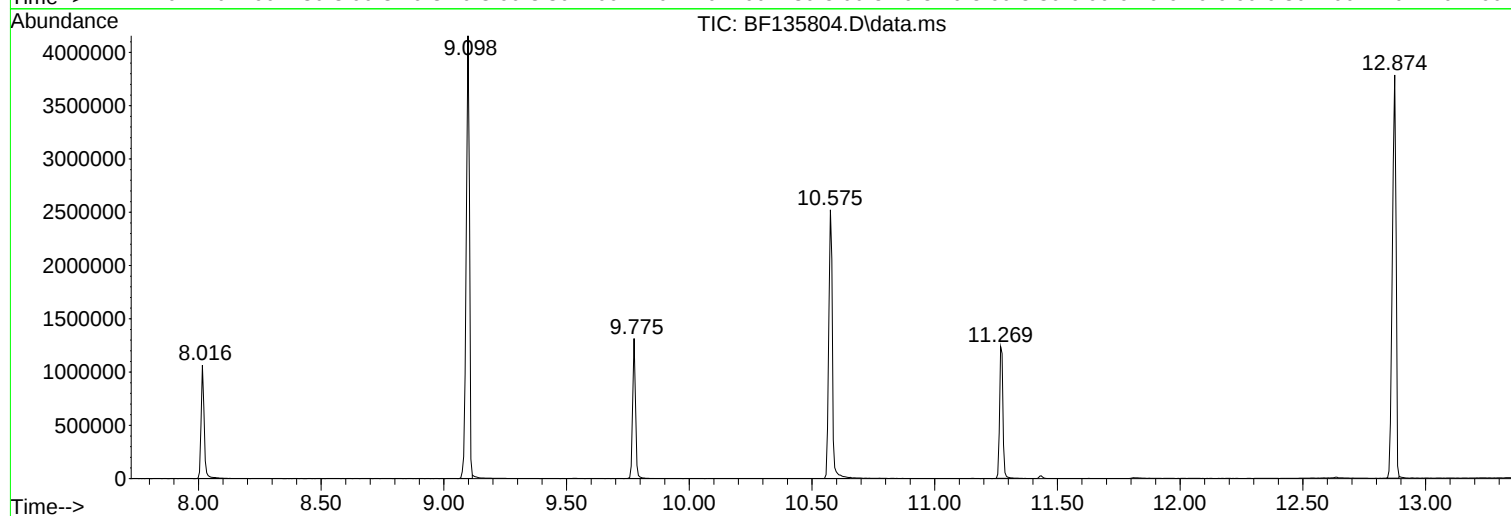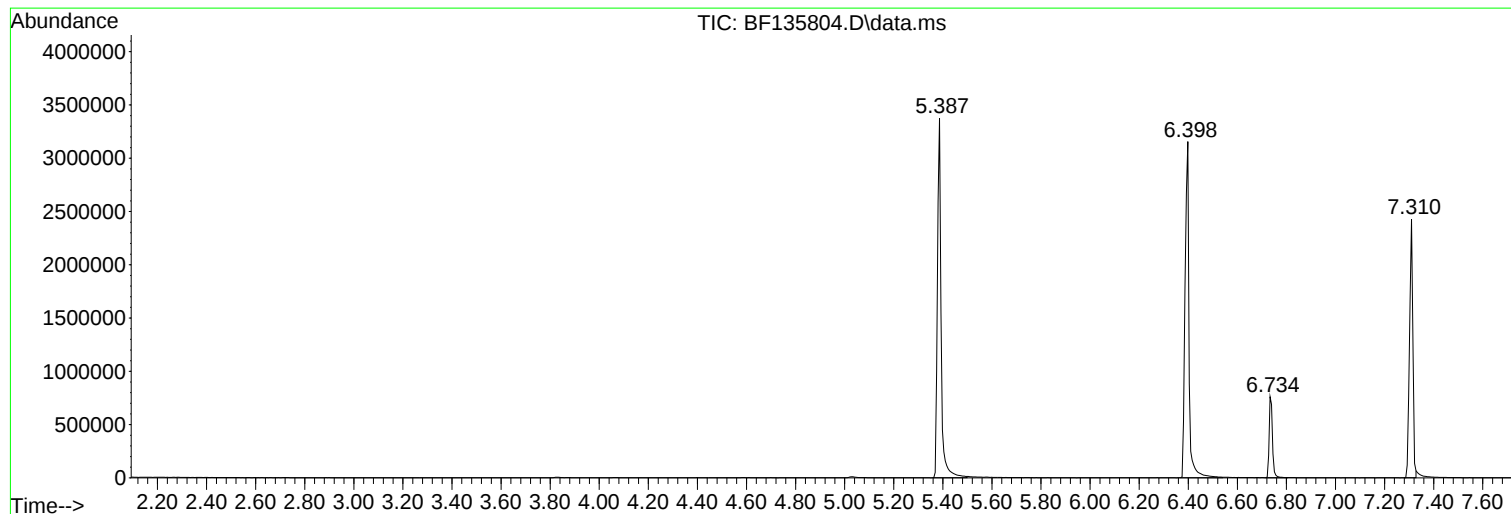

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135804.D
Acq On : 17 Oct 2023 10:56
Operator : CG\JU
Sample : PB156118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135804.D
Acq On : 17 Oct 2023 10:56
Operator : CG\JU
Sample : PB156118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------