
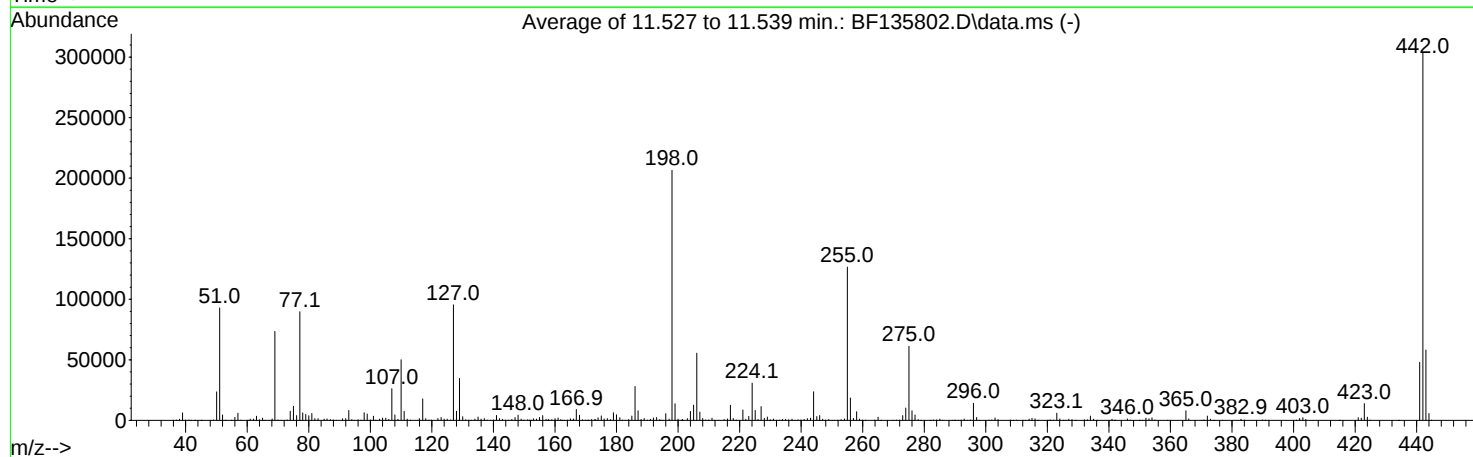


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135802.D
Acq On : 17 Oct 2023 09:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

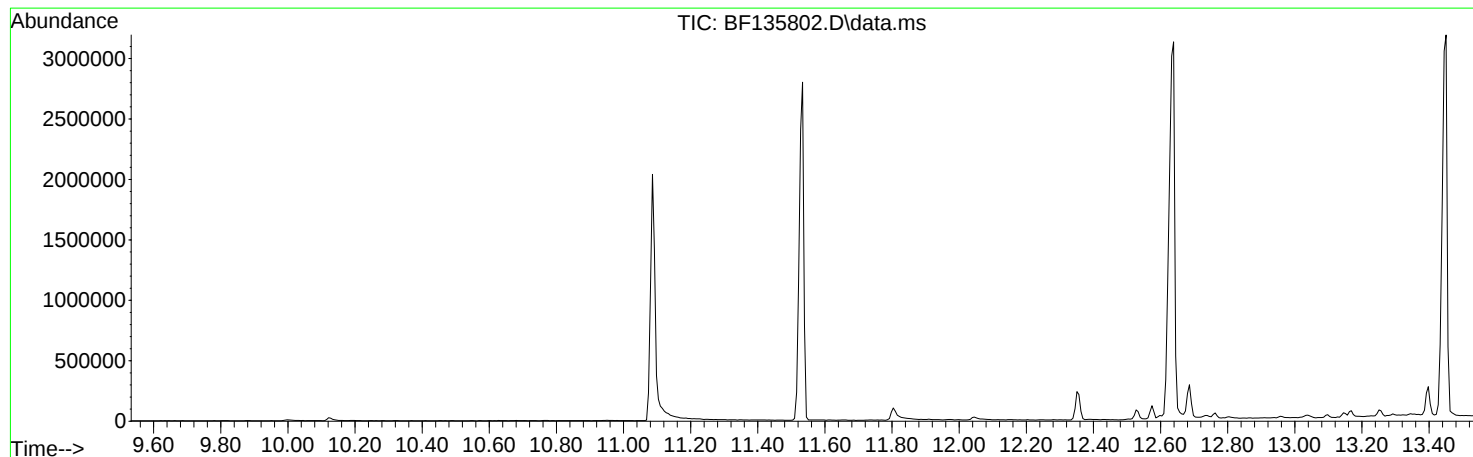




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	92908	PASS
68	69	0.00	2	1.6	1189	PASS
69	198	0.00	100	35.6	73551	PASS
70	69	0.00	2	0.5	392	PASS
127	198	10	80	46.2	95379	PASS
197	198	0.00	2	0.5	1070	PASS
198	198	100	100	100.0	206496	PASS
199	198	5	9	6.7	13800	PASS
275	198	10	60	29.6	61136	PASS
365	198	1	100	3.9	7986	PASS
441	198	0.01	100	23.2	47939	PASS
442	442	50	100	100.0	303787	PASS
443	442	15	24	19.2	58192	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
 Data File : BF135802.D
 Acq On : 17 Oct 2023 09:54
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 17 11:35:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 17 01:22:00 2023
 Response via : Initial Calibration

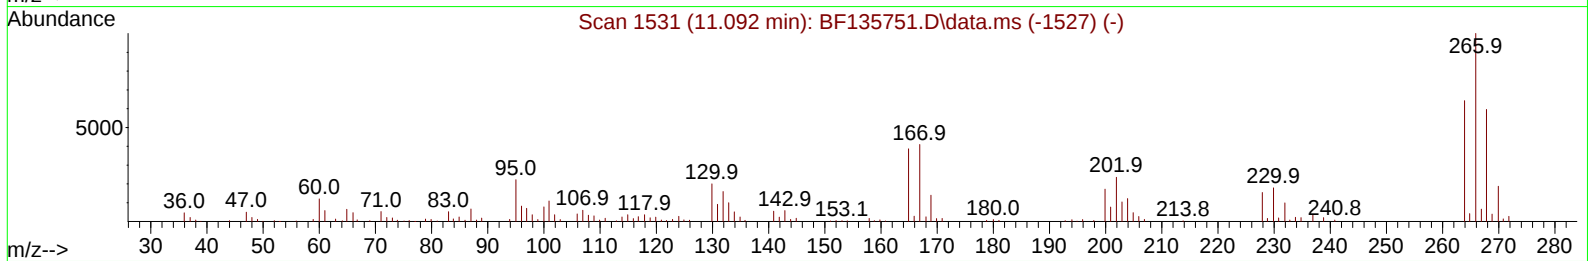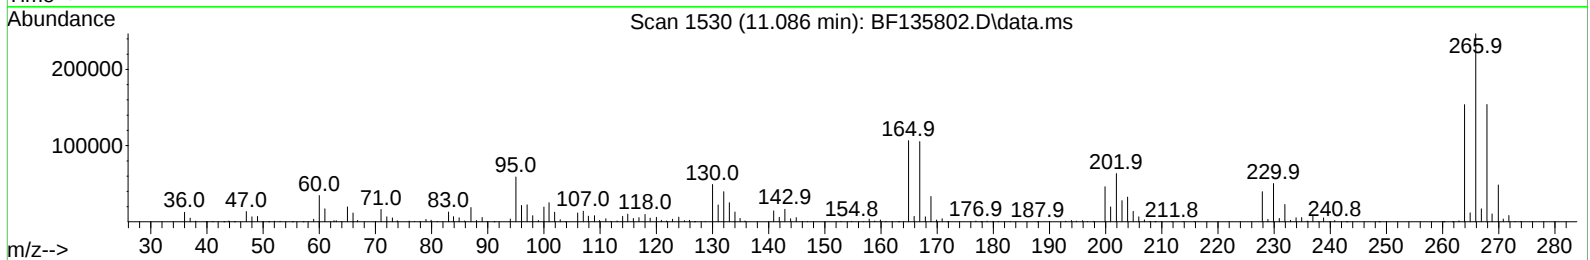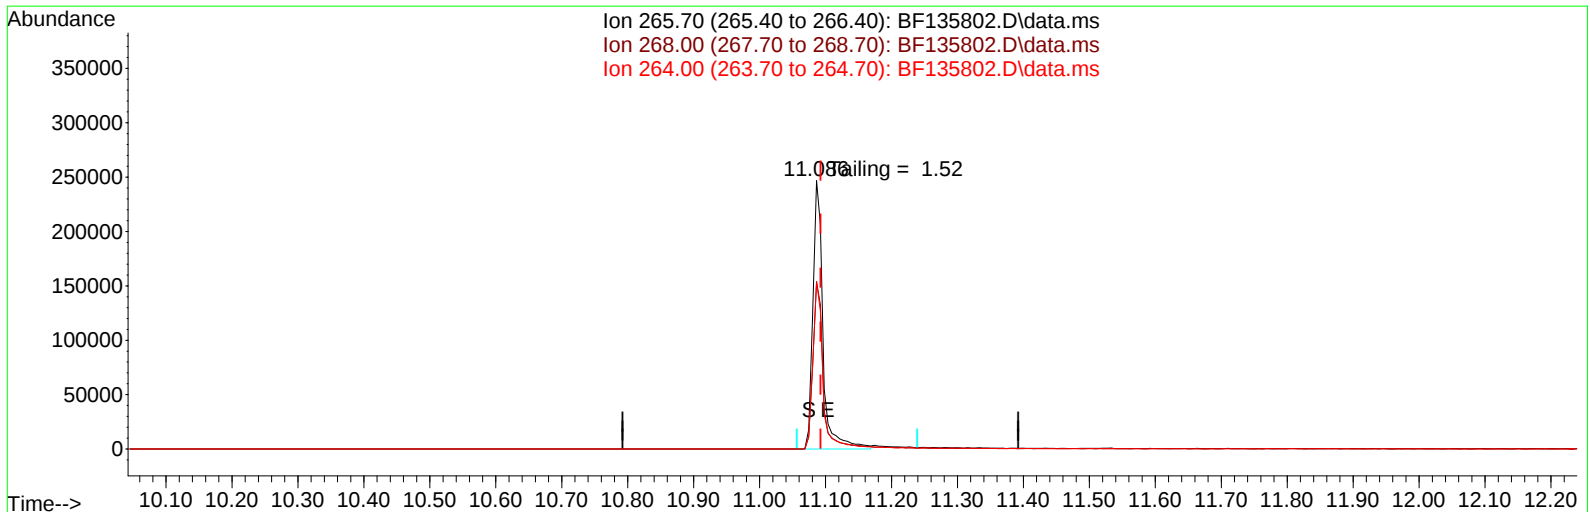

TIC: BF135802.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 325830.29 ng




response 271868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	62.40
264.00	64.30	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101723\
Data File : BF135802.D
Acq On : 17 Oct 2023 09:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 11:35:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

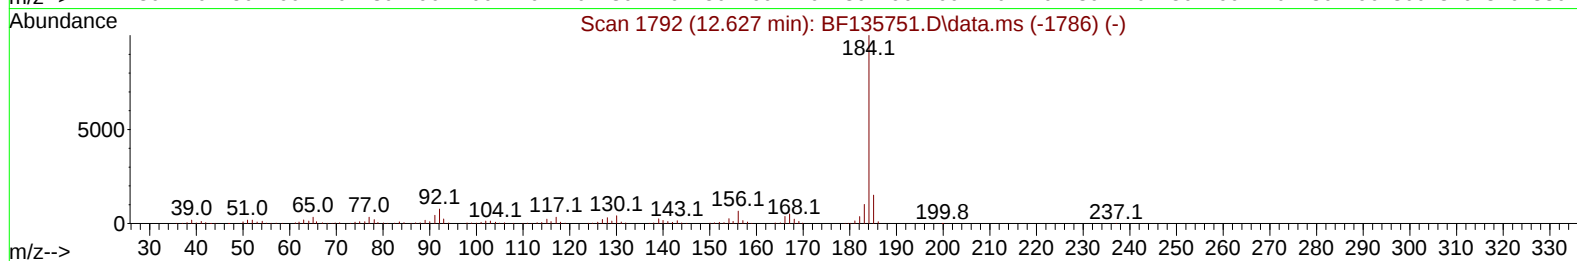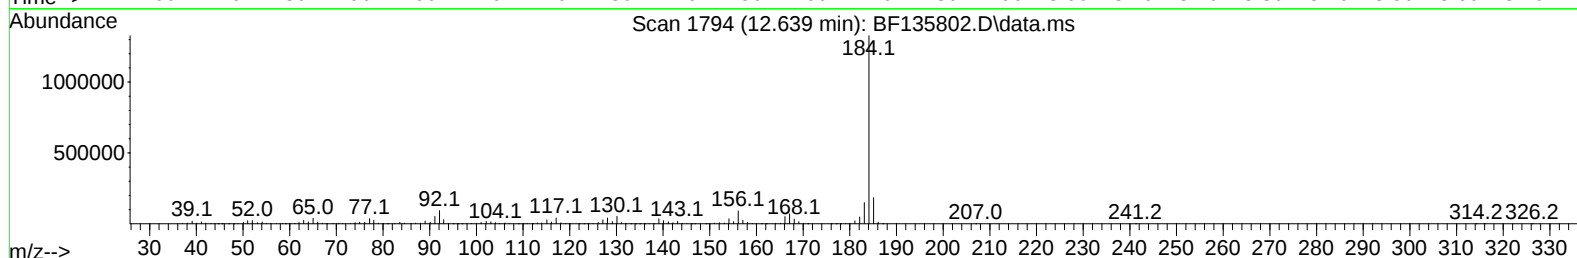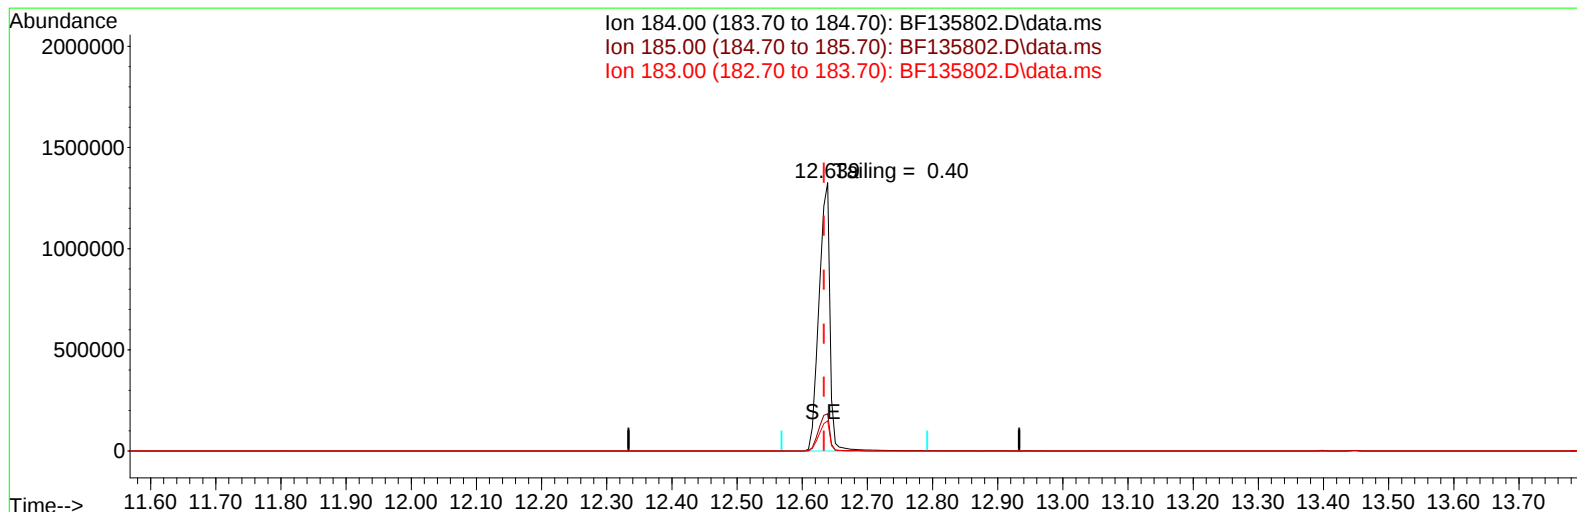

TIC: BF135802.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 261078.01 ng

response 1543877

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.90
183.00	10.20	11.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/17/2023	BNA_F	<u>BF135802.D</u>
Compound Name	Response	Retention Time
DDT	651286	13.451
DDD	16524	13.168
DDE	1376	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17900	669186	2.67

Instrument :
BNA_F
ClientSampleId :
DFTPP