
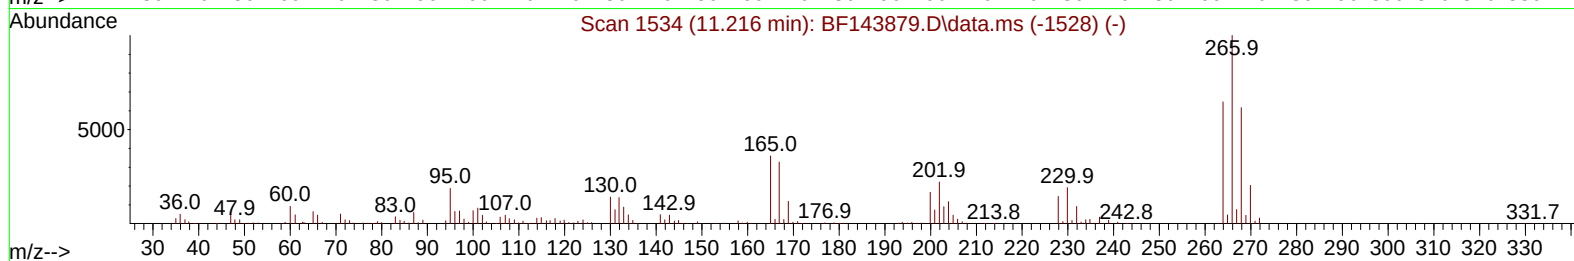
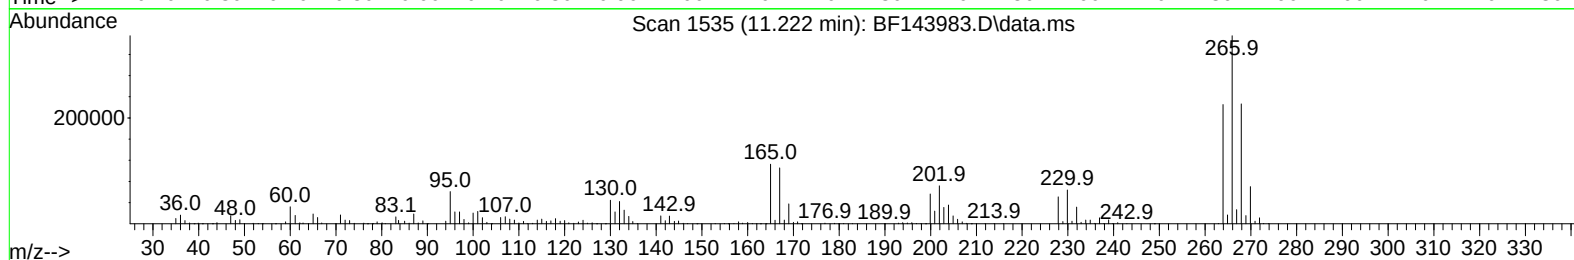


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101725\
Data File : BF143983.D
Acq On : 17 Oct 2025 14:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 15:40:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

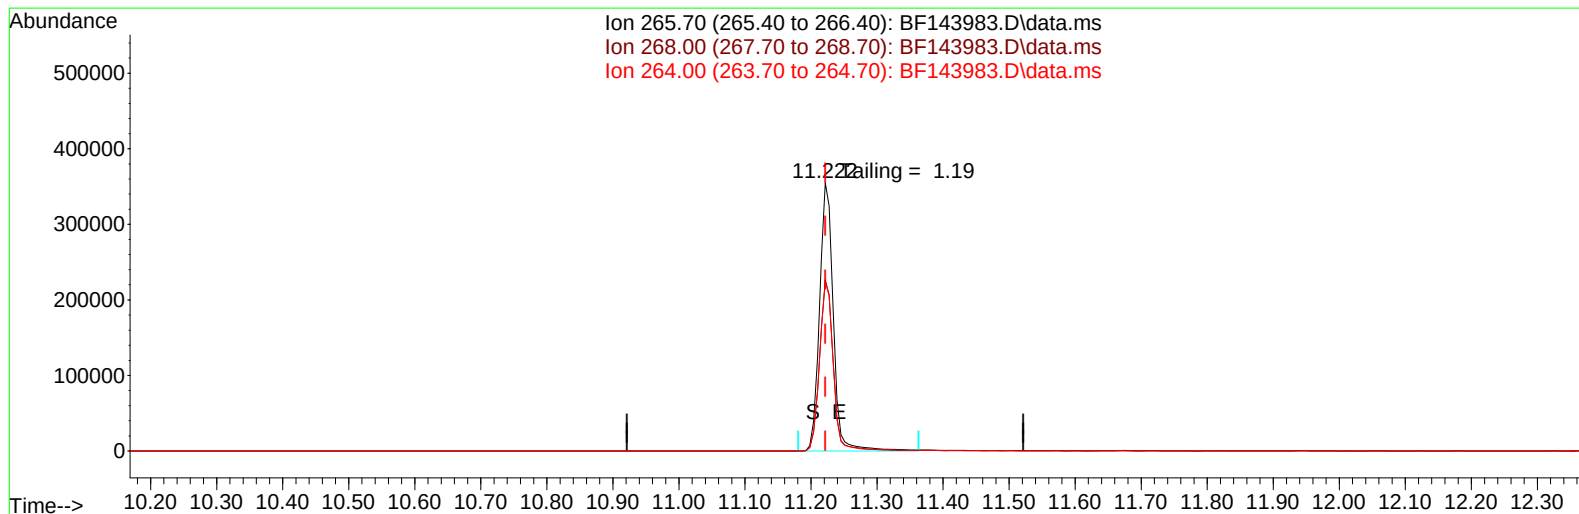

TIC: BF143983.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.000) 1324535.20 ng

response 515849

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.73
264.00	64.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101725\
Data File : BF143983.D
Acq On : 17 Oct 2025 14:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 15:40:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

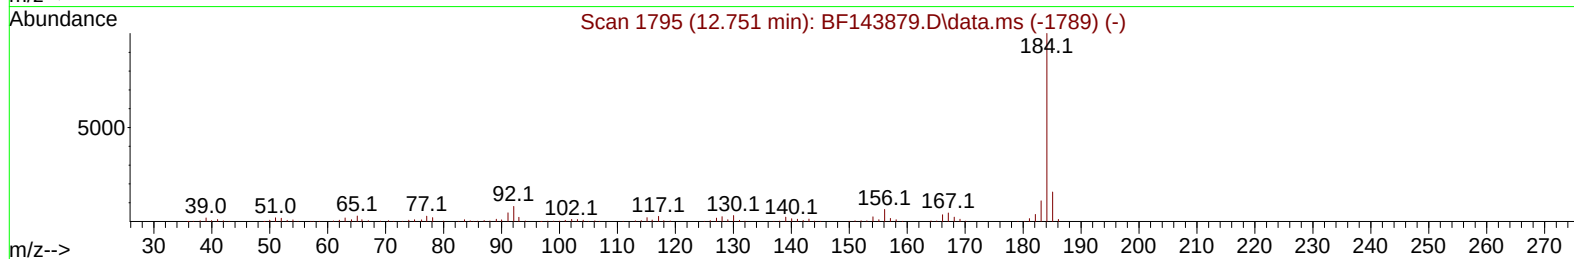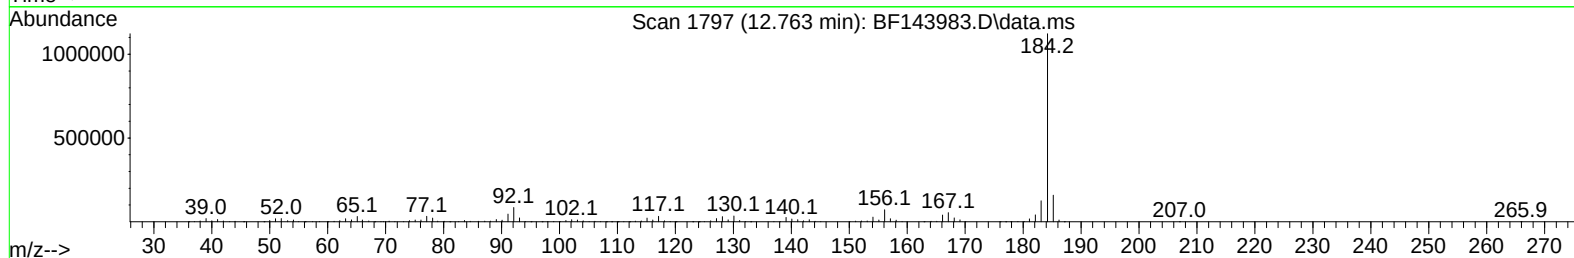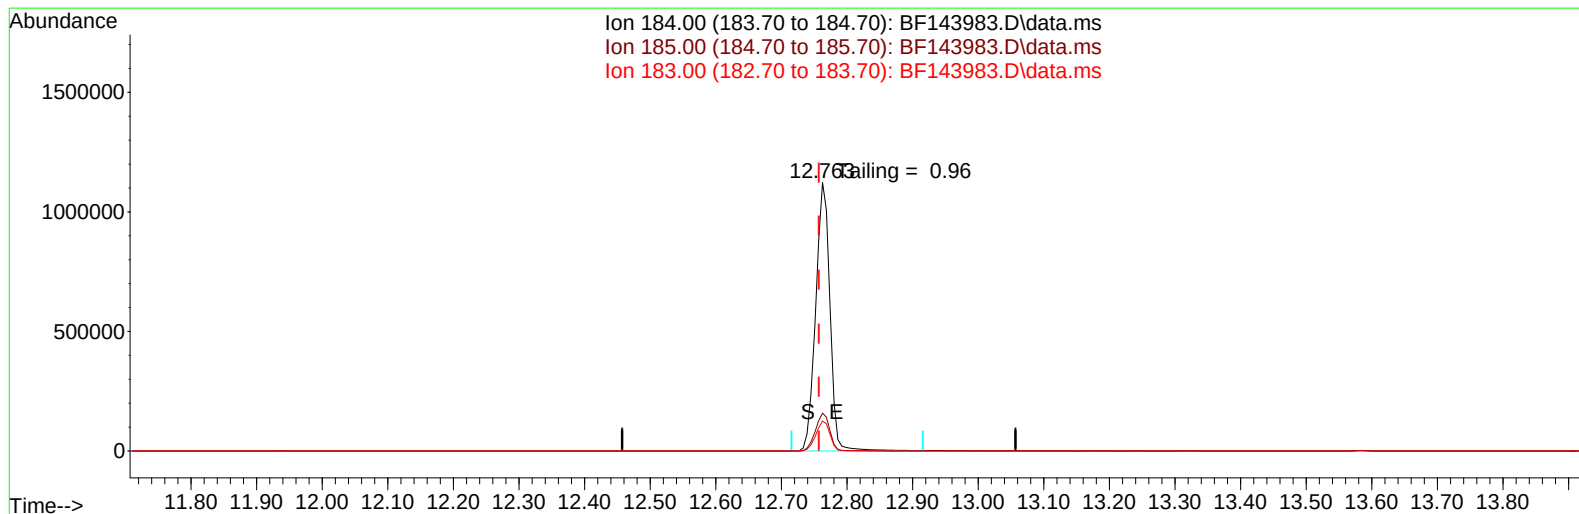

TIC: BF143983.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 1703588

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.18
183.00	11.00	11.18
0.00	0.00	0.00