
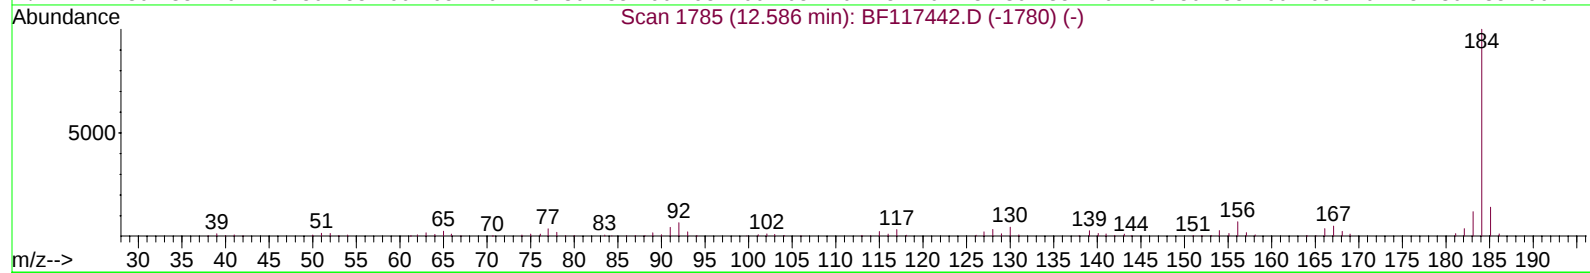
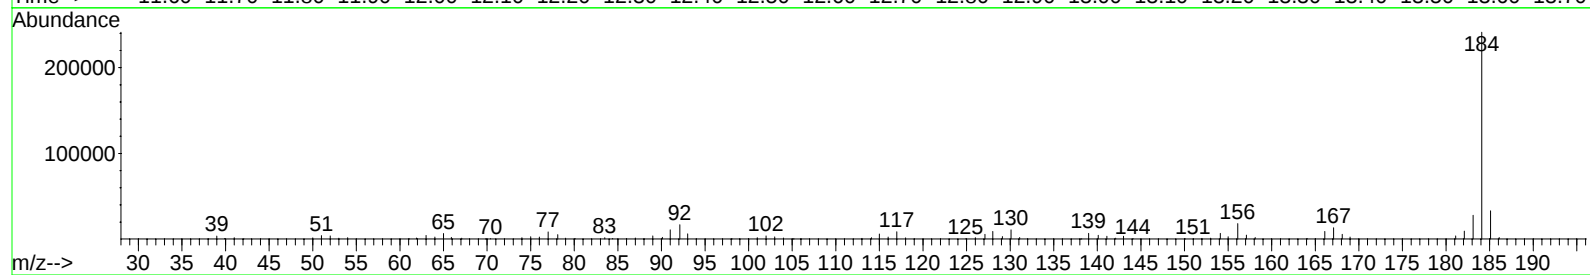


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101819\  
Data File   : BF117439.D  
Acq On      : 18 Oct 2019   14:46  
Operator    : JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Oct 21 18:32:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

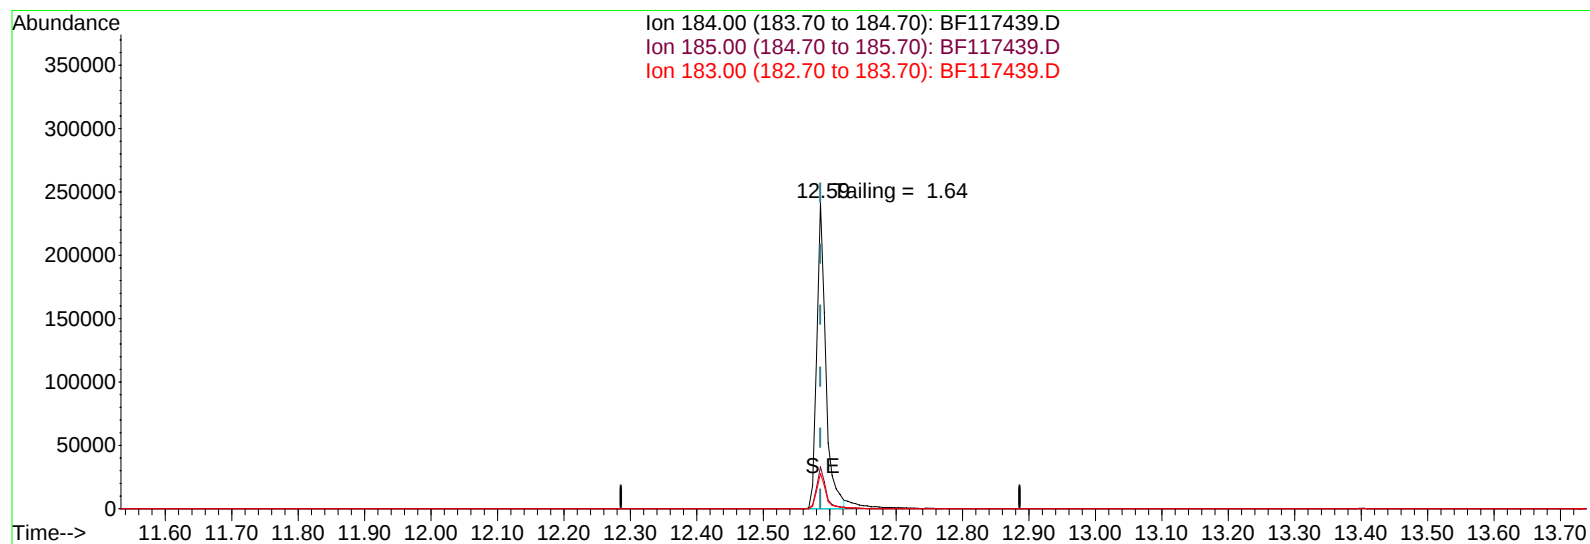

TIC: BF117439.D

(77) Benzidine




12.586min (+0.000) 0.00ng

response 240032

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.72
183.00	12.00	11.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101819\
Data File : BF117439.D
Acq On : 18 Oct 2019 14:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 18:32:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

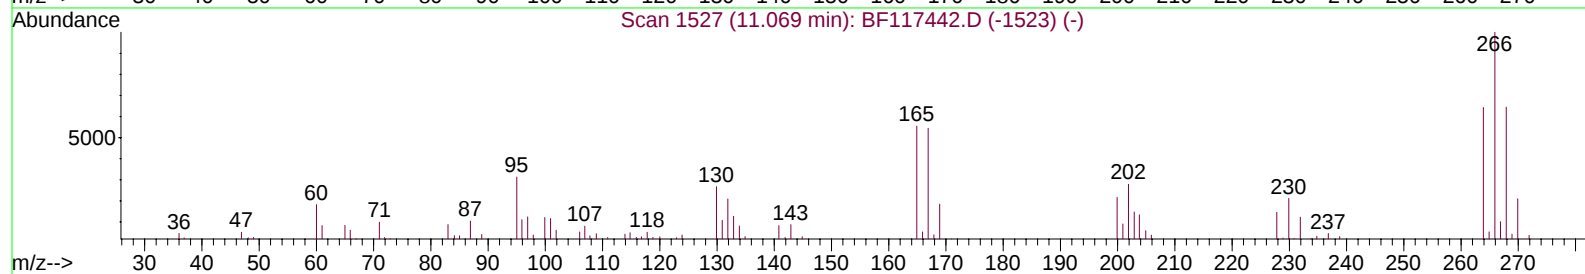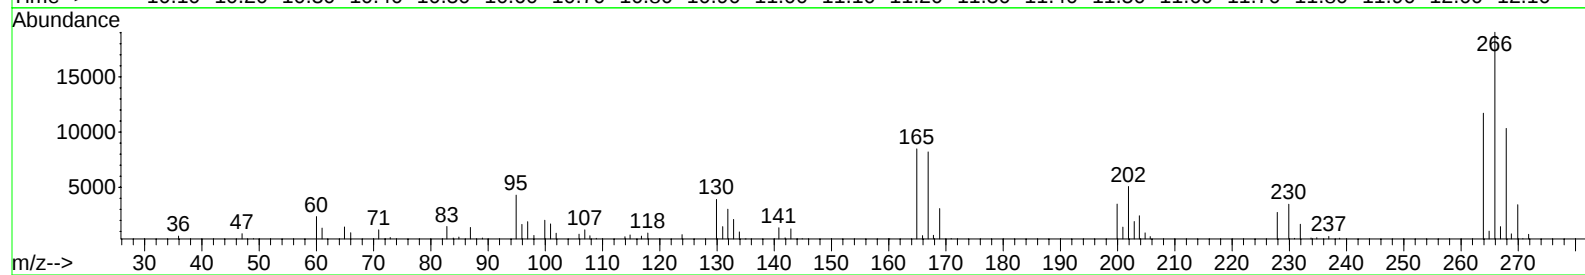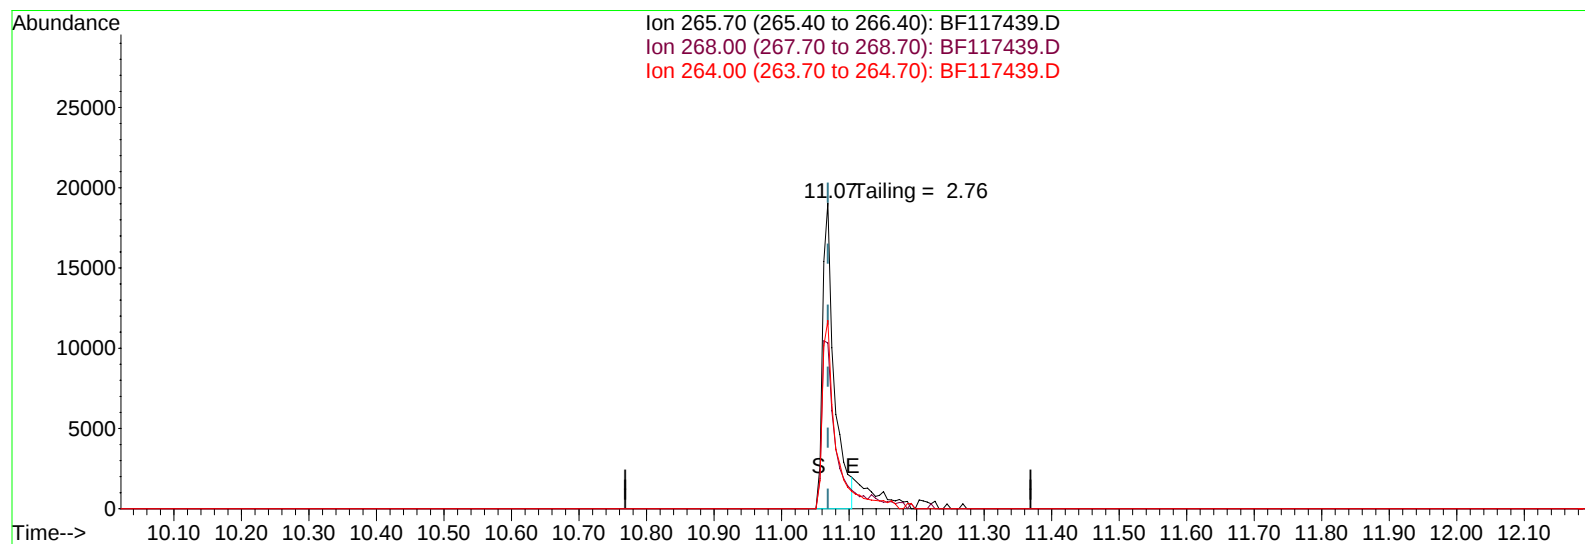

TIC: BF117439.D

(70) Pentachlorophenol (C)

11.068min (-0.000) 0.00ng

response 27250

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	54.23
264.00	64.30	61.52
0.00	0.00	0.00