


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101819\
 Data File : BF117439.D
 Acq On : 18 Oct 2019 14:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

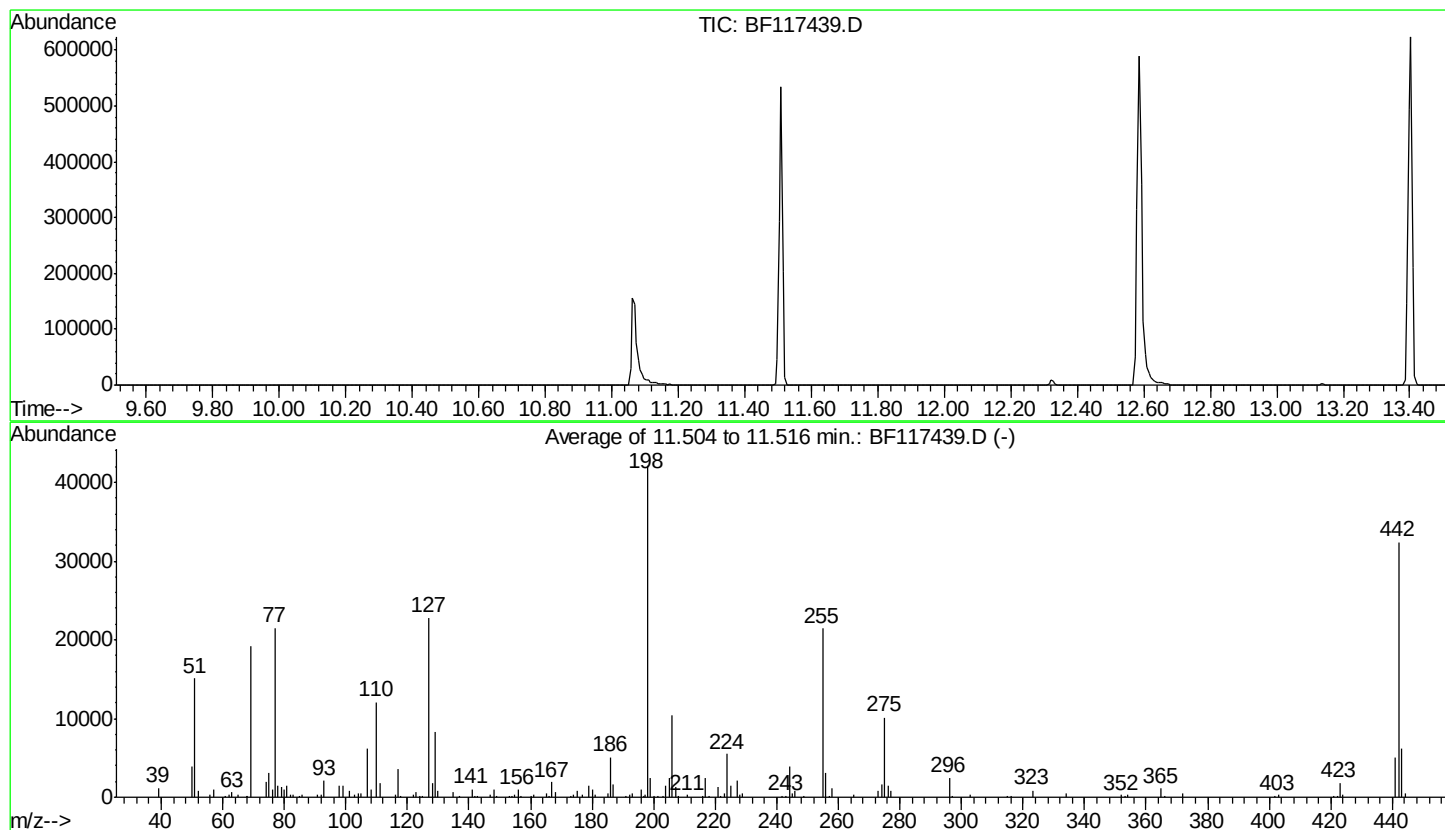

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	15056	PASS
68	69	0.00	2	1.2	234	PASS
69	198	0.00	100	45.4	19148	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	22790	PASS
197	198	0.00	2	0.7	283	PASS
198	198	100	100	100.0	42130	PASS
199	198	5	9	5.8	2426	PASS
275	198	10	60	24.1	10155	PASS
365	198	1	100	2.7	1120	PASS
441	198	0.01	100	12.0	5049	PASS
442	198	50	100	76.8	32367	PASS
443	442	15	24	18.9	6117	PASS