
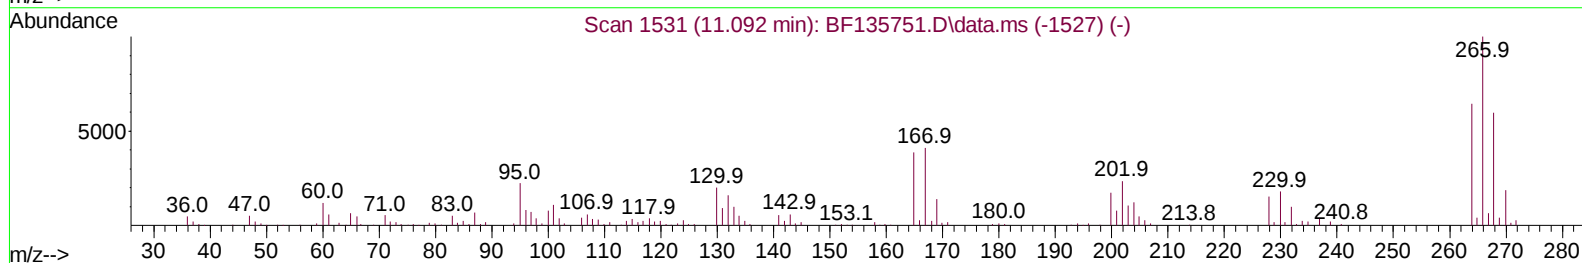
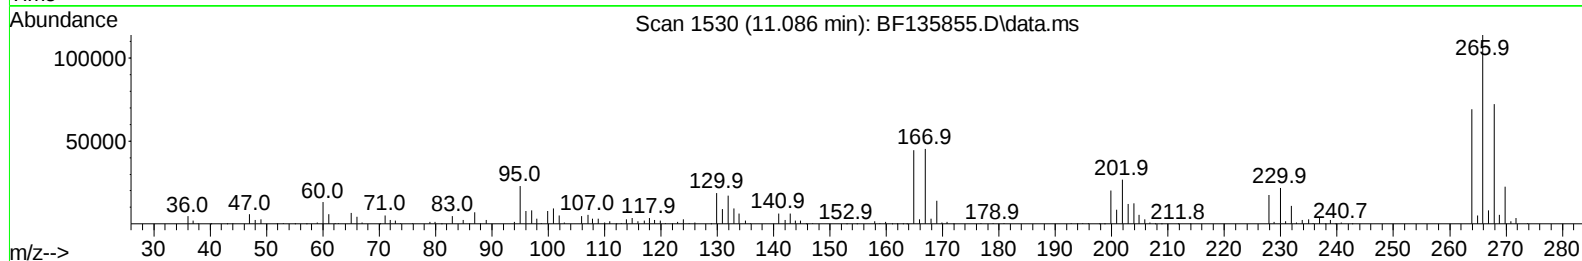


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101823\  
Data File : BF135855.D  
Acq On : 18 Oct 2023 19:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 01:49:10 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 17 01:22:00 2023  
Response via : Initial Calibration

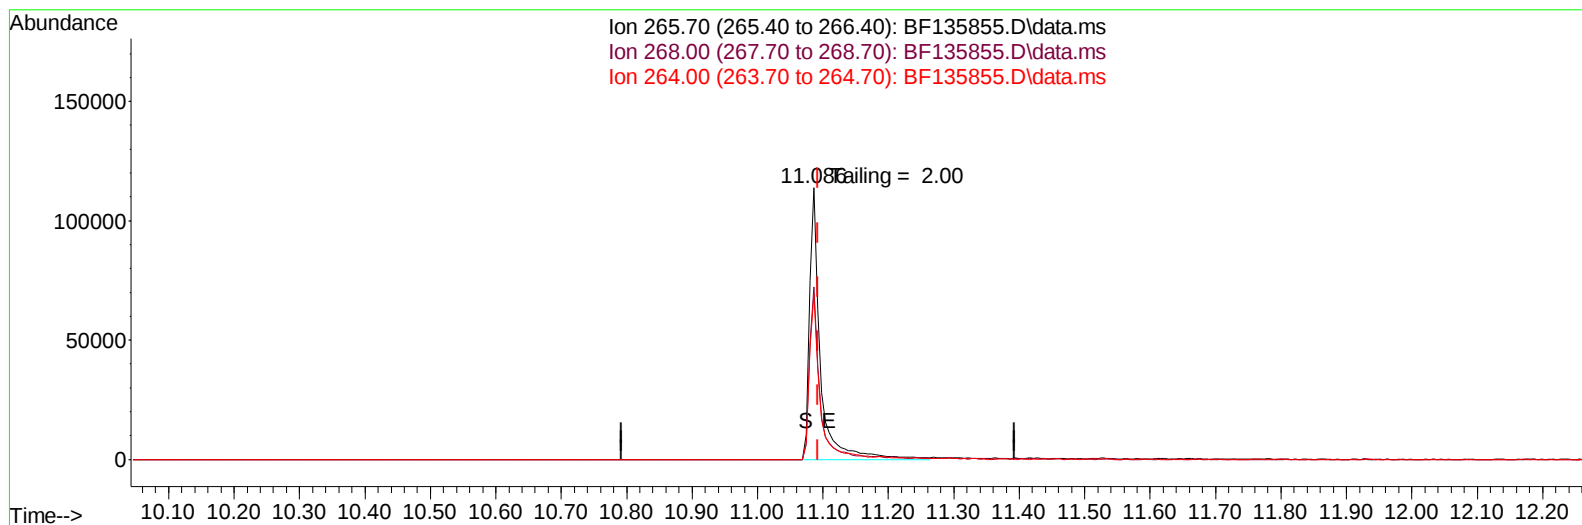

TIC: BF135855.D\data.ms

**(70) Pentachlorophenol (C)**




**11.086min (-0.006) 602810.41 ng**

**response 133641**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.60  | 63.54  |
| 264.00 | 64.30  | 60.64  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101823\  
Data File : BF135855.D  
Acq On : 18 Oct 2023 19:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 01:49:10 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 17 01:22:00 2023  
Response via : Initial Calibration

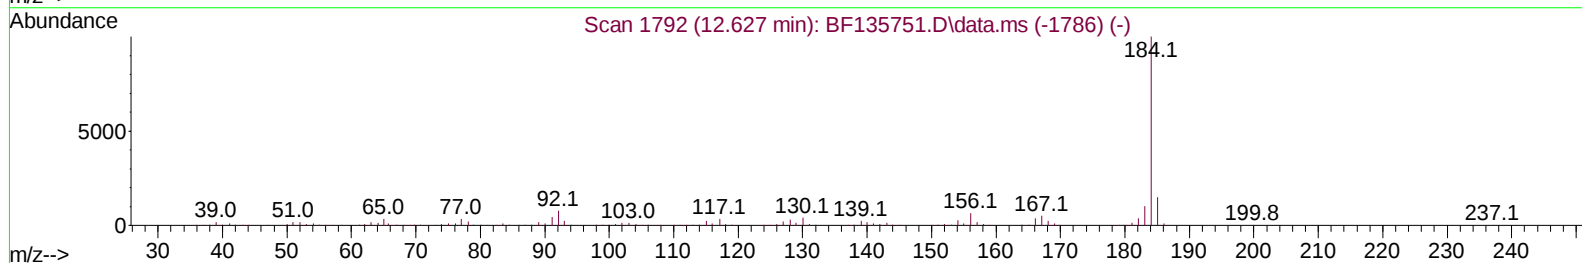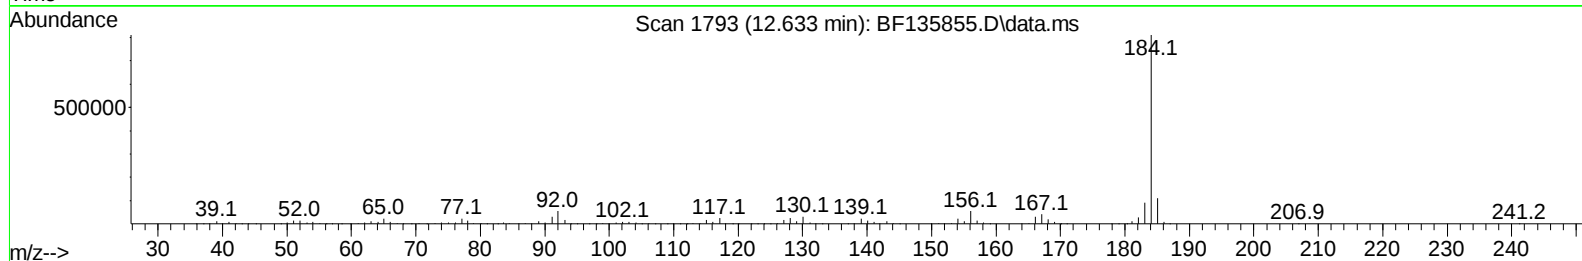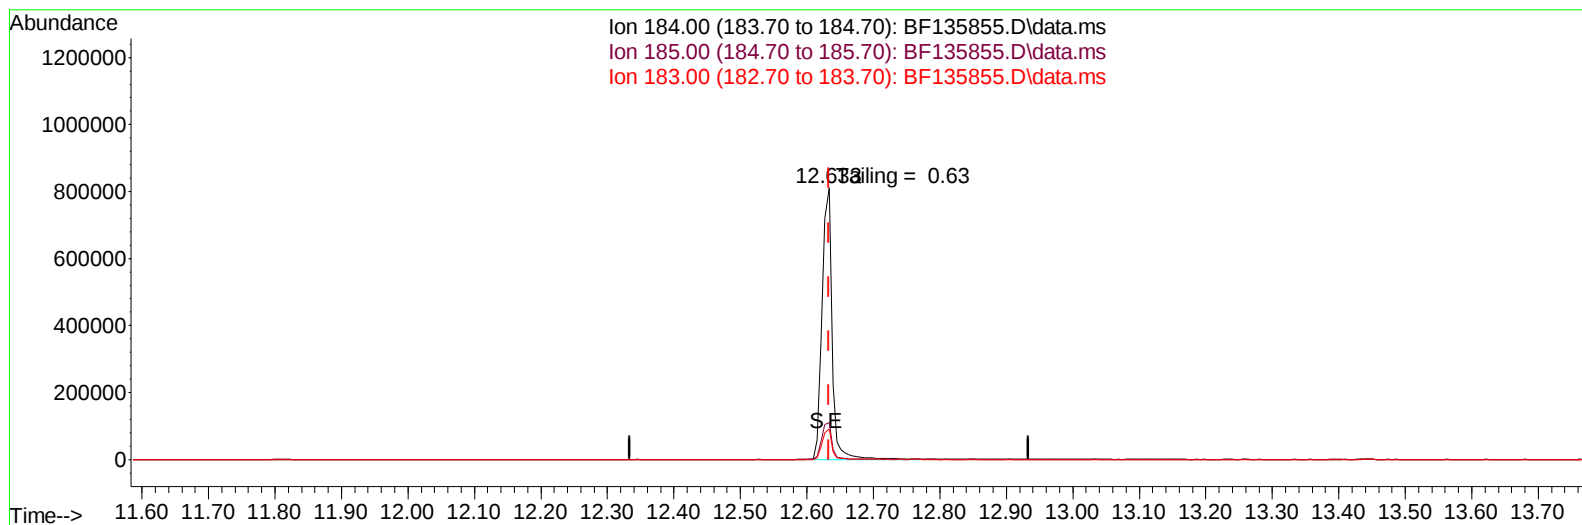

TIC: BF135855.D\data.ms

**(77) Benzidine****12.633min (-0.000) 480437.16 ng****response 828203**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 13.65  |
| 183.00 | 10.20  | 11.20  |
| 0.00   | 0.00   | 0.00   |