
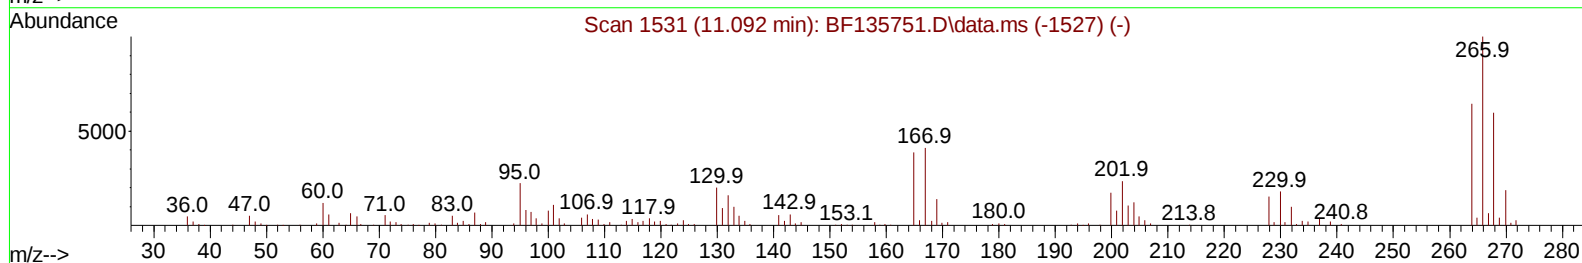
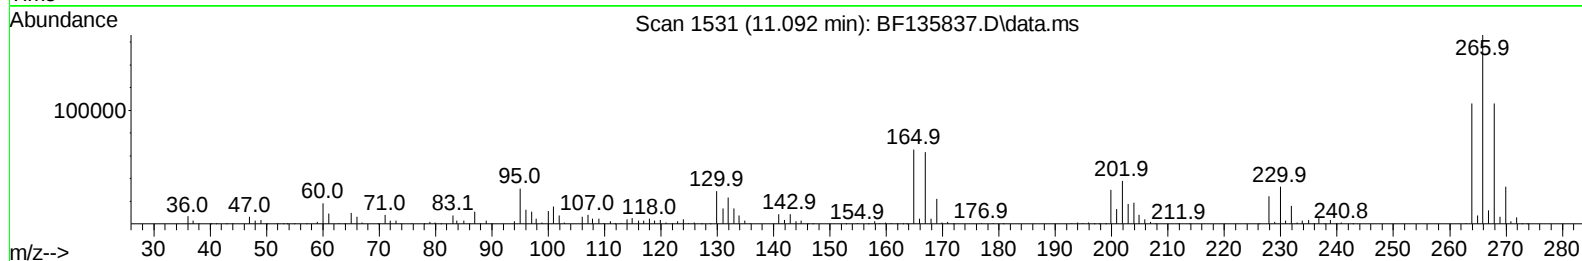


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135837.D
Acq On : 18 Oct 2023 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 19:57:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

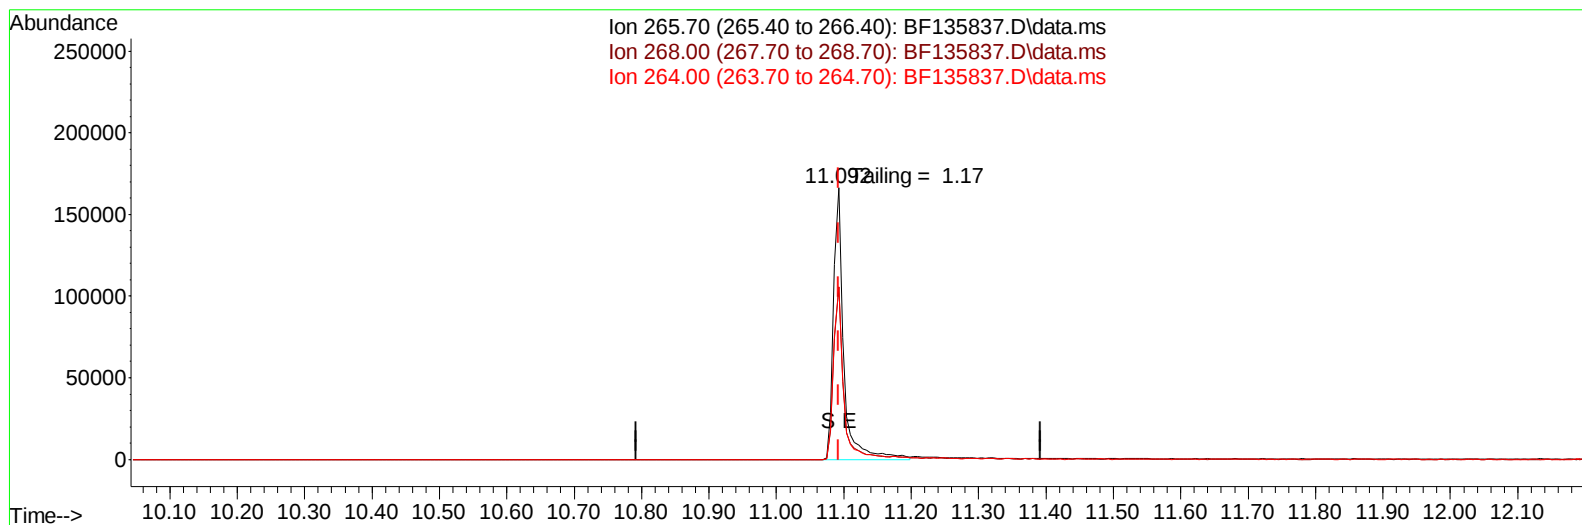

TIC: BF135837.D\data.ms

(70) Pentachlorophenol (C)




11.092min (-0.000) 376475.00 ng

response 174514

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.61
264.00	64.30	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135837.D
Acq On : 18 Oct 2023 09:57
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 19:57:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

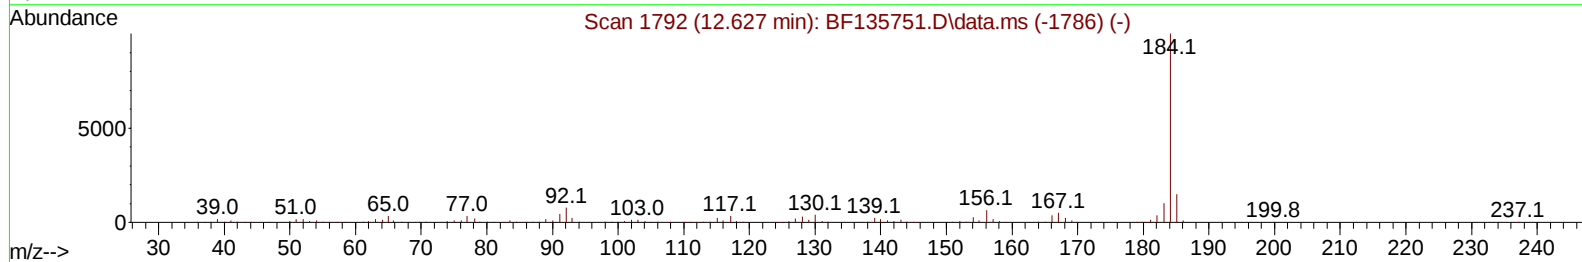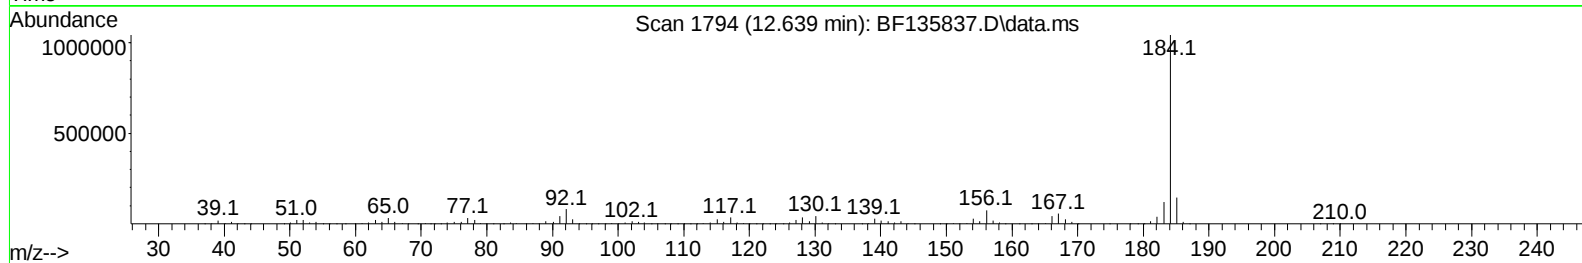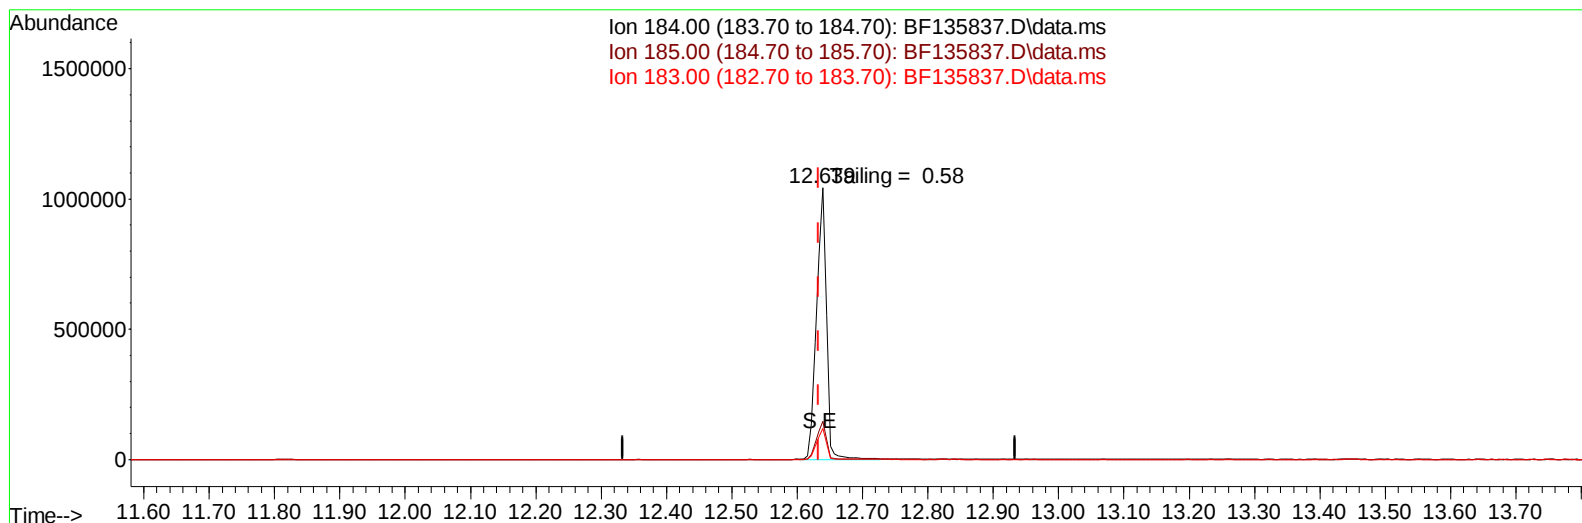

TIC: BF135837.D\data.ms

(77) Benzidine**12.639min (+ 0.006) 117941.08 ng****response 1111788**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.00
183.00	10.20	11.45
0.00	0.00	0.00