

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
 Data File : BF135850.D
 Acq On : 18 Oct 2023 16:38
 Operator : CG\JU
 Sample : 04767-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	485	488	504	rBV	89762	127449	4.99%	0.942%
2	5.381	557	560	593	rBV	594028	938184	36.75%	6.937%
3	6.398	730	733	759	rBV	345171	558212	21.87%	4.127%
4	6.739	788	791	799	rBV	531592	488460	19.14%	3.612%
5	7.310	884	888	909	rBV	1344356	1424461	55.80%	10.533%
6	8.016	1005	1008	1031	rBV	712120	650458	25.48%	4.810%
7	8.245	1044	1047	1049	rBV	26842	29630	1.16%	0.219%
8	8.269	1049	1051	1067	rVB	35040	62650	2.45%	0.463%
9	9.098	1188	1192	1195	rBV	2660573	2423582	94.94%	17.920%
10	9.775	1303	1307	1320	rBV	891420	754441	29.55%	5.578%
11	10.574	1439	1443	1459	rBV	1808789	1702394	66.69%	12.588%
12	11.274	1558	1562	1571	rBV	848784	812905	31.85%	6.011%
13	12.516	1768	1773	1786	rBV4	24405	54027	2.12%	0.399%
14	12.868	1829	1833	1836	rBV	2708072	2552682	100.00%	18.875%
15	13.939	2011	2015	2025	rVB	465360	469729	18.40%	3.473%
16	15.415	2261	2266	2279	rBV	301690	475018	18.61%	3.512%




Sum of corrected areas: 13524282

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135850.D
Acq On : 18 Oct 2023 16:38
Operator : CG\JU
Sample : 04767-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

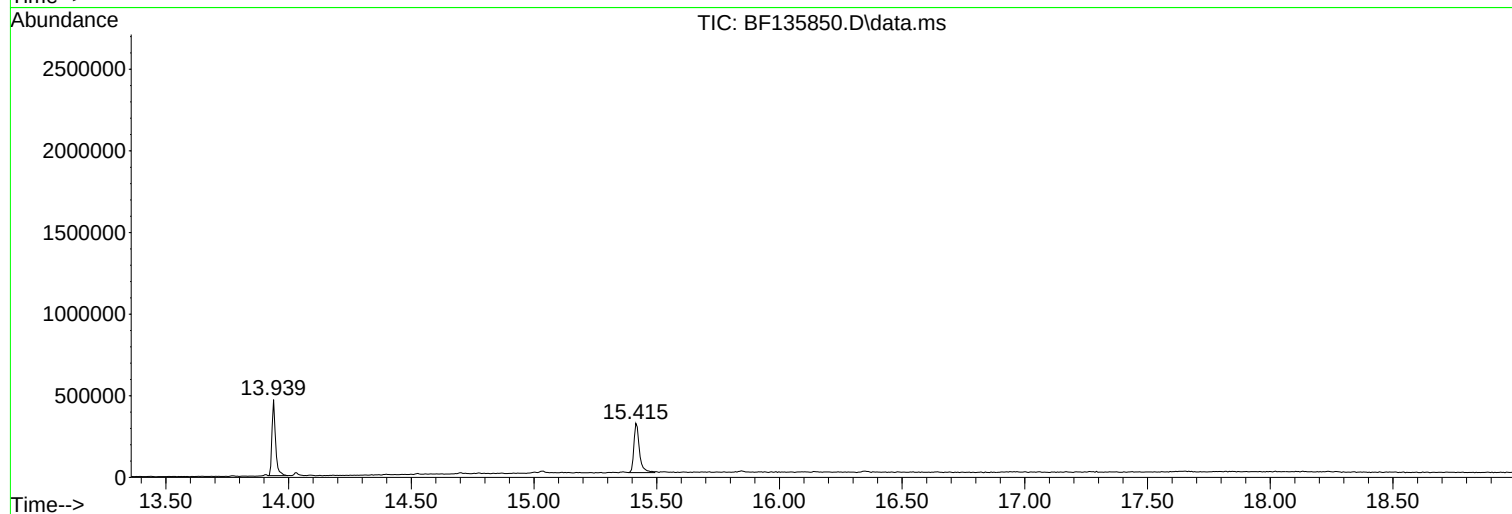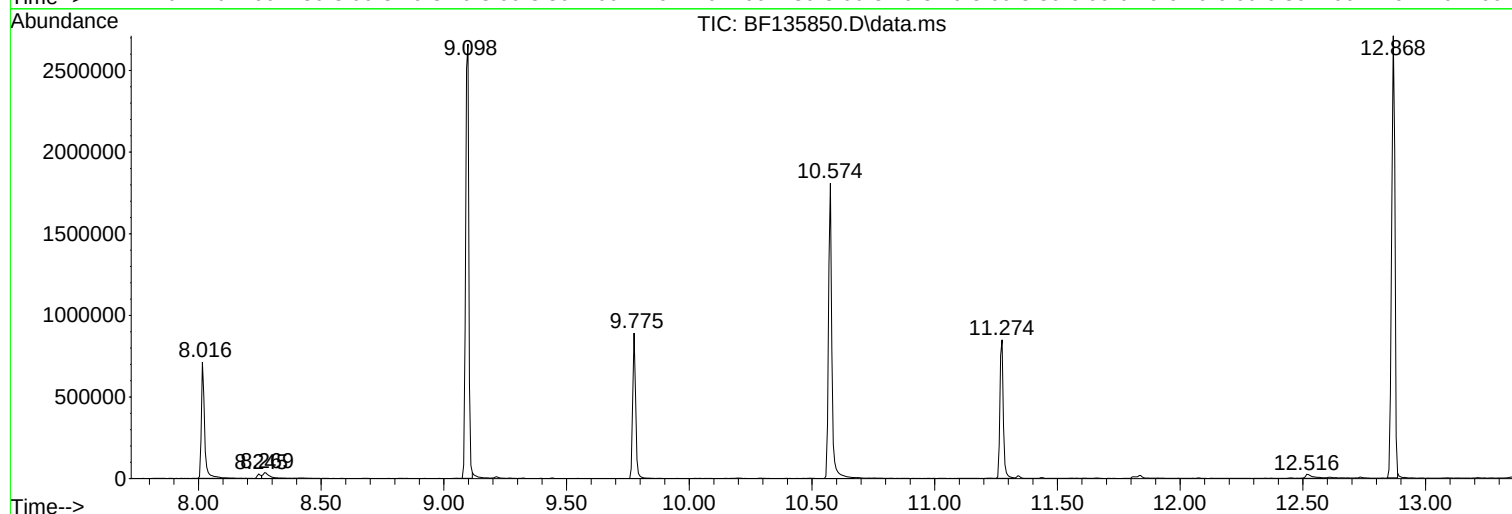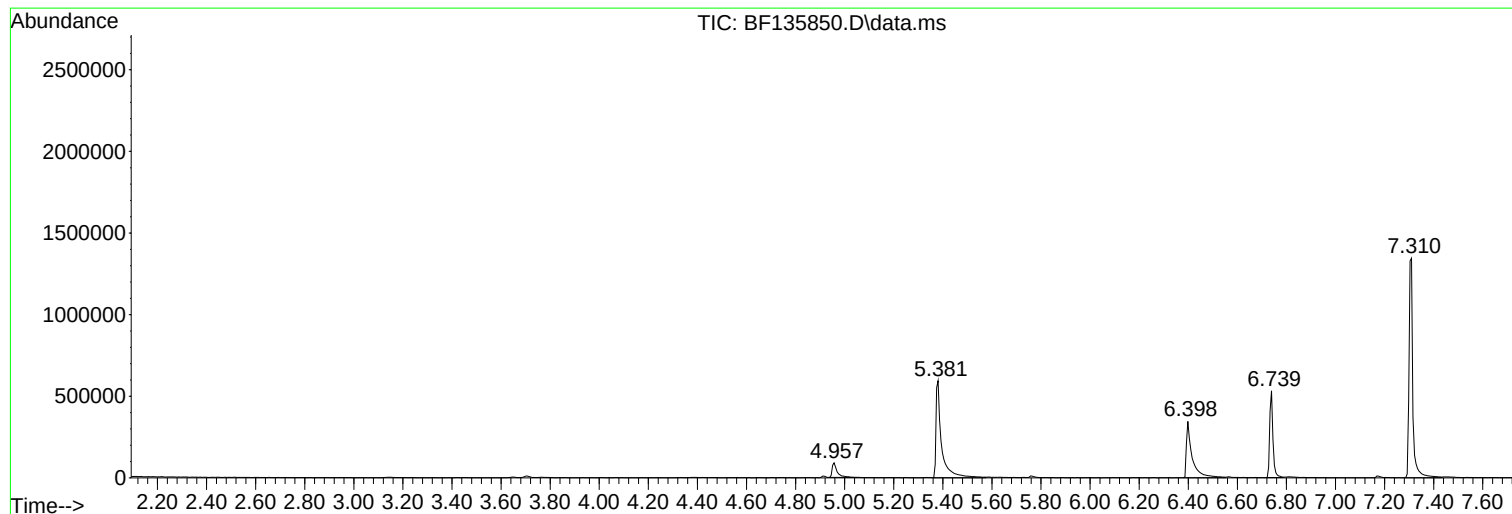

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135850.D
Acq On : 18 Oct 2023 16:38
Operator : CG\JU
Sample : 04767-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.957	5.22 ng	127449	1,4-Dichlorobenzene-d4	6.739

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	3-Hexanol	102	C6H14O	000623-37-0	33		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		

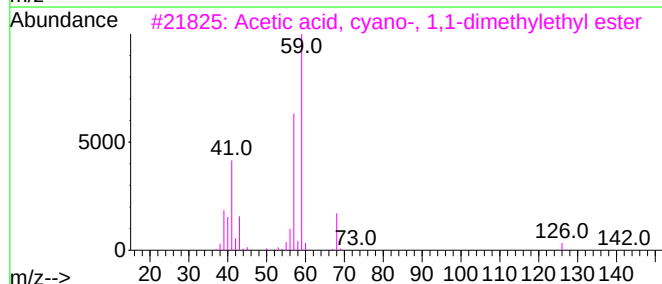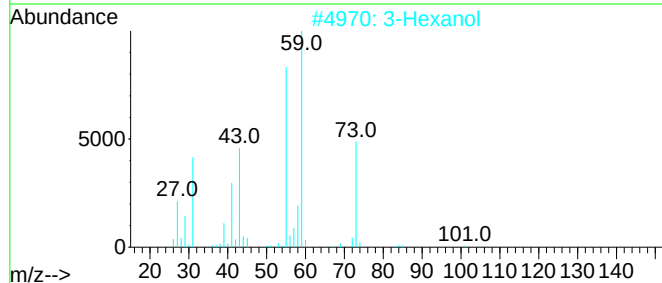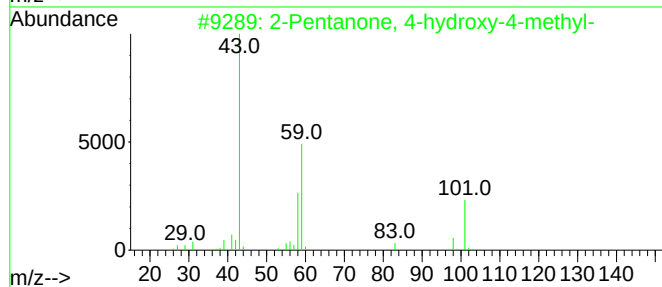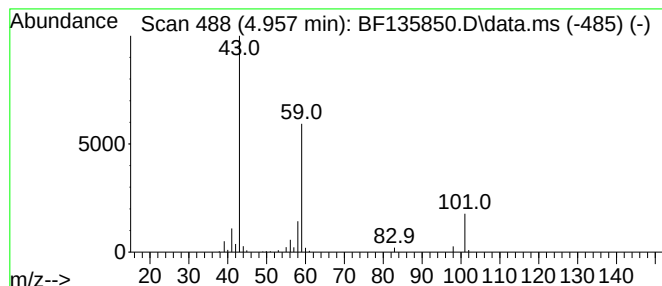

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135850.D
Acq On : 18 Oct 2023 16:38
Operator : CG\JU
Sample : 04767-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.957	5.2	ng	127449	1	6.739	488460	20.0