

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
 Data File : BF135852.D
 Acq On : 18 Oct 2023 17:40
 Operator : CG\JU
 Sample : 04793-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-303-20231005

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	485	488	504	rBV	79110	115382	4.24%	0.842%
2	5.375	556	559	582	rBV	750254	1076524	39.52%	7.853%
3	6.392	730	732	755	rBV	381809	650640	23.89%	4.746%
4	6.740	787	791	800	rBV	480848	478091	17.55%	3.488%
5	7.310	884	888	902	rBV	1760421	1648170	60.51%	12.023%
6	8.016	1005	1008	1029	rBV	693175	637897	23.42%	4.653%
7	9.098	1188	1192	1195	rBV	3061116	2723694	100.00%	19.869%
8	9.775	1303	1307	1318	rBV	814265	686529	25.21%	5.008%
9	10.575	1439	1443	1458	rBV	1580799	1565623	57.48%	11.421%
10	11.269	1558	1561	1581	rBV	750732	730156	26.81%	5.326%
11	12.869	1828	1833	1836	rBV	2714613	2543821	93.40%	18.557%
12	13.939	2011	2015	2027	rVB	434302	450824	16.55%	3.289%
13	15.415	2261	2266	2278	rBV	261180	400776	14.71%	2.924%




Sum of corrected areas: 13708127

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135852.D
Acq On : 18 Oct 2023 17:40
Operator : CG\JU
Sample : 04793-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

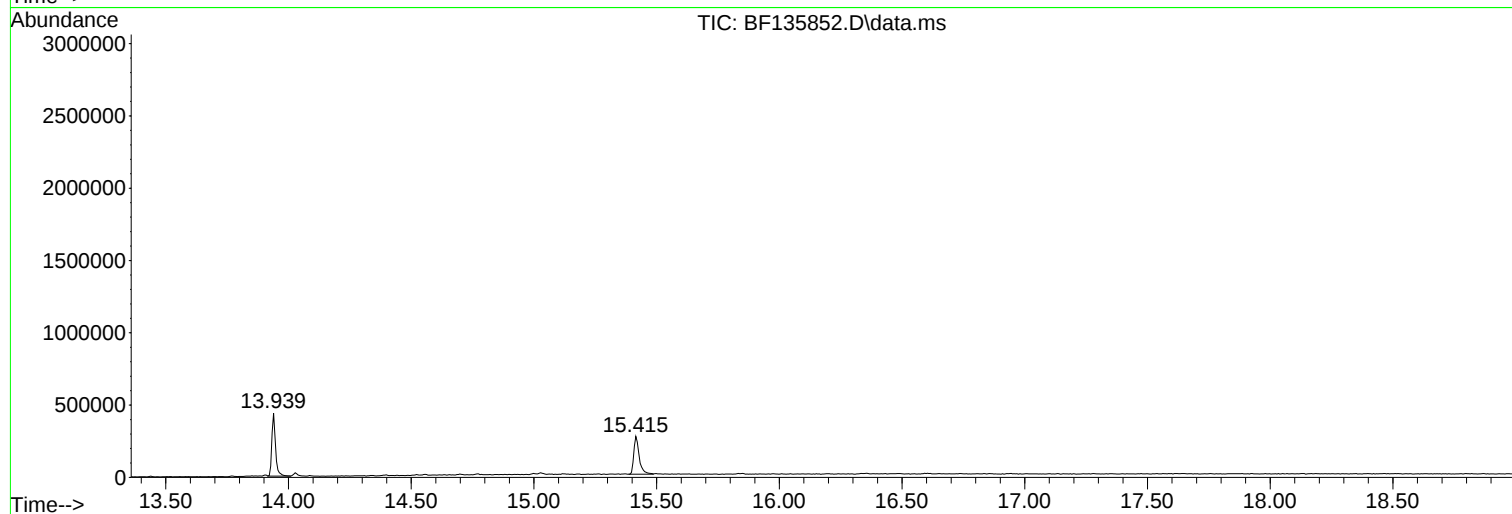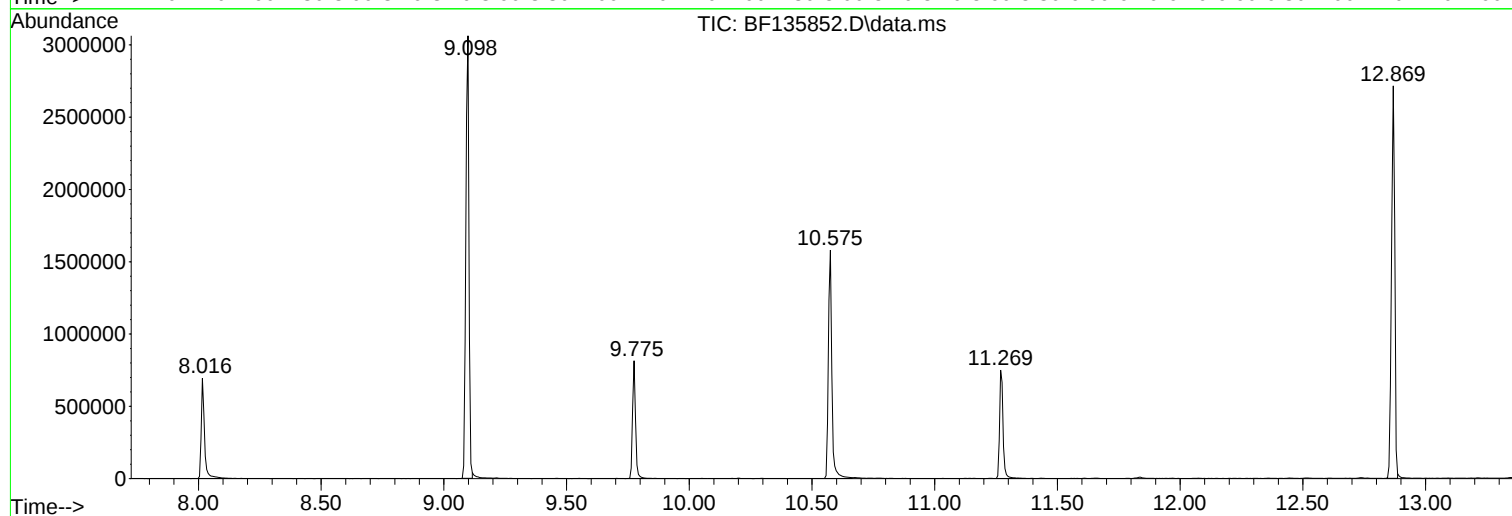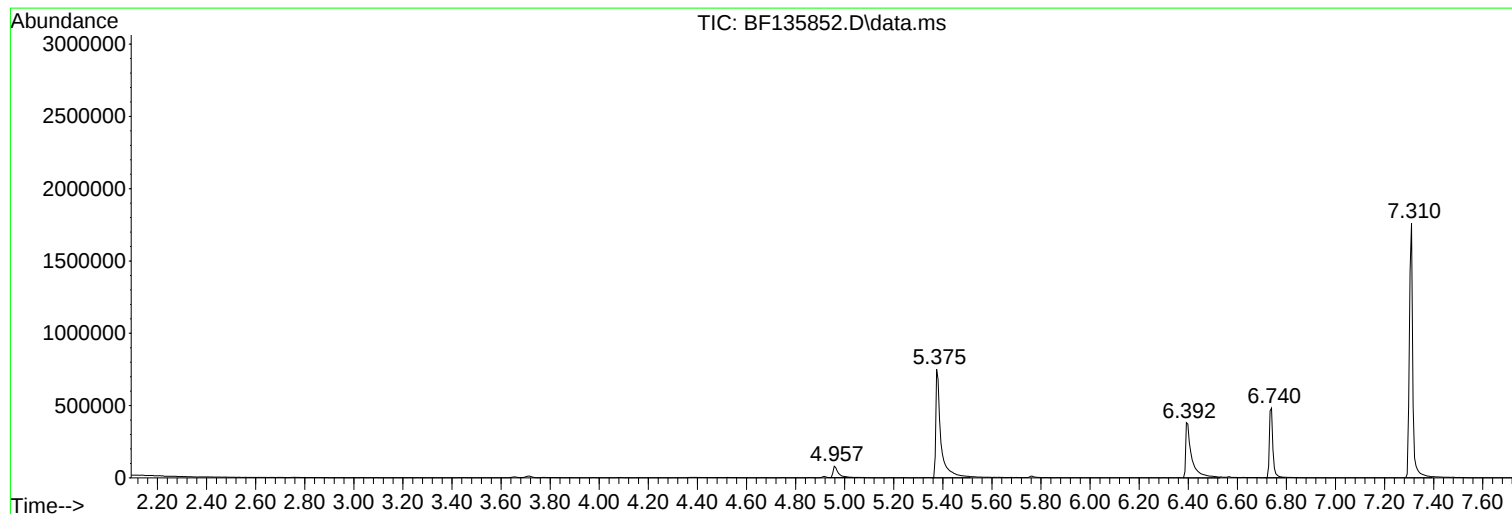

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135852.D
Acq On : 18 Oct 2023 17:40
Operator : CG\JU
Sample : 04793-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231005










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.957	4.83 ng	115382	1,4-Dichlorobenzene-d4	6.739

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33		
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	23		

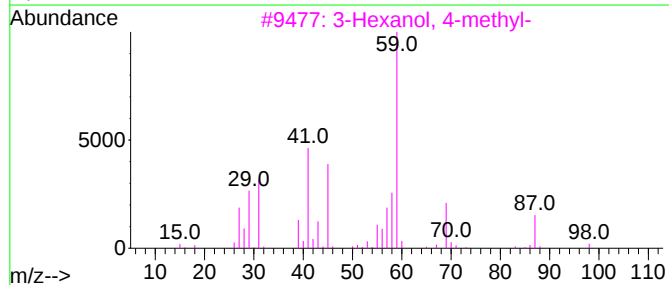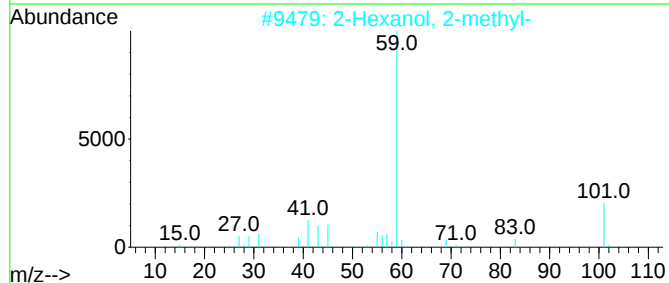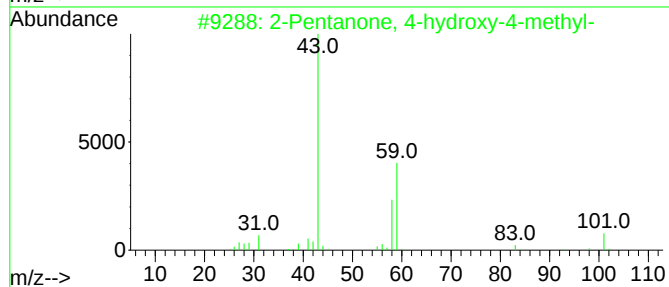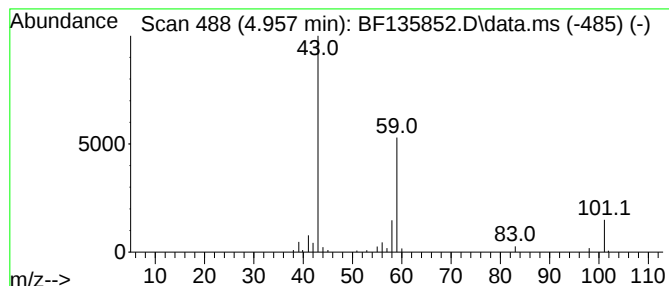

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135852.D
Acq On : 18 Oct 2023 17:40
Operator : CG\JU
Sample : 04793-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.957	4.8	ng	115382	1	6.739	478091	20.0